
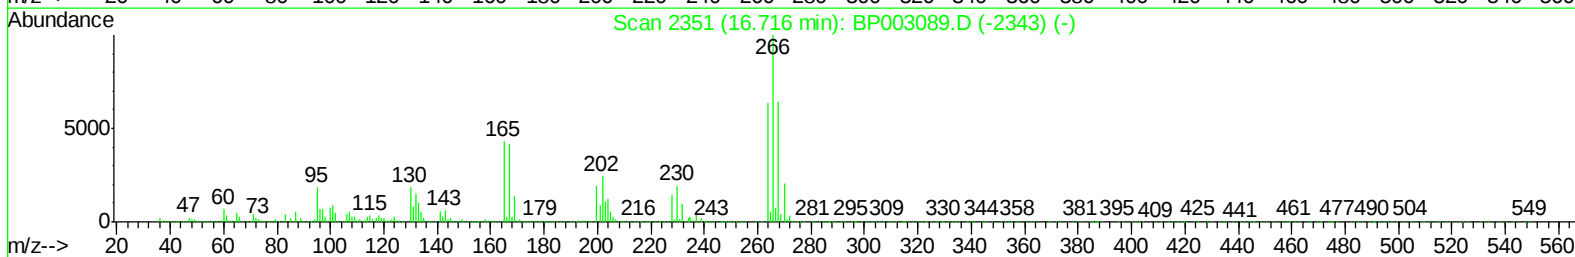
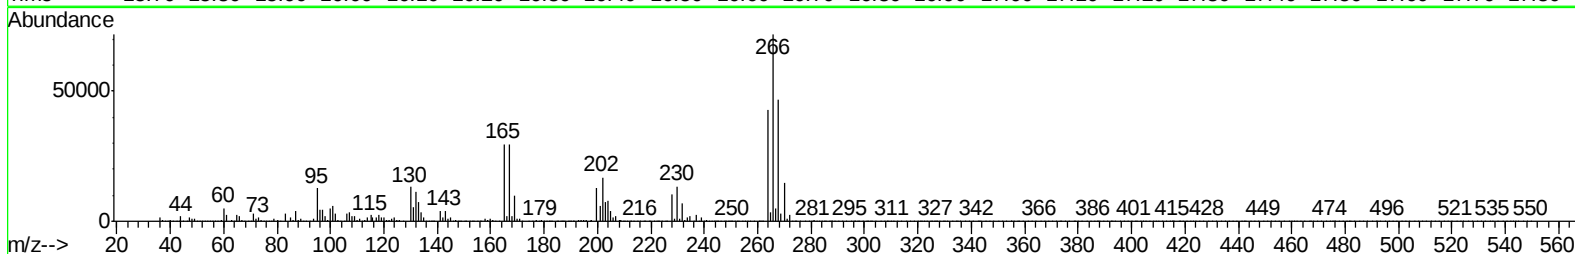


Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP090420\
 Data File : BP003201.D
 Acq On : 04 Sep 2020 09:05
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 05 08:55:01 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP082420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 01 14:37:05 2020
 Response via : Initial Calibration

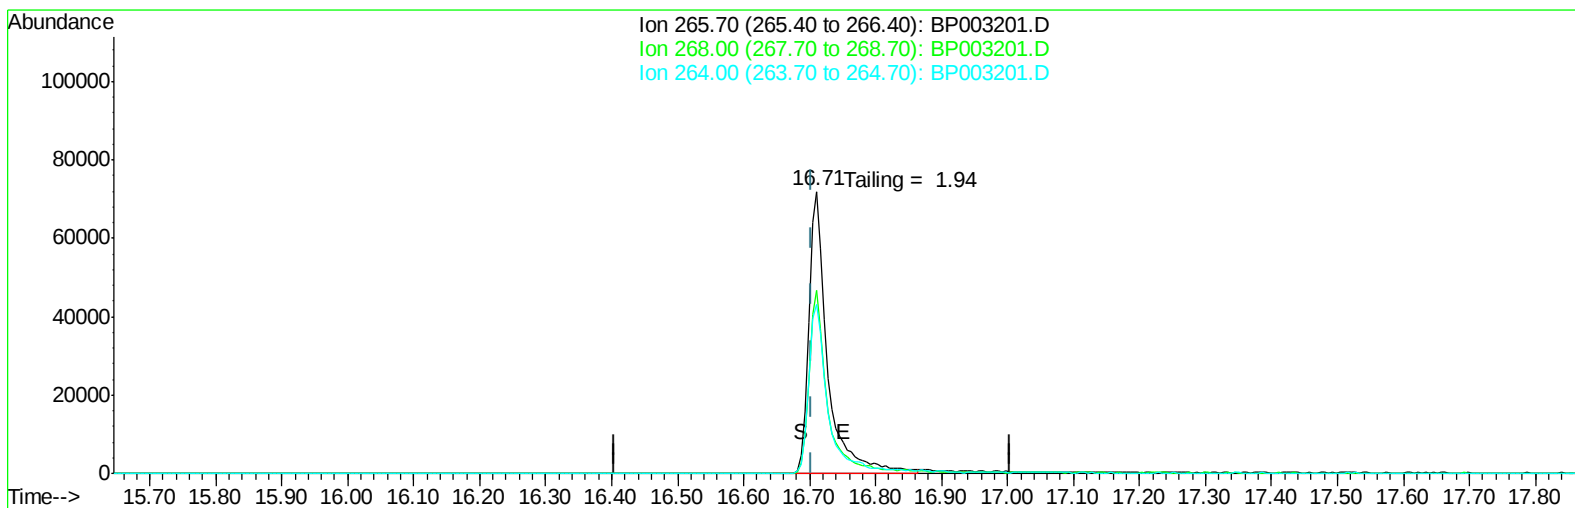

TIC: BP003201.D

(70) Pentachlorophenol (C)




16.710min (+0.006) 2288027.28ng

response 143765

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	65.01
264.00	63.30	59.92
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP090420\
 Data File : BP003201.D
 Acq On : 04 Sep 2020 09:05
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 05 08:55:01 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP082420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 01 14:37:05 2020
 Response via : Initial Calibration

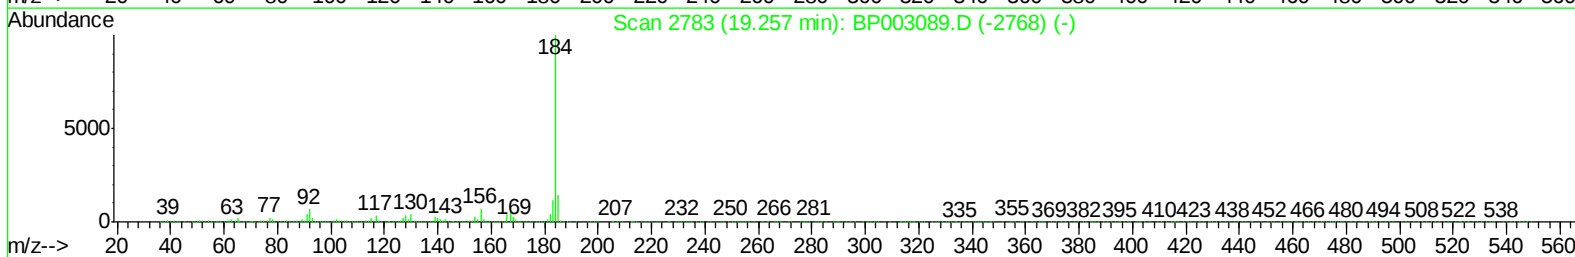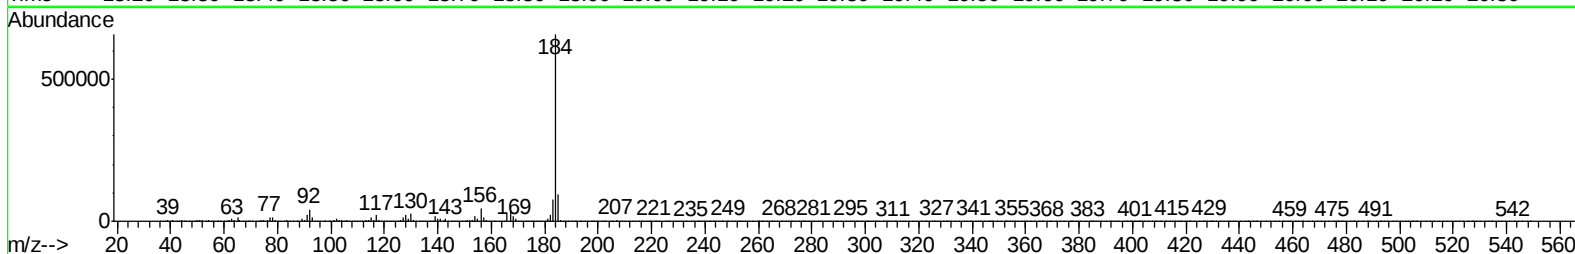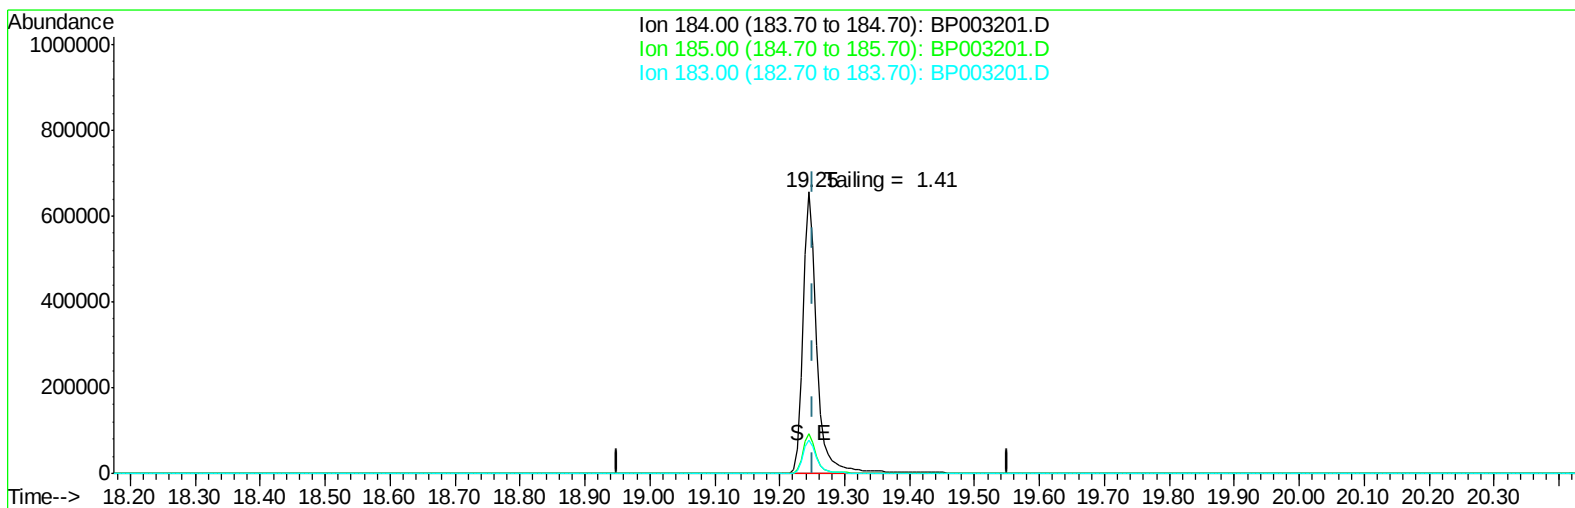

TIC: BP003201.D

(77) Benzidine

19.245min (-0.006) 31586.13ng

response 963014

Ion	Exp%	Act%
184.00	100	100
185.00	14.40	14.14
183.00	12.00	11.92
0.00	0.00	0.00