

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP090420\
 Data File : BP003203.D
 Acq On : 04 Sep 2020 10:13
 Operator : CG/JU
 Sample : PB131395BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB131395BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP082420.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.964	9	13	18	rVB	96410	95933	1.00%	0.197%
2	4.799	320	325	334	rVB	87049	115920	1.21%	0.238%
3	5.264	397	404	420	rBV	3278173	4804972	50.28%	9.868%
4	6.840	664	672	694	rBV	2765928	4574773	47.87%	9.395%
5	7.646	802	809	824	rBV	840160	1330814	13.93%	2.733%
6	8.799	996	1005	1027	rBV	1969847	3368606	35.25%	6.918%
7	10.428	1272	1282	1301	rBV	1012472	1797039	18.80%	3.691%
8	12.910	1696	1704	1720	rBV	5615650	8557192	89.54%	17.574%
9	14.292	1931	1939	1958	rBV2	1431633	2226343	23.30%	4.572%
10	15.787	2185	2193	2219	rBV	3491825	5287672	55.33%	10.860%
11	17.045	2400	2407	2420	rBV	1536248	2329835	24.38%	4.785%
12	19.622	2839	2845	2863	rBV	7675141	9556775	100.00%	19.627%
13	21.139	3097	3103	3114	rBV	1731776	2301071	24.08%	4.726%
14	23.368	3475	3482	3491	rBV2	1223478	2344653	24.53%	4.815%


Sum of corrected areas: 48691598

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP090420\
Data File : BP003203.D
Acq On : 04 Sep 2020 10:13
Operator : CG/JU
Sample : PB131395BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB131395BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP082420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

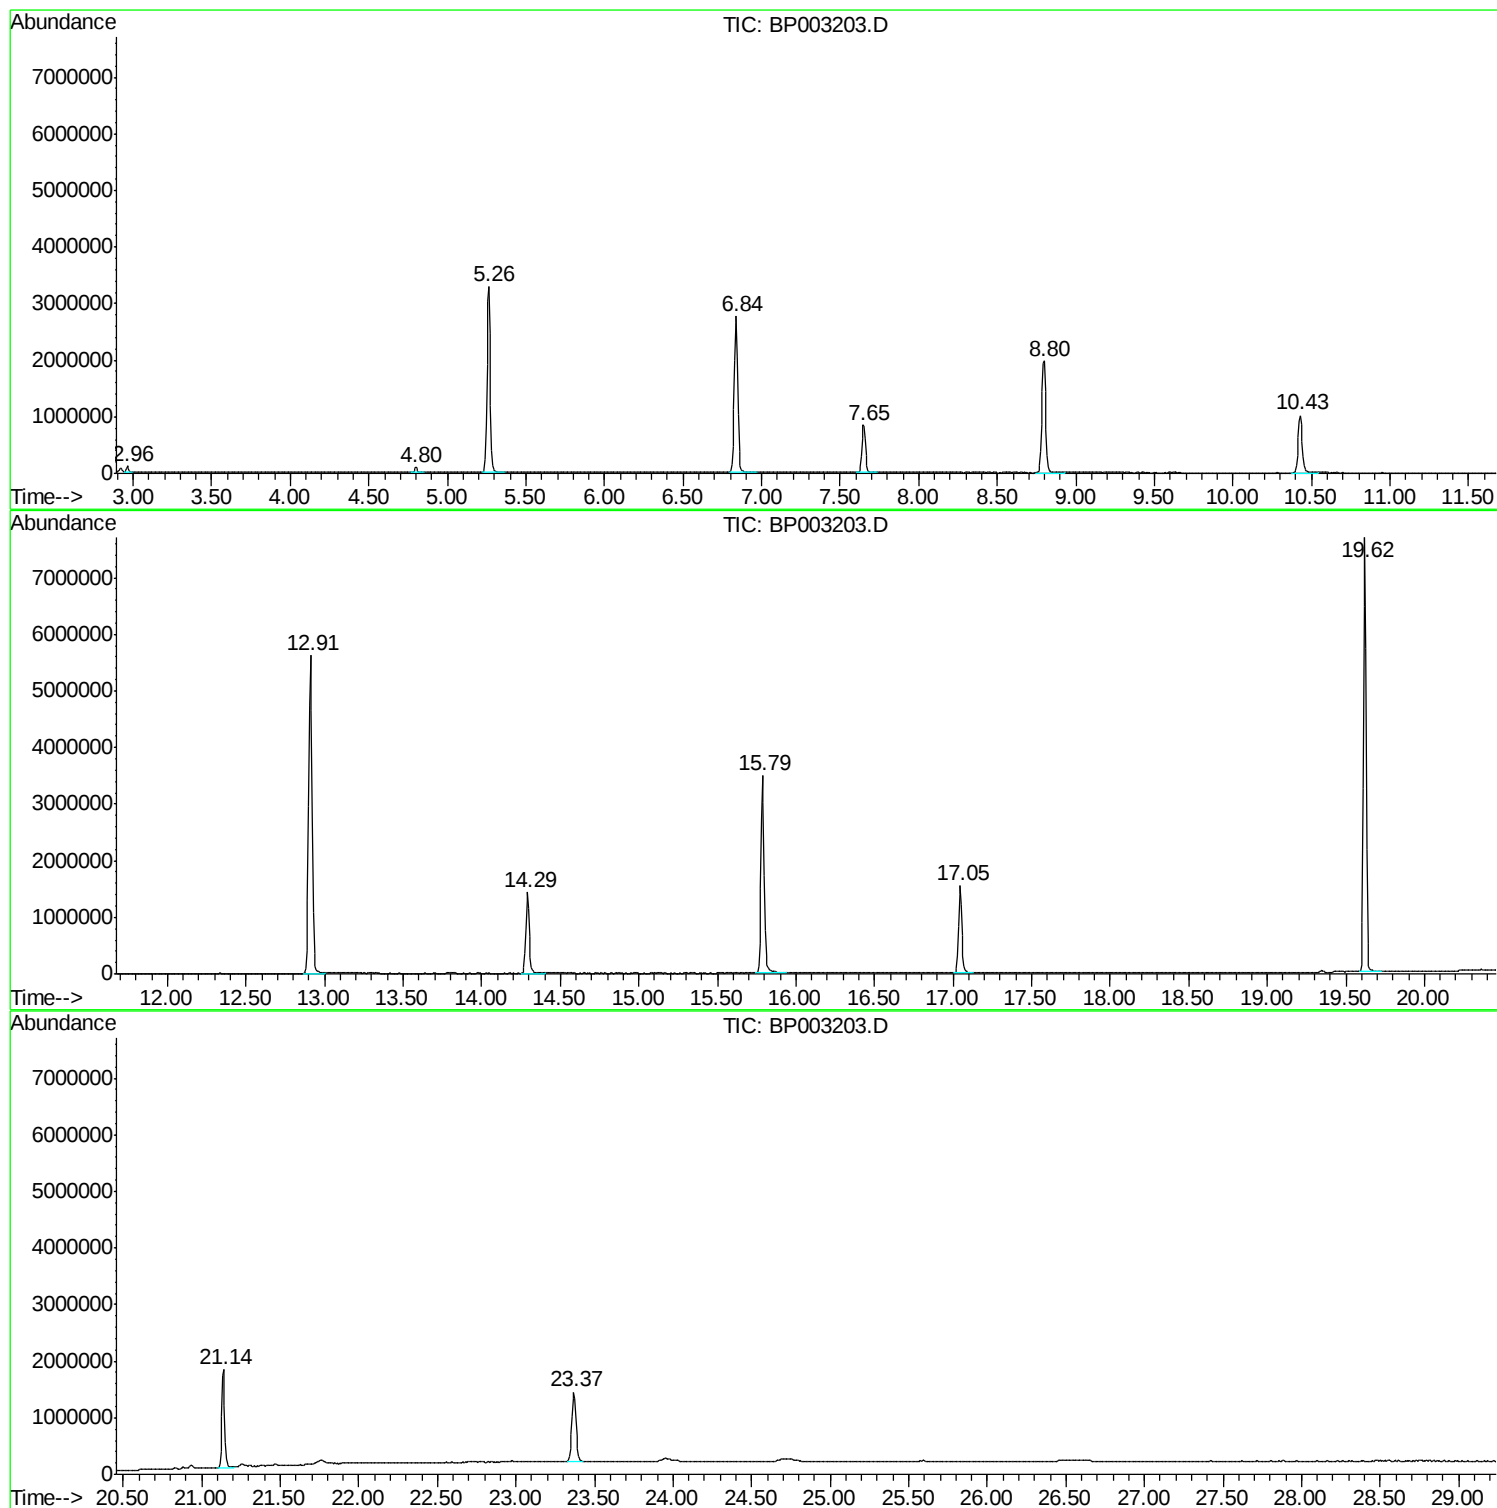

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP090420\
Data File : BP003203.D
Acq On : 04 Sep 2020 10:13
Operator : CG/JU
Sample : PB131395BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB131395BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP082420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP090420\
Data File : BP003203.D
Acq On : 04 Sep 2020 10:13
Operator : CG/JU
Sample : PB131395BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB131395BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP082420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc