


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090420\
 Data File : BP003201.D
 Acq On : 04 Sep 2020 09:05
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP082420.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 01 14:37:05 2020

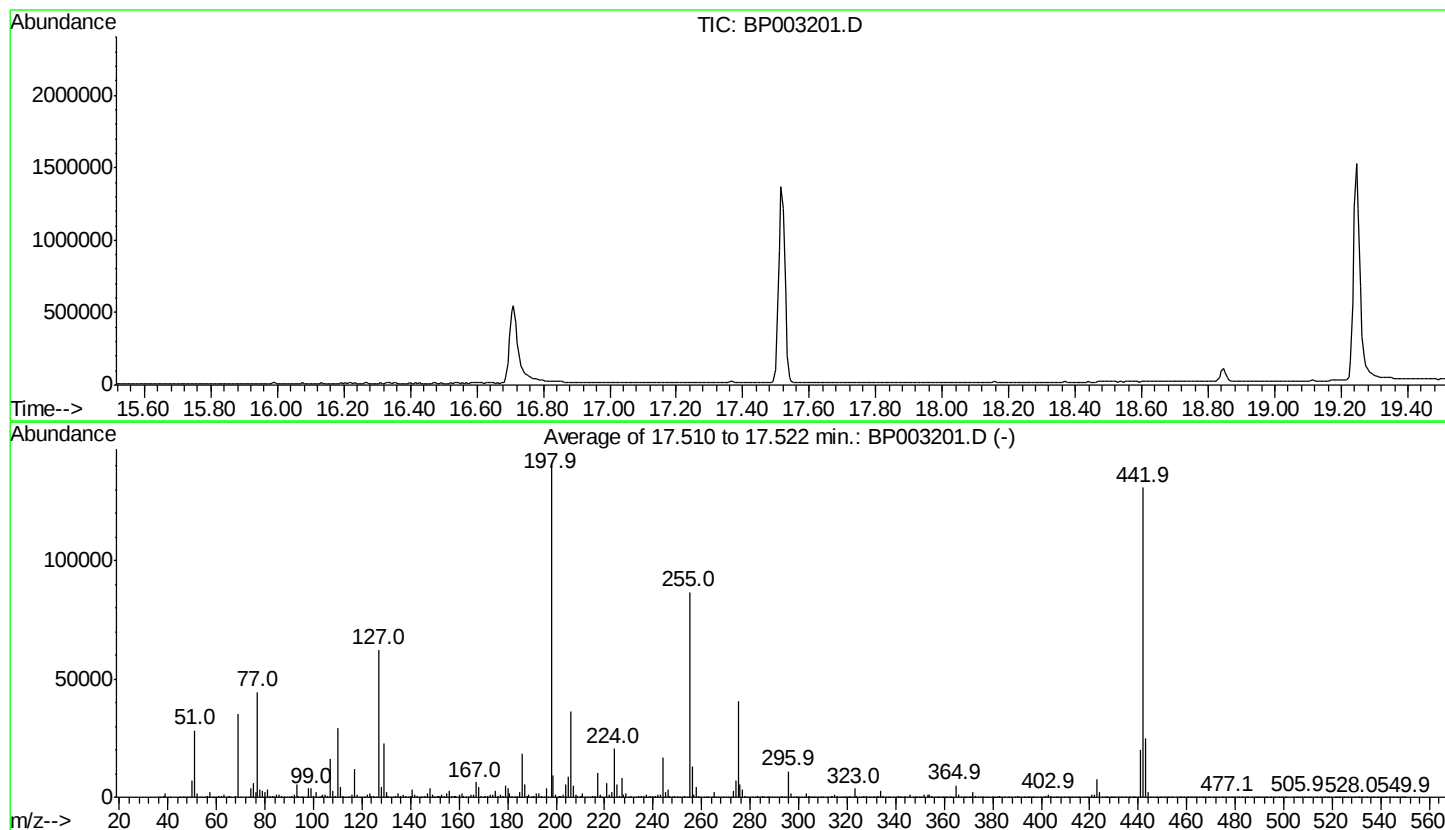

AutoFind: Scans 2486, 2487, 2488; Background Corrected with Scan 2477

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	20.1	28186	PASS
68	69	0.00	2	1.9	662	PASS
69	198	0.00	100	25.0	35079	PASS
70	69	0.00	2	0.6	206	PASS
127	198	10	80	44.4	62243	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	140181	PASS
199	198	5	9	6.8	9467	PASS
275	198	10	60	28.8	40346	PASS
365	198	1	100	3.6	5116	PASS
441	198	0.01	100	14.2	19856	PASS
442	198	50	100	93.4	130898	PASS
443	442	15	24	19.2	25067	PASS