

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090523\
 Data File : BP016952.D
 Acq On : 05 Sep 2023 13:15
 Operator : MA/JU
 Sample : SST04040
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SST040648

Quant Time: Sep 06 01:18:58 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 06 01:15:58 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.981	152	357400	20.000	ng/ul	0.00
20) Naphthalene-d8	10.810	136	1485895	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.640	164	883989	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.410	188	1795081	20.000	ng/ul	0.00
79) Chrysene-d12	21.510	240	1345527	20.000	ng/ul	0.00
88) Perylene-d12	24.051	264	1092429	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.328	96	152408	16.130	ng/uL	0.00
4) Pyridine-d5	3.764	84	1094901	40.555	ng/ul	0.00
7) Phenol-d5	7.134	99	1307193	40.034	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.322	67	814505	39.880	ng/ul	0.00
11) 2-Chlorophenol-d4	7.505	132	977582	41.367	ng/ul	0.00
15) 4-Methylphenol-d8	8.699	113	991255	39.849	ng/ul	0.00
21) Nitrobenzene-d5	9.187	128	489440	42.458	ng/ul	0.00
24) 2-Nitrophenol-d4	9.899	143	539100	43.141	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.422	165	965409	41.846	ng/ul	0.00
31) 4-Chloroaniline-d4	10.975	131	1324518	39.794	ng/ul	0.00
46) Dimethylphthalate-d6	14.057	166	2638612	40.099	ng/ul	0.00
49) Acenaphthylene-d8	14.340	160	3144221	41.404	ng/ul	0.00
54) 4-Nitrophenol-d4	14.857	143	512261	39.854	ng/ul	0.00
60) Fluorene-d10	15.640	176	2263451	40.176	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.769	200	432585	40.044	ng/ul	0.00
73) Anthracene-d10	17.510	188	3390982	41.134	ng/ul	0.00
81) Pyrene-d10	19.745	212	3515429	42.894	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.880	264	2310574	41.691	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.364	88	164290	16.104	ng/uL	98
5) Pyridine	3.787	79	1149270	39.987	ng/ul	97
6) Benzaldehyde	7.140	77	740826	50.059	ng/ul	99
8) Phenol	7.164	94	1361166	40.123	ng/ul	98
10) Bis(2-Chloroethyl)ether	7.417	93	1087512	40.199	ng/ul	99
12) 2-Chlorophenol	7.540	128	1032945	41.029	ng/ul	97
13) 2-Methylphenol	8.422	108	996641	40.051	ng/ul	98
14) 2,2'-oxybis(1-Chloropr...	8.499	45	783858	20.570	ng/ul	99
16) Acetophenone	8.834	105	1621055	40.383	ng/ul	99
17) N-Nitroso-di-n-propyla...	8.811	70	871537	40.643	ng/ul	99
18) 4-Methylphenol	8.763	108	1089197	40.136	ng/ul	99
19) Hexachloroethane	9.052	117	428863	41.121	ng/ul	100
22) Nitrobenzene	9.228	77	1268896	41.224	ng/ul	99
23) Isophorone	9.746	82	2364048	40.881	ng/ul	99
25) 2-Nitrophenol	9.934	139	586251	42.611	ng/ul	97
26) 2,4-Dimethylphenol	9.969	107	1149117	40.906	ng/ul	97
27) Bis(2-Chloroethoxy)met...	10.228	93	1461928	40.792	ng/ul	100
29) 2,4-Dichlorophenol	10.452	162	972323	41.355	ng/ul	99
30) Naphthalene	10.863	128	3279661	40.450	ng/ul	100
32) 4-Chloroaniline	10.999	127	1385380	39.994	ng/ul	100
33) Hexachlorobutadiene	11.093	225	581808	41.402	ng/ul	99
34) Caprolactam	11.822	113	190353	24.440	ng/ul	98
35) 4-Chloro-3-methylphenol	12.099	107	1053643	40.894	ng/ul	99
36) 2-Methylnaphthalene	12.469	142	2164045	40.388	ng/ul	99

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090523\
 Data File : BP016952.D
 Acq On : 05 Sep 2023 13:15
 Operator : MA/JU
 Sample : SST04040
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SST040648


Quant Time: Sep 06 01:18:58 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 06 01:15:58 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.687	142	2172785	40.278	ng/ul	99
39) 1,2,4,5-Tetrachloroben...	12.816	216	1090690	41.877	ng/ul	99
40) Hexachlorocyclopentadiene	12.763	237	688351	40.790	ng/ul	100
41) 2,4,6-Trichlorophenol	13.069	196	748131	42.204	ng/ul	98
42) 2,4,5-Trichlorophenol	13.140	196	813703	42.188	ng/ul	100
43) 1,1'-Biphenyl	13.475	154	2866639	40.967	ng/ul	100
44) 2-Chloronaphthalene	13.522	162	2256722	41.077	ng/ul	99
45) 2-Nitroaniline	13.757	65	700431	42.809	ng/ul	95
47) Dimethylphthalate	14.104	163	2762979	40.018	ng/ul	99
48) 2,6-Dinitrotoluene	14.251	165	572351	42.686	ng/ul	95
50) Acenaphthylene	14.369	152	3482817	40.959	ng/ul	99
51) 3-Nitroaniline	14.587	138	568245	42.465	ng/ul	97
52) Acenaphthene	14.704	153	2407582	40.582	ng/ul	99
53) 2,4-Dinitrophenol	14.787	184	328881	39.560	ng/ul	93
55) 4-Nitrophenol	14.875	109	406190	39.484	ng/ul	95
56) Dibenzofuran	15.046	168	3259153	39.953	ng/ul	100
57) 2,4-Dinitrotoluene	15.028	165	815479	42.369	ng/ul	99
58) 2,3,4,6-Tetrachlorophenol	15.257	232	639115	41.099	ng/ul	100
59) Diethylphthalate	15.457	149	2756475	39.952	ng/ul	100
61) Fluorene	15.693	166	2709763	40.291	ng/ul	100
62) 4-Chlorophenyl-phenyle...	15.687	204	1317612	40.539	ng/ul	99
63) 4-Nitroaniline	15.757	138	518976	44.112	ng/ul	97
66) 4,6-Dinitro-2-methylph...	15.781	198	453644	40.082	ng/ul	98
67) N-Nitrosodiphenylamine	15.910	169	2245566	41.487	ng/ul	99
68) 4-Bromophenyl-phenylether	16.587	248	750367	42.016	ng/ul	97
69) Hexachlorobenzene	16.669	284	805089	41.125	ng/ul	98
70) Atrazine	16.863	200	763793	41.214	ng/ul	100
71) Pentachlorophenol	17.034	266	509565	39.915	ng/ul	99
72) Phenanthrene	17.451	178	4067325	40.776	ng/ul	100
74) Anthracene	17.545	178	4092543	40.815	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.428	216	1102970	43.135	ng/uL	99
76) Pentachlorobenzene	14.934	250	1033450	41.959	ng/uL	99
77) Carbazole	17.828	167	3661915	40.639	ng/ul	99
78) Di-n-butylphthalate	18.339	149	4558078	41.290	ng/ul	100
80) Fluoranthene	19.416	202	4384633	42.847	ng/ul	100
82) Pyrene	19.775	202	4526560	42.603	ng/ul	100
83) Butylbenzylphthalate	20.633	149	1916776	43.623	ng/ul	97
84) 3,3'-Dichlorobenzidine	21.428	252	1243251	41.634	ng/ul	99
85) Benzo(a)anthracene	21.492	228	3877321	40.916	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.369	149	2593099	42.718	ng/ul	100
87) Chrysene	21.545	228	3618991	40.826	ng/ul	98
89) Di-n-octyl phthalate	22.339	149	3967518	43.325	ng/ul	100
90) Benzo(b)fluoranthene	23.257	252	3257453	42.678	ng/ul	100
91) Benzo(k)fluoranthene	23.310	252	3117371	42.177	ng/ul	99
93) Benzo(a)pyrene	23.933	252	2671321	41.962	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	26.745	276	2773255	39.244	ng/ul	99
95) Dibenzo(a,h)anthracene	26.774	278	2293159	39.316	ng/ul	100
96) Benzo(g,h,i)perylene	27.592	276	2155175	38.701	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Sep 06 01:18:58 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 06 01:15:58 2023
Response via : Initial Calibration









#2
1,4-Dioxane
Concen: 16.104 ng/uL
RT: 3.364 min Scan# 11
Delta R.T. 0.000 min
Lab File: BP016952.D
Acq: 05 Sep 2023 13:15




Instrument :
BNA_P
ClientSampleId :
SSTD040648


Tgt Ion: 88 Resp: 164290
Ion Ratio Lower Upper
88 100
43 31.1 25.0 37.6
58 74.0 60.6 90.8

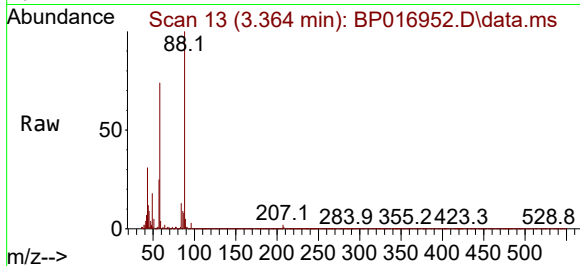

#5
Pyridine
Concen: 39.987 ng/uL
RT: 3.787 min Scan# 85
Delta R.T. 0.000 min
Lab File: BP016952.D
Acq: 05 Sep 2023 13:15

Tgt Ion: 79 Resp: 1149270
Ion Ratio Lower Upper
79 100
52 73.5 60.1 90.1
51 35.6 30.5 45.7



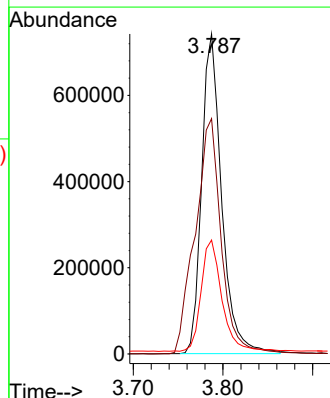
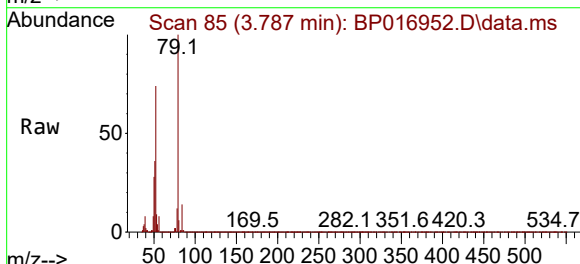




#6
Benzaldehyde
Concen: 50.059 ng/ul
RT: 7.140 min Scan# 61
Delta R.T. 0.000 min
Lab File: BP016952.D
Acq: 05 Sep 2023 13:15




Instrument :
BNA_P
ClientSampleId :
SSTD040648


Tgt Ion: 77 Resp: 740826
Ion Ratio Lower Upper
77 100
105 94.9 75.4 113.0
106 90.8 71.4 107.2



#8
Phenol
Concen: 40.123 ng/ul
RT: 7.164 min Scan# 659
Delta R.T. 0.006 min
Lab File: BP016952.D
Acq: 05 Sep 2023 13:15

Tgt Ion: 94 Resp: 1361166
Ion Ratio Lower Upper
94 100
65 28.1 23.2 34.8
66 35.6 29.4 44.2









#10
 Bis(2-Chloroethyl)ether
 Concen: 40.199 ng/ul
 RT: 7.417 min Scan# 702
 Delta R.T. 0.000 min
 Lab File: BP016952.D
 Acq: 05 Sep 2023 13:15

Instrument :
 BNA_P
 ClientSampleId :
 SSTD040648

Tgt Ion: 93 Resp: 1087512




Ion	Ratio	Lower	Upper
93	100		
63	77.9	63.4	95.2
95	32.0	26.1	39.1

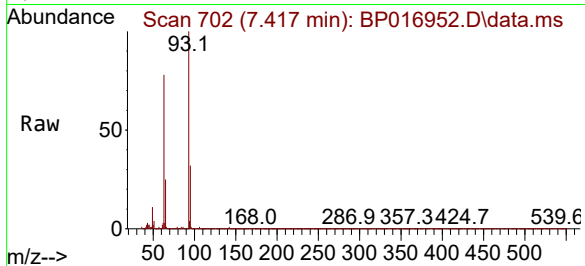


#12
 2-Chlorophenol
 Concen: 41.029 ng/ul
 RT: 7.540 min Scan# 723
 Delta R.T. 0.006 min
 Lab File: BP016952.D
 Acq: 05 Sep 2023 13:15

Tgt Ion: 128 Resp: 1032945

Ion	Ratio	Lower	Upper
128	100		
64	48.5	40.2	60.2
130	33.0	25.2	37.8




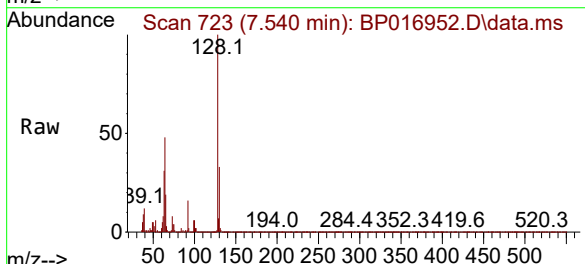




#13
2-Methylphenol
Concen: 40.051 ng/ul
RT: 8.422 min Scan# 81
Delta R.T. 0.000 min
Lab File: BP016952.D
Acq: 05 Sep 2023 13:15




Instrument :
BNA_P
ClientSampleId :
SSTD040648


Tgt Ion:108 Resp: 996641
Ion Ratio Lower Upper
108 100
107 89.8 70.6 106.0

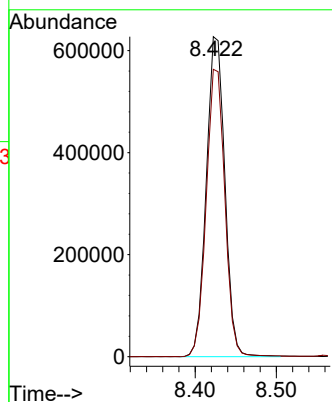

#14
2,2'-oxybis(1-Chloropropane)
Concen: 20.570 ng/ul
RT: 8.499 min Scan# 886
Delta R.T. -0.017 min
Lab File: BP016952.D
Acq: 05 Sep 2023 13:15

Tgt Ion: 45 Resp: 783858
Ion Ratio Lower Upper
45 100
77 14.0 11.3 16.9
79 10.4 9.0 13.4









#16
Acetophenone
Concen: 40.383 ng/ul
RT: 8.834 min Scan# 943
Delta R.T. 0.000 min
Lab File: BP016952.D
Acq: 05 Sep 2023 13:15




Instrument :
BNA_P
ClientSampleId :
SSTD040648


Tgt Ion:105 Resp: 1621055
Ion Ratio Lower Upper
105 100
77 80.6 63.6 95.4
51 28.7 23.4 35.0



#17
N-Nitroso-di-n-propylamine
Concen: 40.643 ng/ul
RT: 8.811 min Scan# 939
Delta R.T. 0.006 min
Lab File: BP016952.D
Acq: 05 Sep 2023 13:15

Tgt Ion: 70 Resp: 871537
Ion Ratio Lower Upper
70 100
42 58.0 47.4 71.2
101 9.4 7.3 10.9
130 19.6 15.6 23.4









#18
4-Methylphenol
Concen: 40.136 ng/ul
RT: 8.763 min Scan# 91
Delta R.T. 0.006 min
Lab File: BP016952.D
Acq: 05 Sep 2023 13:15




Instrument :
BNA_P
ClientSampleId :
SSTD040648


Tgt Ion:108 Resp: 1089197
Ion Ratio Lower Upper
108 100
107 112.6 90.6 135.8



#19
Hexachloroethane
Concen: 41.121 ng/ul
RT: 9.052 min Scan# 980
Delta R.T. 0.000 min
Lab File: BP016952.D
Acq: 05 Sep 2023 13:15

Tgt Ion:117 Resp: 428863
Ion Ratio Lower Upper
117 100
201 94.7 75.8 113.6
199 59.3 46.8 70.2



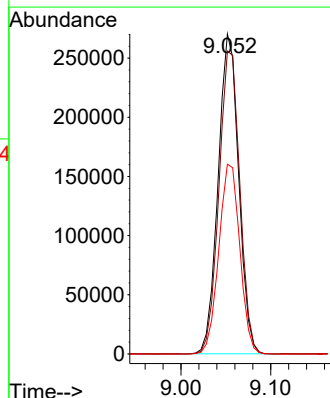





#22
Nitrobenzene
Concen: 41.224 ng/ul
RT: 9.228 min Scan# 1009
Delta R.T. 0.006 min
Lab File: BP016952.D
Acq: 05 Sep 2023 13:15




Instrument :
BNA_P
ClientSampleId :
SSTD040648


Tgt Ion: 77 Resp: 1268896
Ion Ratio Lower Upper
77 100
123 43.5 34.4 51.6
65 13.3 10.6 15.8

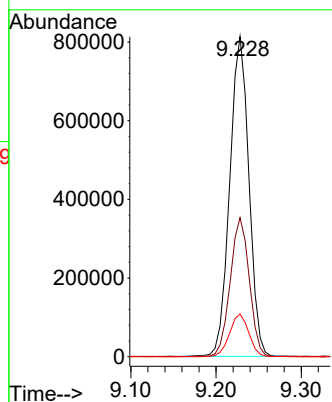

#23
Isophorone
Concen: 40.881 ng/ul
RT: 9.746 min Scan# 1098
Delta R.T. 0.006 min
Lab File: BP016952.D
Acq: 05 Sep 2023 13:15

Tgt Ion: 82 Resp: 2364048
Ion Ratio Lower Upper
82 100
95 6.7 5.3 7.9
138 17.1 13.4 20.2









#25
2-Nitrophenol
Concen: 42.611 ng/ul
RT: 9.934 min Scan# 1129
Delta R.T. 0.006 min
Lab File: BP016952.D
Acq: 05 Sep 2023 13:15




Instrument :
BNA_P
ClientSampleId :
SSTD040648


Tgt Ion:139 Resp: 586251
Ion Ratio Lower Upper
139 100
65 52.3 44.0 66.0
109 29.3 24.1 36.1

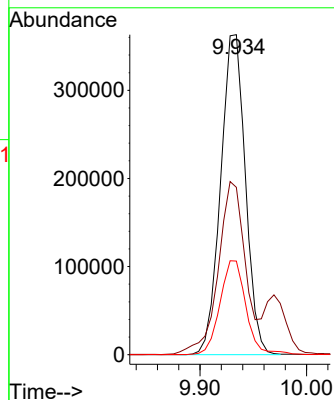

#26
2,4-Dimethylphenol
Concen: 40.906 ng/ul
RT: 9.969 min Scan# 1136
Delta R.T. 0.000 min
Lab File: BP016952.D
Acq: 05 Sep 2023 13:15

Tgt Ion:107 Resp: 1149117
Ion Ratio Lower Upper
107 100
121 49.3 41.0 61.6
122 83.9 69.0 103.4

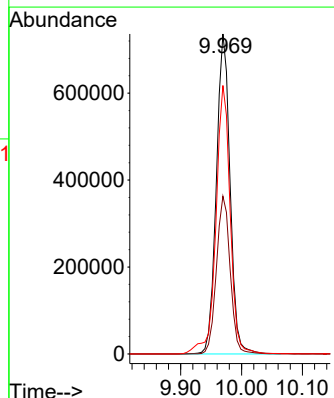



#27

Bis(2-Chloroethoxy)methane

Concen: 40.792 ng/ul

RT: 10.228 min Scan# 1180

Delta R.T. 0.000 min

Lab File: BP016952.D

Acq: 05 Sep 2023 13:15

Instrument :

BNA_P

ClientSampleId :

SSTD040648





Tgt Ion: 93 Resp: 1461928

Ion Ratio Lower Upper

93 100

95 32.2 26.0 39.0

123 10.8 8.6 13.0



#29

2,4-Dichlorophenol

Concen: 41.355 ng/ul

RT: 10.452 min Scan# 1218

Delta R.T. 0.000 min

Lab File: BP016952.D

Acq: 05 Sep 2023 13:15




Tgt Ion:162 Resp: 972323


Ion Ratio Lower Upper

162 100

164 64.6 51.8 77.6

98 37.2 28.2 42.4



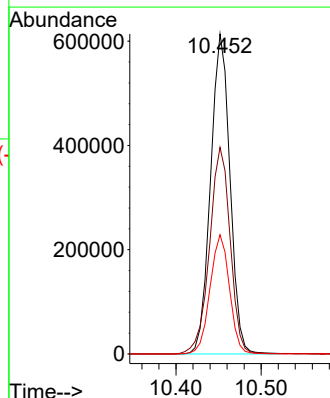





#30
Naphthalene
Concen: 40.450 ng/ul
RT: 10.863 min Scan# 11
Delta R.T. 0.000 min
Lab File: BP016952.D
Acq: 05 Sep 2023 13:15




Instrument :
BNA_P
ClientSampleId :
SSTD040648


Tgt Ion:128 Resp: 3279661
Ion Ratio Lower Upper
128 100
129 10.9 8.8 13.2
127 13.2 10.3 15.5

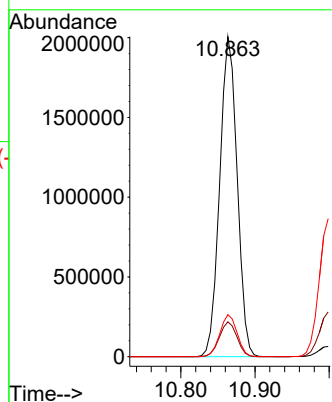

#32
4-Chloroaniline
Concen: 39.994 ng/ul
RT: 10.999 min Scan# 1311
Delta R.T. 0.006 min
Lab File: BP016952.D
Acq: 05 Sep 2023 13:15

Tgt Ion:127 Resp: 1385380
Ion Ratio Lower Upper
127 100
129 32.4 26.0 39.0









#33
Hexachlorobutadiene
Concen: 41.402 ng/ul
RT: 11.093 min Scan# 11
Delta R.T. 0.000 min
Lab File: BP016952.D
Acq: 05 Sep 2023 13:15




Instrument :
BNA_P
ClientSampleId :
SSTD040648


Tgt Ion:225 Resp: 581808
Ion Ratio Lower Upper
225 100
223 63.2 50.1 75.1
227 62.3 50.9 76.3

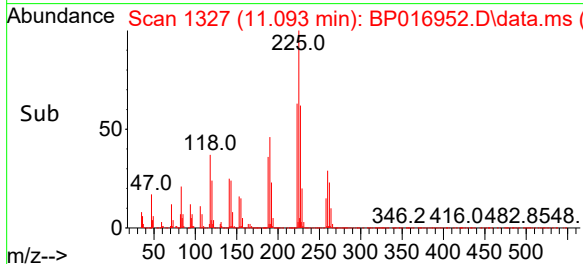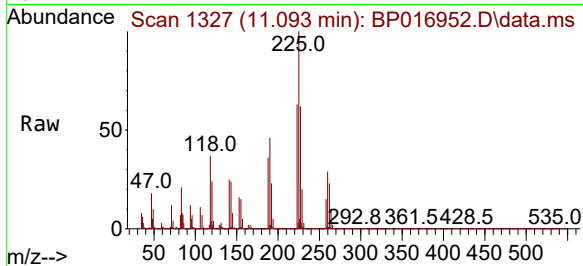

#34
Caprolactam
Concen: 24.440 ng/ul
RT: 11.822 min Scan# 1451
Delta R.T. 0.012 min
Lab File: BP016952.D
Acq: 05 Sep 2023 13:15

Tgt Ion:113 Resp: 190353
Ion Ratio Lower Upper
113 100
55 175.4 142.3 213.5
56 129.1 102.2 153.2


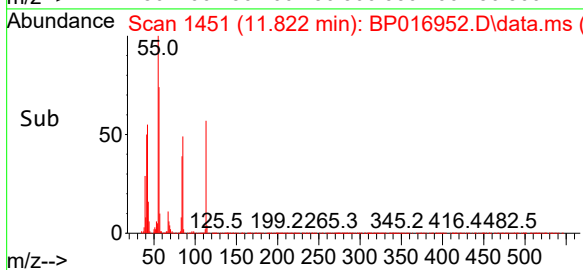

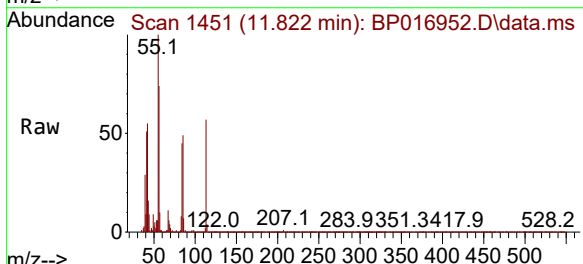




#35
4-Chloro-3-methylphenol
Concen: 40.894 ng/ul
RT: 12.099 min Scan# 1497
Delta R.T. 0.006 min
Lab File: BP016952.D
Acq: 05 Sep 2023 13:15




Instrument :
BNA_P
ClientSampleId :
SSTD040648


Tgt Ion:107 Resp: 1053643
Ion Ratio Lower Upper
107 100
144 25.9 20.3 30.5
142 79.5 63.8 95.8

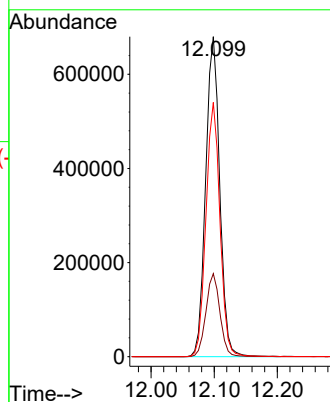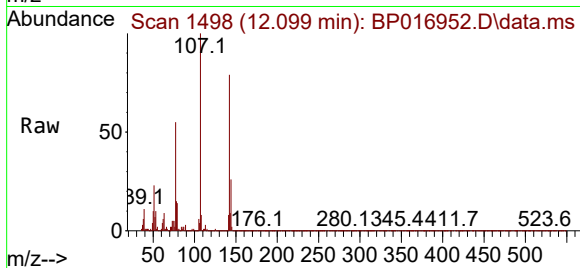

#36
2-Methylnaphthalene
Concen: 40.388 ng/ul
RT: 12.469 min Scan# 1561
Delta R.T. 0.000 min
Lab File: BP016952.D
Acq: 05 Sep 2023 13:15

Tgt Ion:142 Resp: 2164045
Ion Ratio Lower Upper
142 100
141 89.6 71.1 106.7

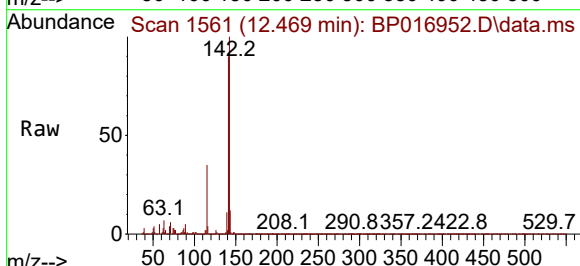



#37

1-Methylnaphthalene

Concen: 40.278 ng/ul

RT: 12.687 min Scan# 1598

Delta R.T. 0.000 min

Lab File: BP016952.D

Acq: 05 Sep 2023 13:15

Instrument :

BNA_P

ClientSampleId :

SSTD040648





Tgt Ion:142 Resp: 2172785

Ion Ratio Lower Upper

142 100

141 91.9 74.5 111.7

116 3.8 3.1 4.7

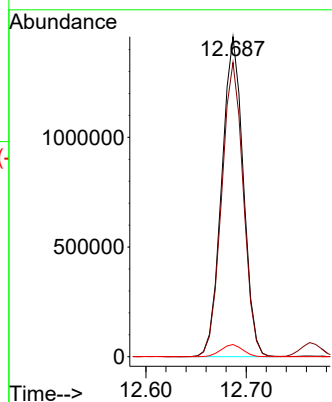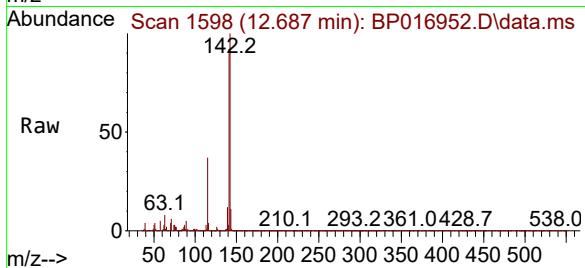

#39

1,2,4,5-Tetrachlorobenzene

Concen: 41.877 ng/ul

RT: 12.816 min Scan# 1620

Delta R.T. 0.000 min

Lab File: BP016952.D

Acq: 05 Sep 2023 13:15

Tgt Ion:216 Resp: 1090690




Ion Ratio Lower Upper


216 100

214 78.8 62.8 94.2

179 22.2 17.5 26.3

108 18.8 14.6 21.8


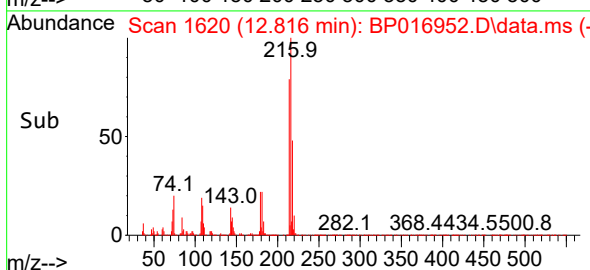

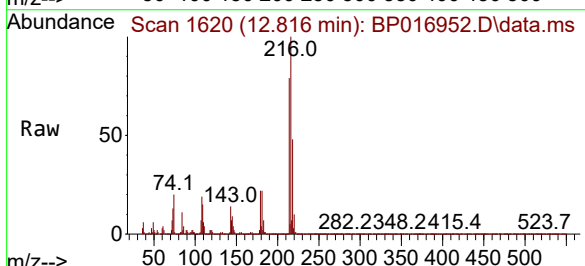




#40
Hexachlorocyclopentadiene
Concen: 40.790 ng/ul
RT: 12.763 min Scan# 1611
Delta R.T. 0.000 min
Lab File: BP016952.D
Acq: 05 Sep 2023 13:15




Instrument :
BNA_P
ClientSampleId :
SSTD040648


Tgt Ion:237 Resp: 688351
Ion Ratio Lower Upper
237 100
235 63.2 50.8 76.2
272 12.3 10.0 15.0



#41
2,4,6-Trichlorophenol
Concen: 42.204 ng/ul
RT: 13.069 min Scan# 1663
Delta R.T. 0.000 min
Lab File: BP016952.D
Acq: 05 Sep 2023 13:15

Tgt Ion:196 Resp: 748131
Ion Ratio Lower Upper
196 100
198 97.0 75.8 113.6
200 31.4 24.6 36.8





#42

2,4,5-Trichlorophenol

Concen: 42.188 ng/ul

RT: 13.140 min Scan# 1

Delta R.T. 0.000 min

Lab File: BP016952.D

Acq: 05 Sep 2023 13:15

Instrument :

BNA_P

ClientSampleId :

SSTD040648





Tgt Ion:196 Resp: 813703

Ion Ratio Lower Upper

196 100

198 93.6 74.9 112.3

200 30.4 24.5 36.7

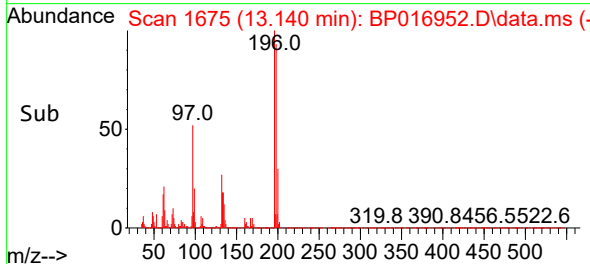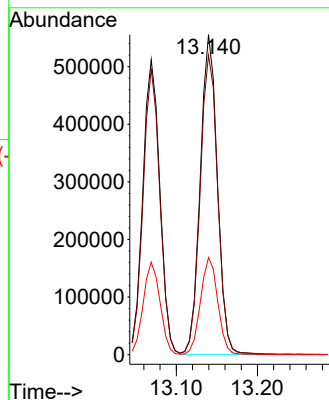

#43

1,1'-Biphenyl

Concen: 40.967 ng/ul

RT: 13.475 min Scan# 1732

Delta R.T. 0.000 min

Lab File: BP016952.D

Acq: 05 Sep 2023 13:15




Tgt Ion:154 Resp: 2866639


Ion Ratio Lower Upper

154 100

153 41.1 32.7 49.1

76 14.6 11.5 17.3



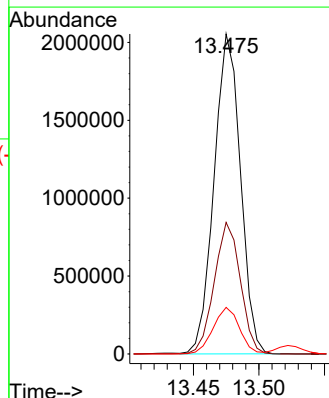





#44
2-Chloronaphthalene
Concen: 41.077 ng/ul
RT: 13.522 min Scan# 1740
Delta R.T. 0.000 min
Lab File: BP016952.D
Acq: 05 Sep 2023 13:15




Instrument :
BNA_P
ClientSampleId :
SSTD040648


Tgt Ion:162 Resp: 2256722
Ion Ratio Lower Upper
162 100
164 32.8 26.2 39.4
127 39.3 30.8 46.2

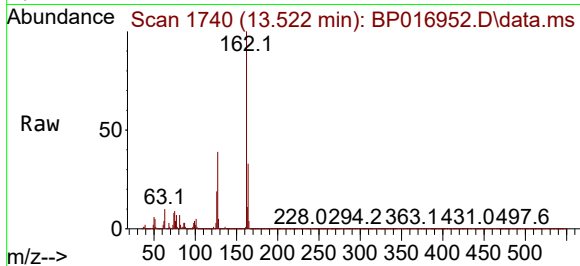

#45
2-Nitroaniline
Concen: 42.809 ng/ul
RT: 13.757 min Scan# 1780
Delta R.T. 0.006 min
Lab File: BP016952.D
Acq: 05 Sep 2023 13:15

Tgt Ion: 65 Resp: 700431
Ion Ratio Lower Upper
65 100
92 68.6 55.4 83.0
138 103.6 76.8 115.2




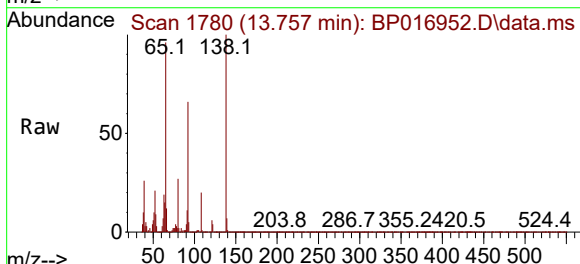




#47
Dimethylphthalate
Concen: 40.018 ng/ul
RT: 14.104 min Scan# 1839
Delta R.T. 0.000 min
Lab File: BP016952.D
Acq: 05 Sep 2023 13:15




Instrument :
BNA_P
ClientSampleId :
SSTD040648


Tgt Ion:163 Resp: 2762979
Ion Ratio Lower Upper
163 100
194 3.9 3.1 4.7
164 10.2 7.9 11.9

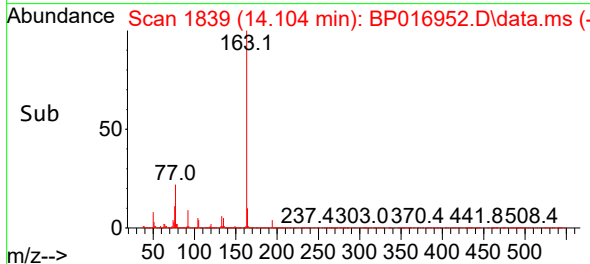

#48
2,6-Dinitrotoluene
Concen: 42.686 ng/ul
RT: 14.251 min Scan# 1864
Delta R.T. 0.006 min
Lab File: BP016952.D
Acq: 05 Sep 2023 13:15

Tgt Ion:165 Resp: 572351
Ion Ratio Lower Upper
165 100
89 58.5 50.0 75.0
121 20.6 17.8 26.6


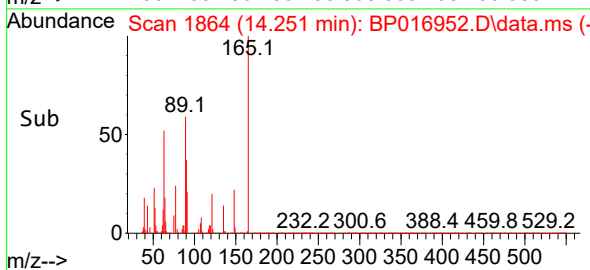

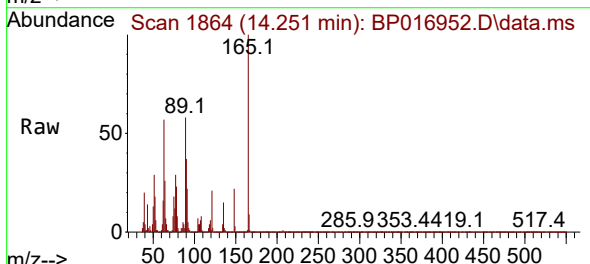




#50
Acenaphthylene
Concen: 40.959 ng/ul
RT: 14.369 min Scan# 1884
Delta R.T. 0.000 min
Lab File: BP016952.D
Acq: 05 Sep 2023 13:15




Instrument :
BNA_P
ClientSampleId :
SSTD040648


Tgt Ion:152 Resp: 3482817
Ion Ratio Lower Upper
152 100
151 20.1 15.9 23.9
153 13.4 10.5 15.7

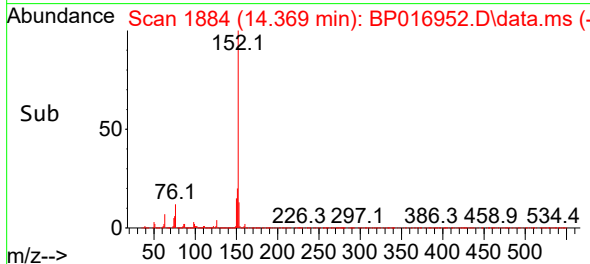

#51
3-Nitroaniline
Concen: 42.465 ng/ul
RT: 14.587 min Scan# 1921
Delta R.T. 0.006 min
Lab File: BP016952.D
Acq: 05 Sep 2023 13:15

Tgt Ion:138 Resp: 568245
Ion Ratio Lower Upper
138 100
108 10.4 8.4 12.6
92 118.4 97.2 145.8


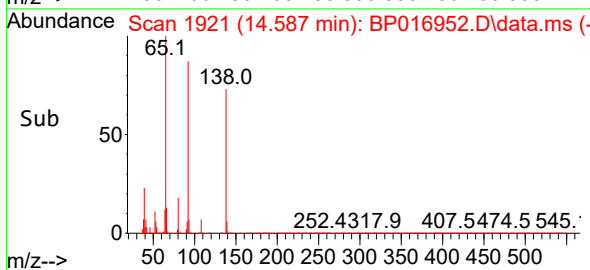

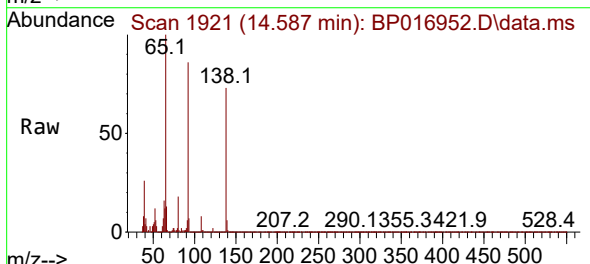




#52
Acenaphthene
Concen: 40.582 ng/ul
RT: 14.704 min Scan# 1941
Delta R.T. 0.000 min
Lab File: BP016952.D
Acq: 05 Sep 2023 13:15




Instrument :
BNA_P
ClientSampleId :
SSTD040648


Tgt Ion:153 Resp: 2407582
Ion Ratio Lower Upper
153 100
152 47.3 38.6 57.8
154 88.1 70.2 105.4



#53
2,4-Dinitrophenol
Concen: 39.560 ng/ul
RT: 14.787 min Scan# 1955
Delta R.T. 0.006 min
Lab File: BP016952.D
Acq: 05 Sep 2023 13:15

Tgt Ion:184 Resp: 328881
Ion Ratio Lower Upper
184 100
63 67.8 61.6 92.4
154 62.2 50.8 76.2









#55
4-Nitrophenol
Concen: 39.484 ng/ul
RT: 14.875 min Scan# 1969
Delta R.T. 0.006 min
Lab File: BP016952.D
Acq: 05 Sep 2023 13:15




Instrument :
BNA_P
ClientSampleId :
SSTD040648


Tgt Ion:109 Resp: 406190
Ion Ratio Lower Upper
109 100
139 136.7 105.0 157.4
65 140.6 108.4 162.6

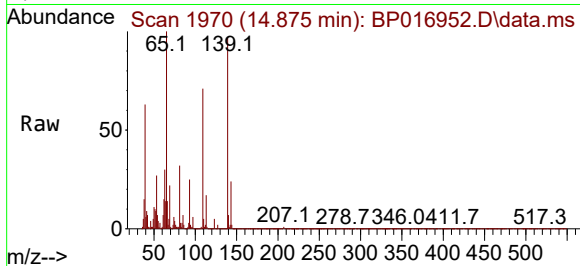

#56
Dibenzofuran
Concen: 39.953 ng/ul
RT: 15.046 min Scan# 1999
Delta R.T. 0.006 min
Lab File: BP016952.D
Acq: 05 Sep 2023 13:15

Tgt Ion:168 Resp: 3259153
Ion Ratio Lower Upper
168 100
139 37.3 30.1 45.1

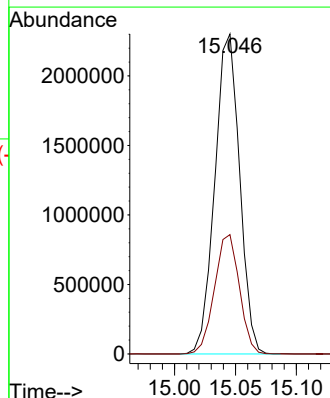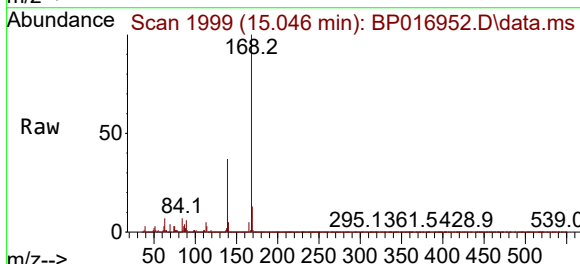



#57

2,4-Dinitrotoluene

Concen: 42.369 ng/ul

RT: 15.028 min Scan# 1996

Delta R.T. 0.000 min

Lab File: BP016952.D

Acq: 05 Sep 2023 13:15

Instrument :

BNA_P

ClientSampleId :

SSTD040648





Tgt Ion:165 Resp: 815479

Ion Ratio Lower Upper

165 100

63 52.2 42.1 63.1

182 2.6 2.3 3.5

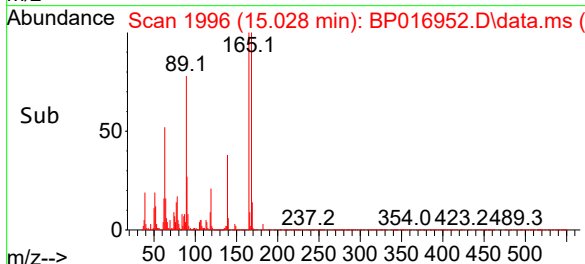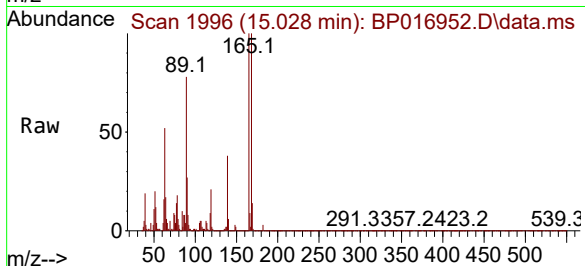

#58

2,3,4,6-Tetrachlorophenol

Concen: 41.099 ng/ul

RT: 15.257 min Scan# 2035

Delta R.T. 0.000 min

Lab File: BP016952.D

Acq: 05 Sep 2023 13:15

Tgt Ion:232 Resp: 639115




Ion Ratio Lower Upper


232 100

131 48.8 39.2 58.8

130 2.6 2.0 3.0

166 33.7 27.2 40.8


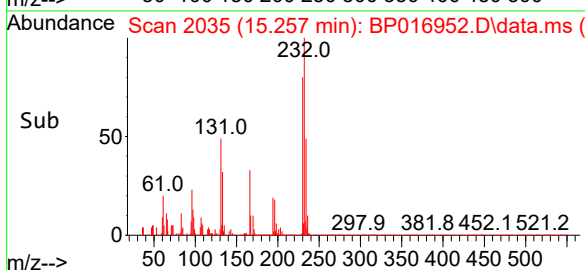

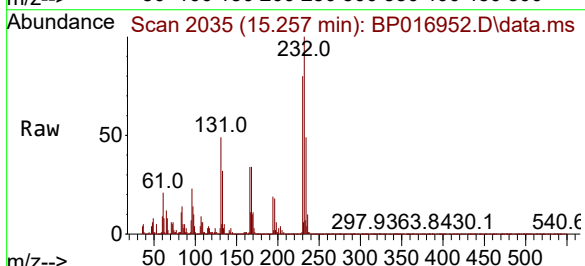




#59
Diethylphthalate
Concen: 39.952 ng/ul
RT: 15.457 min Scan# 2069
Delta R.T. 0.000 min
Lab File: BP016952.D
Acq: 05 Sep 2023 13:15




Instrument :
BNA_P
ClientSampleId :
SSTD040648


Tgt Ion:149 Resp: 2756475
Ion Ratio Lower Upper
149 100
177 21.8 17.3 25.9
150 12.6 10.1 15.1

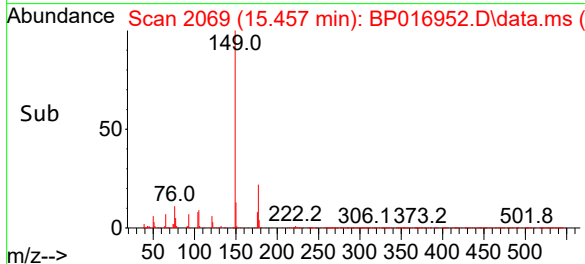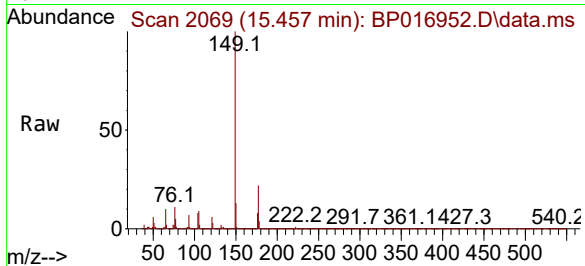

#61
Fluorene
Concen: 40.291 ng/ul
RT: 15.693 min Scan# 2109
Delta R.T. 0.000 min
Lab File: BP016952.D
Acq: 05 Sep 2023 13:15

Tgt Ion:166 Resp: 2709763
Ion Ratio Lower Upper
166 100
165 98.2 78.3 117.5
167 13.7 10.6 16.0


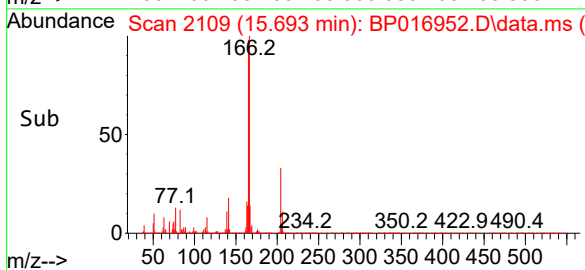

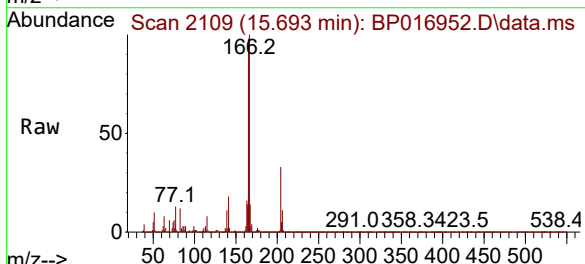




#62
4-Chlorophenyl-phenylether
Concen: 40.539 ng/ul
RT: 15.687 min Scan# 2108
Delta R.T. 0.000 min
Lab File: BP016952.D
Acq: 05 Sep 2023 13:15




Instrument :
BNA_P
ClientSampleId :
SSTD040648


Tgt Ion:204 Resp: 1317612
Ion Ratio Lower Upper
204 100
206 33.4 26.4 39.6
141 57.2 46.2 69.4

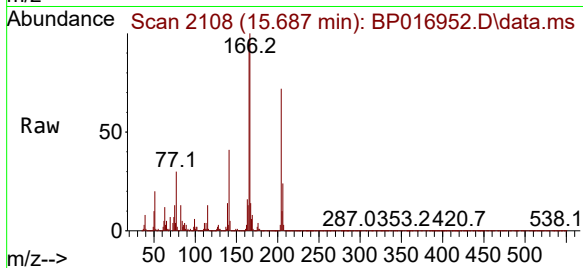

#63
4-Nitroaniline
Concen: 44.112 ng/ul
RT: 15.757 min Scan# 2120
Delta R.T. 0.006 min
Lab File: BP016952.D
Acq: 05 Sep 2023 13:15

Tgt Ion:138 Resp: 518976
Ion Ratio Lower Upper
138 100
92 53.2 41.9 62.9
108 91.8 70.3 105.5




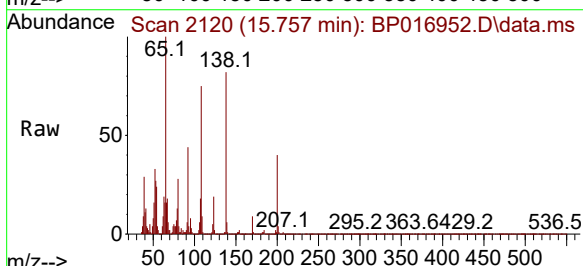




#66
4,6-Dinitro-2-methylphenol
Concen: 40.082 ng/ul
RT: 15.781 min Scan# 2124
Delta R.T. 0.000 min
Lab File: BP016952.D
Acq: 05 Sep 2023 13:15




Instrument :
BNA_P
ClientSampleId :
SSTD040648


Tgt Ion:198 Resp: 453644
Ion Ratio Lower Upper
198 100
182 4.2 3.6 5.4
77 27.9 21.4 32.0

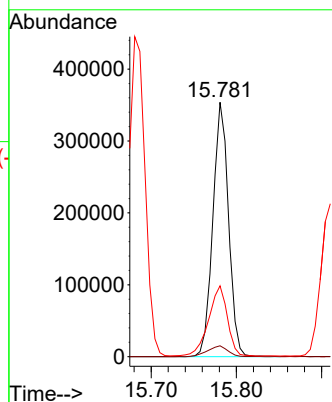

#67
N-Nitrosodiphenylamine
Concen: 41.487 ng/ul
RT: 15.910 min Scan# 2146
Delta R.T. 0.000 min
Lab File: BP016952.D
Acq: 05 Sep 2023 13:15

Tgt Ion:169 Resp: 2245566
Ion Ratio Lower Upper
169 100
168 66.5 54.2 81.4
167 37.2 29.4 44.2


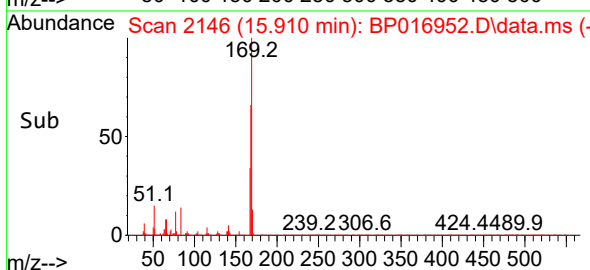






#68
4-Bromophenyl-phenylether
Concen: 42.016 ng/ul
RT: 16.587 min Scan# 2261
Delta R.T. 0.000 min
Lab File: BP016952.D
Acq: 05 Sep 2023 13:15




Instrument :
BNA_P
ClientSampleId :
SSTD040648


Tgt Ion:248 Resp: 750367
Ion Ratio Lower Upper
248 100
250 97.4 76.8 115.2
141 79.1 66.3 99.5

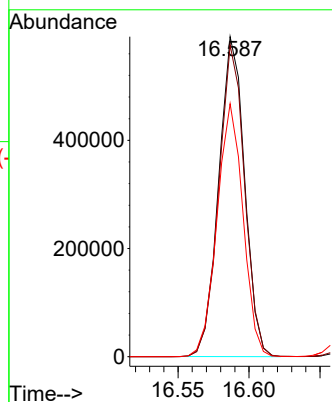

#69
Hexachlorobenzene
Concen: 41.125 ng/ul
RT: 16.669 min Scan# 2275
Delta R.T. 0.000 min
Lab File: BP016952.D
Acq: 05 Sep 2023 13:15

Tgt Ion:284 Resp: 805089
Ion Ratio Lower Upper
284 100
142 41.7 31.9 47.9
249 33.9 27.0 40.6

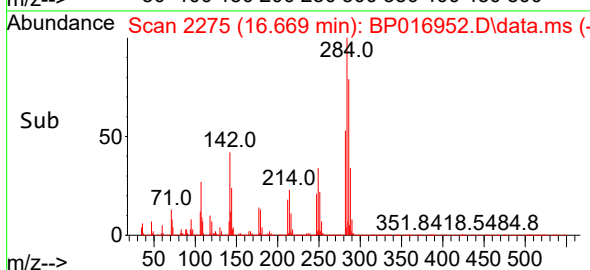



#70

Atrazine

Concen: 41.214 ng/ul

RT: 16.863 min Scan# 21

Delta R.T. 0.000 min

Lab File: BP016952.D

Acq: 05 Sep 2023 13:15

Instrument :

BNA_P

ClientSampleId :

SSTD040648





Tgt Ion:200 Resp: 763793

Ion Ratio Lower Upper

200 100

173 27.8 21.8 32.8

215 47.9 38.3 57.5

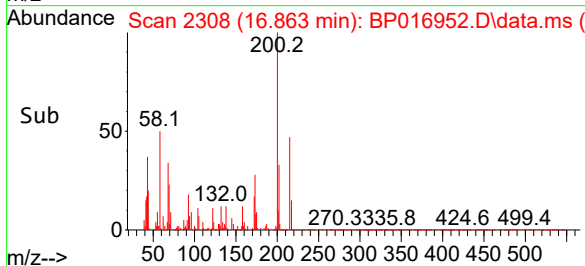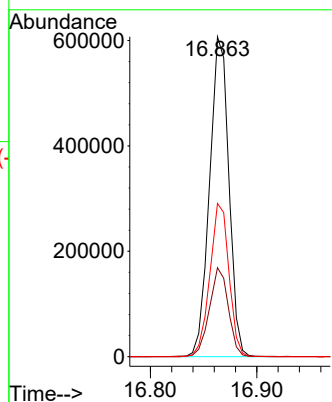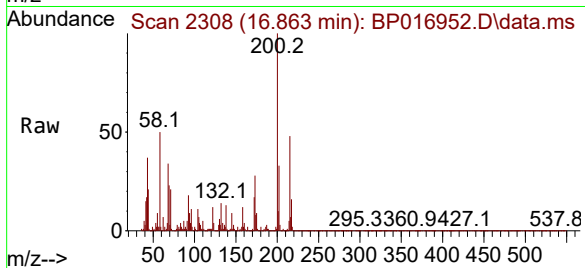

#71

Pentachlorophenol

Concen: 39.915 ng/ul

RT: 17.034 min Scan# 2337

Delta R.T. 0.000 min

Lab File: BP016952.D

Acq: 05 Sep 2023 13:15




Tgt Ion:266 Resp: 509565


Ion Ratio Lower Upper

266 100

264 62.1 50.4 75.6

268 62.4 50.4 75.6


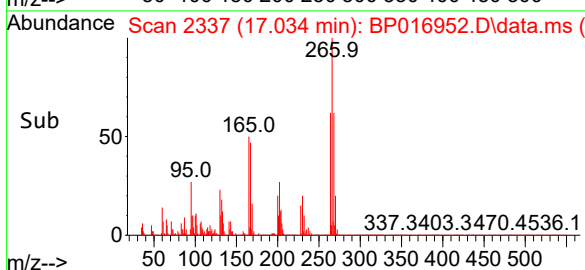

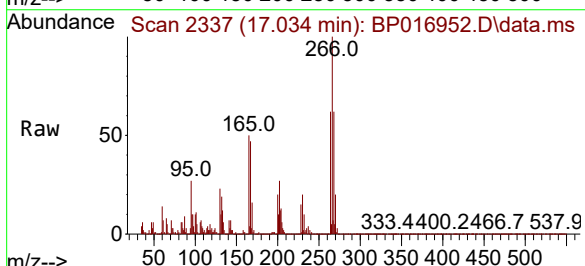




#72
Phenanthrene
Concen: 40.776 ng/ul
RT: 17.451 min Scan# 2408
Delta R.T. 0.000 min
Lab File: BP016952.D
Acq: 05 Sep 2023 13:15




Instrument :
BNA_P
ClientSampleId :
SSTD040648


Tgt Ion:178 Resp: 4067325
Ion Ratio Lower Upper
178 100
179 15.8 12.5 18.7
176 19.9 15.8 23.8

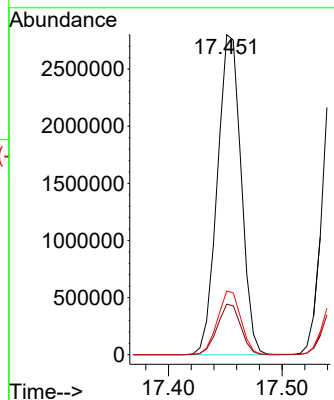

#74
Anthracene
Concen: 40.815 ng/ul
RT: 17.545 min Scan# 2424
Delta R.T. 0.000 min
Lab File: BP016952.D
Acq: 05 Sep 2023 13:15

Tgt Ion:178 Resp: 4092543
Ion Ratio Lower Upper
178 100
179 15.6 12.3 18.5
176 19.1 15.0 22.6

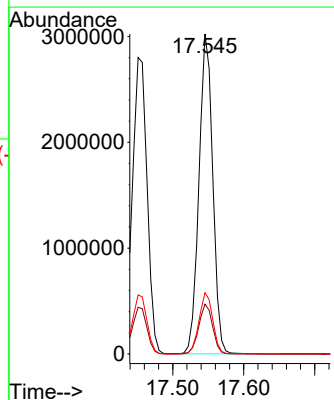



#75

1,2,3,4-Tetrachlorobenzene

Concen: 43.135 ng/uL

RT: 13.428 min Scan# 1

Delta R.T. 0.000 min

Lab File: BP016952.D

Acq: 05 Sep 2023 13:15

Instrument :

BNA_P

ClientSampleId :

SSTD040648





Tgt Ion:216 Resp: 1102970

Ion Ratio Lower Upper

216 100

214 79.2 64.5 96.7

218 48.2 38.6 57.8

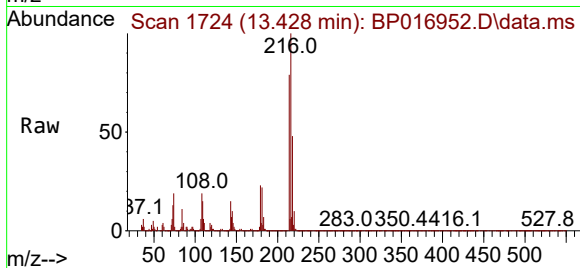

#76

Pentachlorobenzene

Concen: 41.959 ng/uL

RT: 14.934 min Scan# 1980

Delta R.T. 0.000 min

Lab File: BP016952.D

Acq: 05 Sep 2023 13:15




Tgt Ion:250 Resp: 1033450


Ion Ratio Lower Upper

250 100

248 63.3 51.2 76.8

252 64.0 50.9 76.3

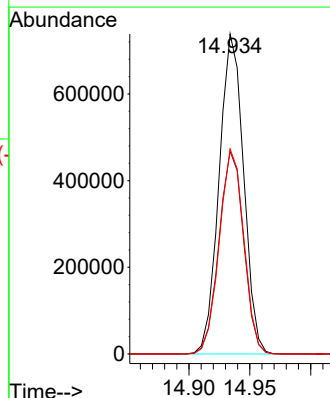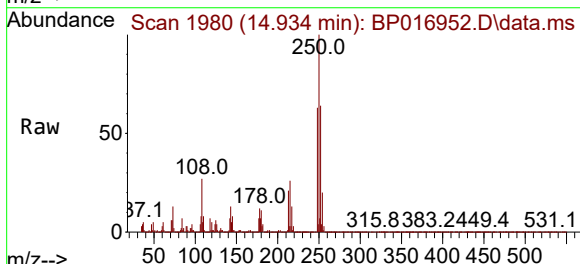



#77

Carbazole

Concen: 40.639 ng/ul

RT: 17.828 min Scan# 2472

Delta R.T. 0.000 min

Lab File: BP016952.D

Acq: 05 Sep 2023 13:15

Instrument :

BNA_P

ClientSampleId :

SSTD040648





Tgt Ion:167 Resp: 3661915

Ion Ratio Lower Upper

167 100

166 22.0 17.3 25.9

139 12.9 10.3 15.5

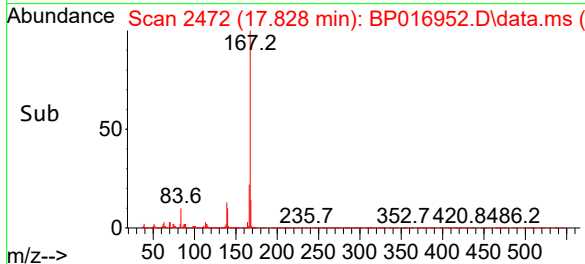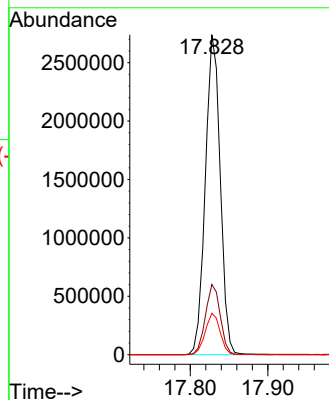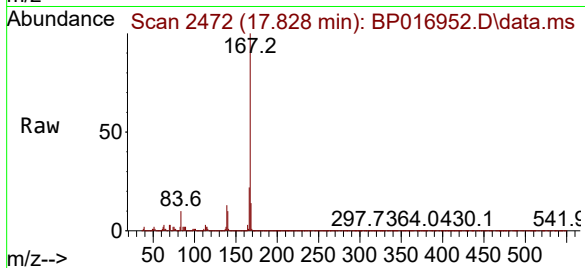

#78

Di-n-butylphthalate

Concen: 41.290 ng/ul

RT: 18.339 min Scan# 2559

Delta R.T. 0.000 min

Lab File: BP016952.D

Acq: 05 Sep 2023 13:15




Tgt Ion:149 Resp: 4558078


Ion Ratio Lower Upper

149 100

150 9.4 7.4 11.2

104 5.3 4.2 6.4

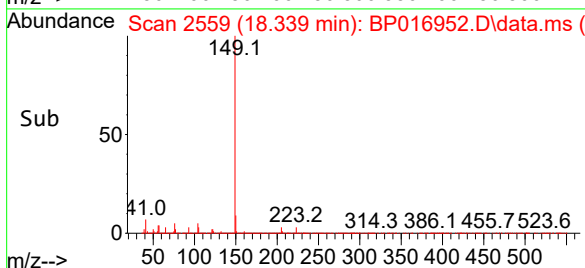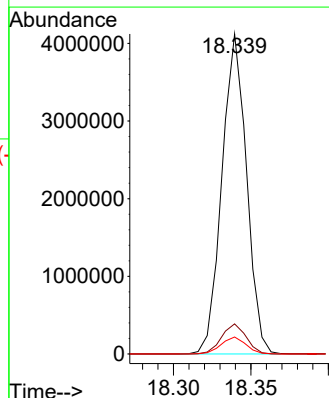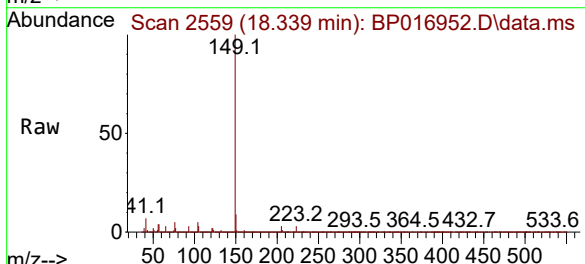



#80

Fluoranthene

Concen: 42.847 ng/ul

RT: 19.416 min Scan# 21

Delta R.T. 0.000 min

Lab File: BP016952.D

Acq: 05 Sep 2023 13:15

Instrument :

BNA_P

ClientSampleId :

SSTD040648





Tgt Ion:202 Resp: 4384633

Ion Ratio Lower Upper

202 100

101 12.6 10.0 15.0

100 9.5 7.5 11.3

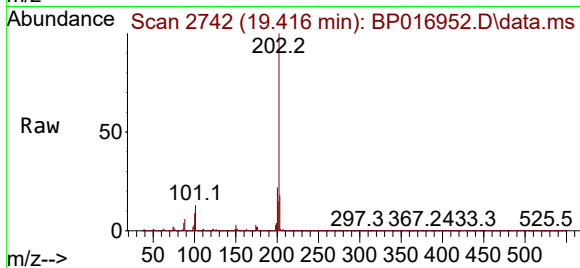

#82

Pyrene

Concen: 42.603 ng/ul

RT: 19.775 min Scan# 2803

Delta R.T. 0.000 min

Lab File: BP016952.D

Acq: 05 Sep 2023 13:15




Tgt Ion:202 Resp: 4526560


Ion Ratio Lower Upper

202 100

101 14.4 11.3 16.9

100 11.7 9.4 14.0

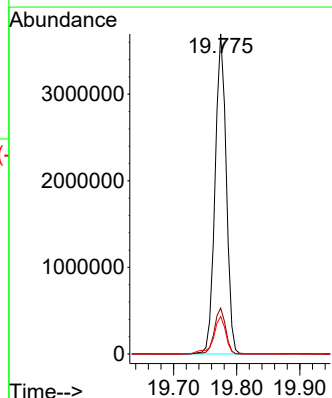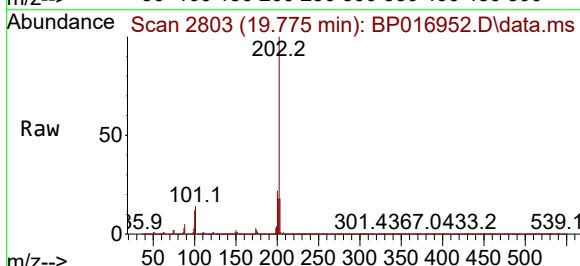



#83

Butylbenzylphthalate

Concen: 43.623 ng/ul

RT: 20.633 min Scan# 2949

Delta R.T. 0.000 min

Lab File: BP016952.D

Acq: 05 Sep 2023 13:15

Instrument :

BNA_P

ClientSampleId :

SSTD040648





Tgt Ion:149 Resp: 1916776

Ion Ratio Lower Upper

149 100

91 71.0 59.1 88.7

206 20.6 15.7 23.5

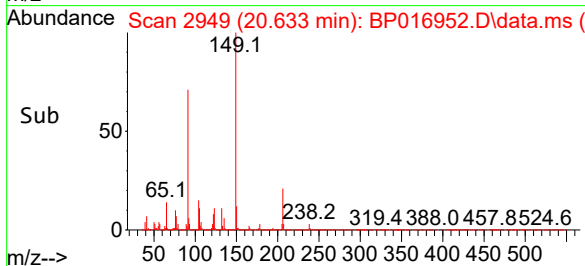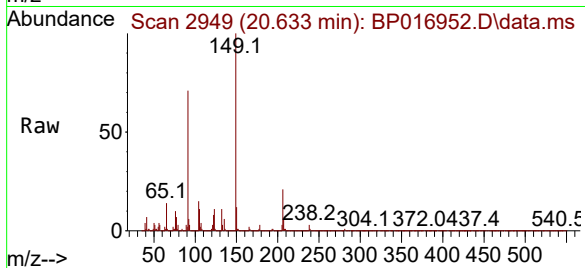

#84

3,3'-Dichlorobenzidine

Concen: 41.634 ng/ul

RT: 21.428 min Scan# 3084

Delta R.T. 0.000 min

Lab File: BP016952.D

Acq: 05 Sep 2023 13:15




Tgt Ion:252 Resp: 1243251


Ion Ratio Lower Upper

252 100

254 63.9 51.8 77.6

126 12.9 10.4 15.6


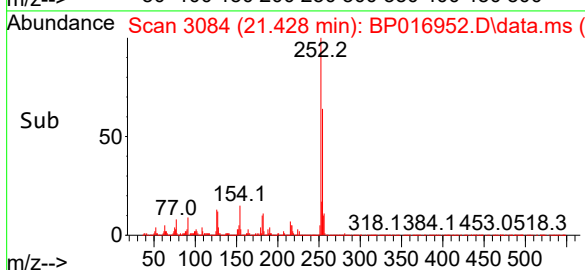

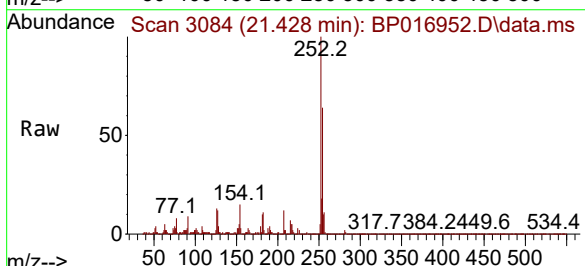




#85
Benzo(a)anthracene
Concen: 40.916 ng/ul
RT: 21.492 min Scan# 3095
Delta R.T. 0.000 min
Lab File: BP016952.D
Acq: 05 Sep 2023 13:15




Instrument :
BNA_P
ClientSampleId :
SSTD040648


Tgt Ion:228 Resp: 3877321
Ion Ratio Lower Upper
228 100
229 20.2 15.8 23.8
226 28.6 22.2 33.2

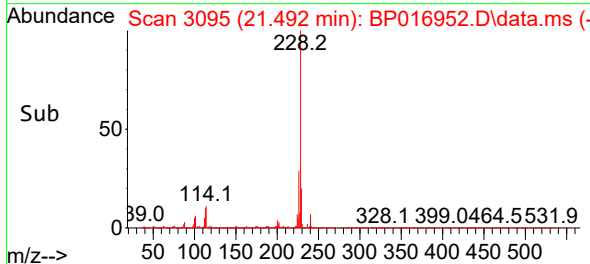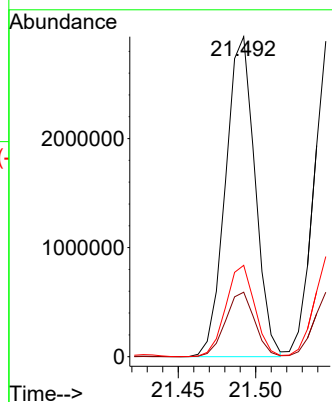

#86
Bis(2-ethylhexyl)phthalate
Concen: 42.718 ng/ul
RT: 21.369 min Scan# 3074
Delta R.T. 0.000 min
Lab File: BP016952.D
Acq: 05 Sep 2023 13:15

Tgt Ion:149 Resp: 2593099
Ion Ratio Lower Upper
149 100
167 27.0 21.4 32.2
279 3.9 3.0 4.4




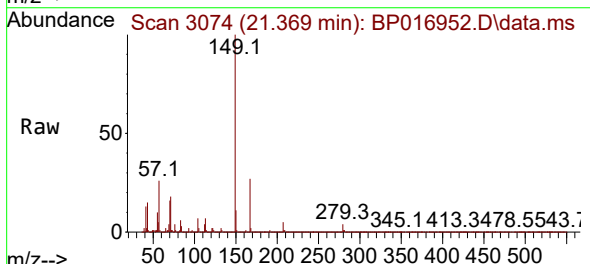




#87
Chrysene
Concen: 40.826 ng/ul
RT: 21.545 min Scan# 3104
Delta R.T. 0.000 min
Lab File: BP016952.D
Acq: 05 Sep 2023 13:15




Instrument :
BNA_P
ClientSampleId :
SSTD040648


Tgt Ion:228 Resp: 3618991
Ion Ratio Lower Upper
228 100
226 31.8 24.6 36.8
229 20.4 15.9 23.9



#89
Di-n-octyl phthalate
Concen: 43.325 ng/ul
RT: 22.339 min Scan# 3239
Delta R.T. 0.000 min
Lab File: BP016952.D
Acq: 05 Sep 2023 13:15

Tgt Ion:149 Resp: 3967518









#90
Benzo(b)fluoranthene
Concen: 42.678 ng/ul
RT: 23.257 min Scan# 31
Delta R.T. 0.000 min
Lab File: BP016952.D
Acq: 05 Sep 2023 13:15




Instrument :
BNA_P
ClientSampleId :
SSTD040648


Tgt Ion:252 Resp: 3257453
Ion Ratio Lower Upper
252 100
253 22.0 17.6 26.4
125 11.3 8.8 13.2

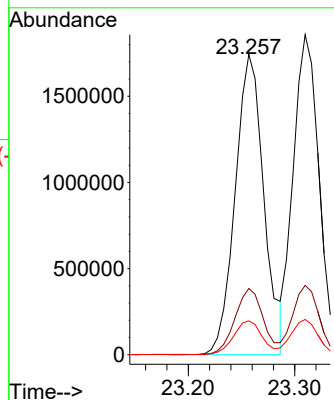

#91
Benzo(k)fluoranthene
Concen: 42.177 ng/ul
RT: 23.310 min Scan# 3404
Delta R.T. 0.000 min
Lab File: BP016952.D
Acq: 05 Sep 2023 13:15

Tgt Ion:252 Resp: 3117371
Ion Ratio Lower Upper
252 100
253 21.6 17.7 26.5
125 11.0 8.9 13.3

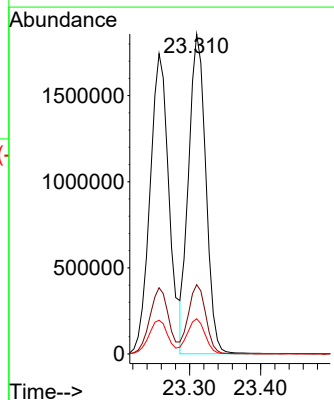



#93

Benzo(a)pyrene

Concen: 41.962 ng/ul

RT: 23.933 min Scan# 3510

Delta R.T. 0.000 min

Lab File: BP016952.D

Acq: 05 Sep 2023 13:15

Instrument :

BNA_P

ClientSampleId :

SSTD040648





Tgt Ion:252 Resp: 2671321

Ion Ratio Lower Upper

252 100

253 22.0 17.8 26.6

125 12.1 9.9 14.9

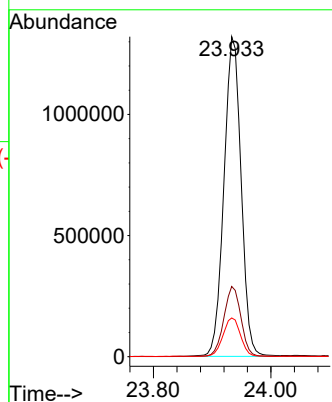

#94

Indeno(1,2,3-cd)pyrene

Concen: 39.244 ng/ul

RT: 26.745 min Scan# 3988

Delta R.T. 0.000 min

Lab File: BP016952.D

Acq: 05 Sep 2023 13:15




Tgt Ion:276 Resp: 2773255


Ion Ratio Lower Upper

276 100

138 26.5 21.4 32.0

277 24.6 20.0 30.0





#95

Dibenzo(a,h)anthracene

Concen: 39.316 ng/ul

RT: 26.774 min Scan# 3992

Delta R.T. 0.006 min

Lab File: BP016952.D

Acq: 05 Sep 2023 13:15

Instrument :

BNA_P

ClientSampleId :

SSTD040648





Tgt Ion:278 Resp: 2293159

Ion Ratio Lower Upper

278 100

139 18.5 14.9 22.3

279 24.4 19.6 29.4

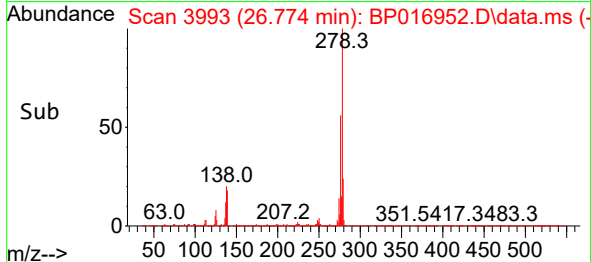

#96

Benzo(g,h,i)perylene

Concen: 38.701 ng/ul

RT: 27.592 min Scan# 4132

Delta R.T. 0.000 min

Lab File: BP016952.D

Acq: 05 Sep 2023 13:15

Tgt Ion:276 Resp: 2155175

Ion Ratio Lower Upper

276 100

138 25.2 19.5 29.3

277 23.5 18.7 28.1

