

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090623\
 Data File : BP016962.D
 Acq On : 06 Sep 2023 19:36
 Operator : MA/JU
 Sample : 04148-13
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBJW9

Quant Time: Sep 06 22:17:00 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 06 01:52:05 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.981	152	499759	20.000	ng/ul	0.00
20) Naphthalene-d8	10.810	136	2200074	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.640	164	1374813	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.410	188	2968725	20.000	ng/ul	0.00
79) Chrysene-d12	21.504	240	2475532	20.000	ng/ul	0.00
88) Perylene-d12	24.051	264	2289027	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.328	96	52312	3.959	ng/uL	0.00
4) Pyridine-d5	3.770	84	281627	7.460	ng/ul	0.00
7) Phenol-d5	7.128	99	302314	6.621	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.322	67	935047	32.741	ng/ul	0.00
11) 2-Chlorophenol-d4	7.499	132	839958	25.419	ng/ul	0.00
15) 4-Methylphenol-d8	8.687	113	596998	17.163	ng/ul	0.00
21) Nitrobenzene-d5	9.181	128	577240	33.819	ng/ul	0.00
24) 2-Nitrophenol-d4	9.893	143	606371	32.773	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.422	165	1055320	30.895	ng/ul	0.00
31) 4-Chloroaniline-d4	10.969	131	465196	9.439	ng/ul	0.00
46) Dimethylphthalate-d6	14.057	166	4189415	40.937	ng/ul	0.00
49) Acenaphthylene-d8	14.340	160	4342057	36.765	ng/ul	0.00
54) 4-Nitrophenol-d4	14.857	143	139876	6.997	ng/ul	0.00
60) Fluorene-d10	15.640	176	3442734	39.292	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.763	200	672641	37.650	ng/ul	0.00
73) Anthracene-d10	17.510	188	5669770	41.587	ng/ul	0.00
81) Pyrene-d10	19.745	212	6464459	42.872	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.886	264	5071745	43.674	ng/ul	0.00


Target Compounds					Qvalue
2) 1,4-Dioxane	3.364	88	18411	1.291 ng/uL#	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090623\
Data File : BP016962.D
Acq On : 06 Sep 2023 19:36
Operator : MA/JU
Sample : 04148-13
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJW9

Quant Time: Sep 06 22:17:00 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 06 01:52:05 2023
Response via : Initial Calibration

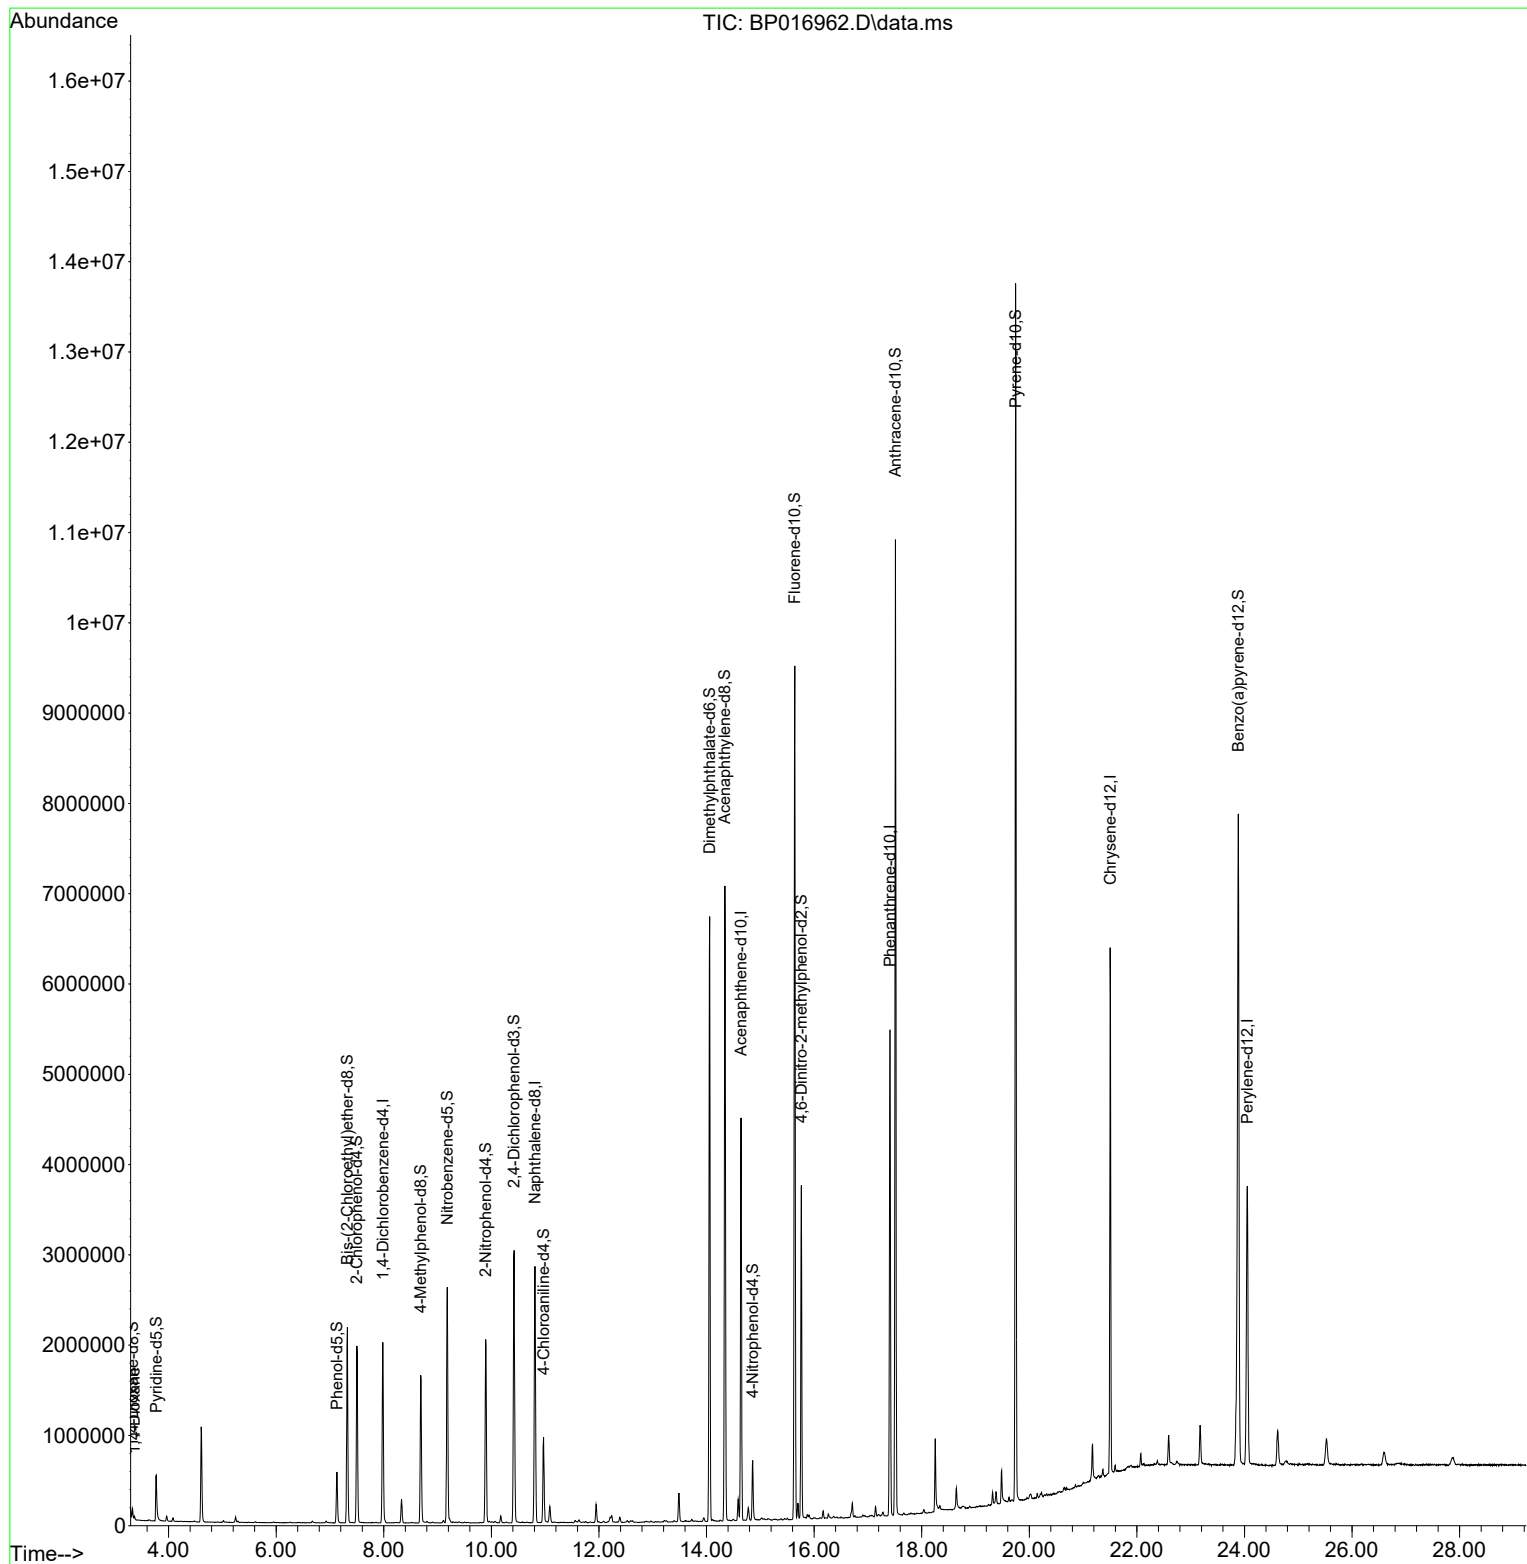

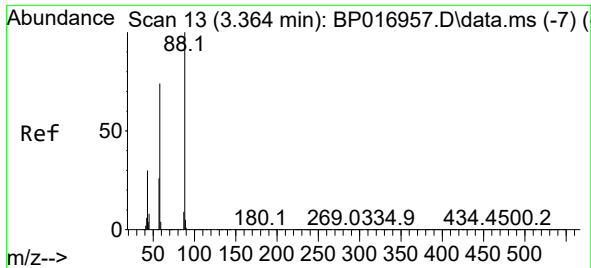

#2
1,4-Dioxane
Concen: 1.291 ng/uL
RT: 3.364 min Scan# 11
Delta R.T. 0.001 min
Lab File: BP016962.D
Acq: 06 Sep 2023 19:36

Instrument :
BNA_P
ClientSampleId :
BBJW9

Tgt Ion: 88 Resp: 18411
Ion Ratio Lower Upper
88 100
43 38.9 25.0 37.6#
58 76.3 60.6 90.8

