

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090623\
 Data File : BP016966.D
 Acq On : 06 Sep 2023 21:54
 Operator : MA/JU
 Sample : 04148-17
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBK25

Quant Time: Sep 06 22:46:36 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 06 01:52:05 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.981	152	492137	20.000	ng/ul	0.00
20) Naphthalene-d8	10.810	136	2142834	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.640	164	1340010	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.404	188	2847363	20.000	ng/ul	0.00
79) Chrysene-d12	21.504	240	2268093	20.000	ng/ul	0.00
88) Perylene-d12	24.045	264	2118339	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.329	96	59984	4.610	ng/uL	0.00
4) Pyridine-d5	3.770	84	253935	6.831	ng/ul	0.00
7) Phenol-d5	7.128	99	312421	6.949	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.322	67	1030871	36.655	ng/ul	0.00
11) 2-Chlorophenol-d4	7.499	132	895695	27.525	ng/ul	0.00
15) 4-Methylphenol-d8	8.687	113	542292	15.832	ng/ul	0.00
21) Nitrobenzene-d5	9.181	128	628518	37.807	ng/ul	0.00
24) 2-Nitrophenol-d4	9.893	143	691167	38.353	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.416	165	1110331	33.373	ng/ul	0.00
31) 4-Chloroaniline-d4	10.969	131	435281	9.068	ng/ul	0.00
46) Dimethylphthalate-d6	14.051	166	4200120	42.108	ng/ul	0.00
49) Acenaphthylene-d8	14.340	160	4484212	38.954	ng/ul	0.00
54) 4-Nitrophenol-d4	14.851	143	141703	7.273	ng/ul	0.00
60) Fluorene-d10	15.634	176	3539580	41.446	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.763	200	628707	36.691	ng/ul	0.00
73) Anthracene-d10	17.510	188	5421000	41.457	ng/ul	0.00
81) Pyrene-d10	19.745	212	6175176	44.699	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.880	264	4712444	43.850	ng/ul	0.00
Target Compounds						
34) Caprolactam	11.810	113	242803	21.623	ng/ul	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090623\
Data File : BP016966.D
Acq On : 06 Sep 2023 21:54
Operator : MA/JU
Sample : 04148-17
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBK25

Quant Time: Sep 06 22:46:36 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 06 01:52:05 2023
Response via : Initial Calibration

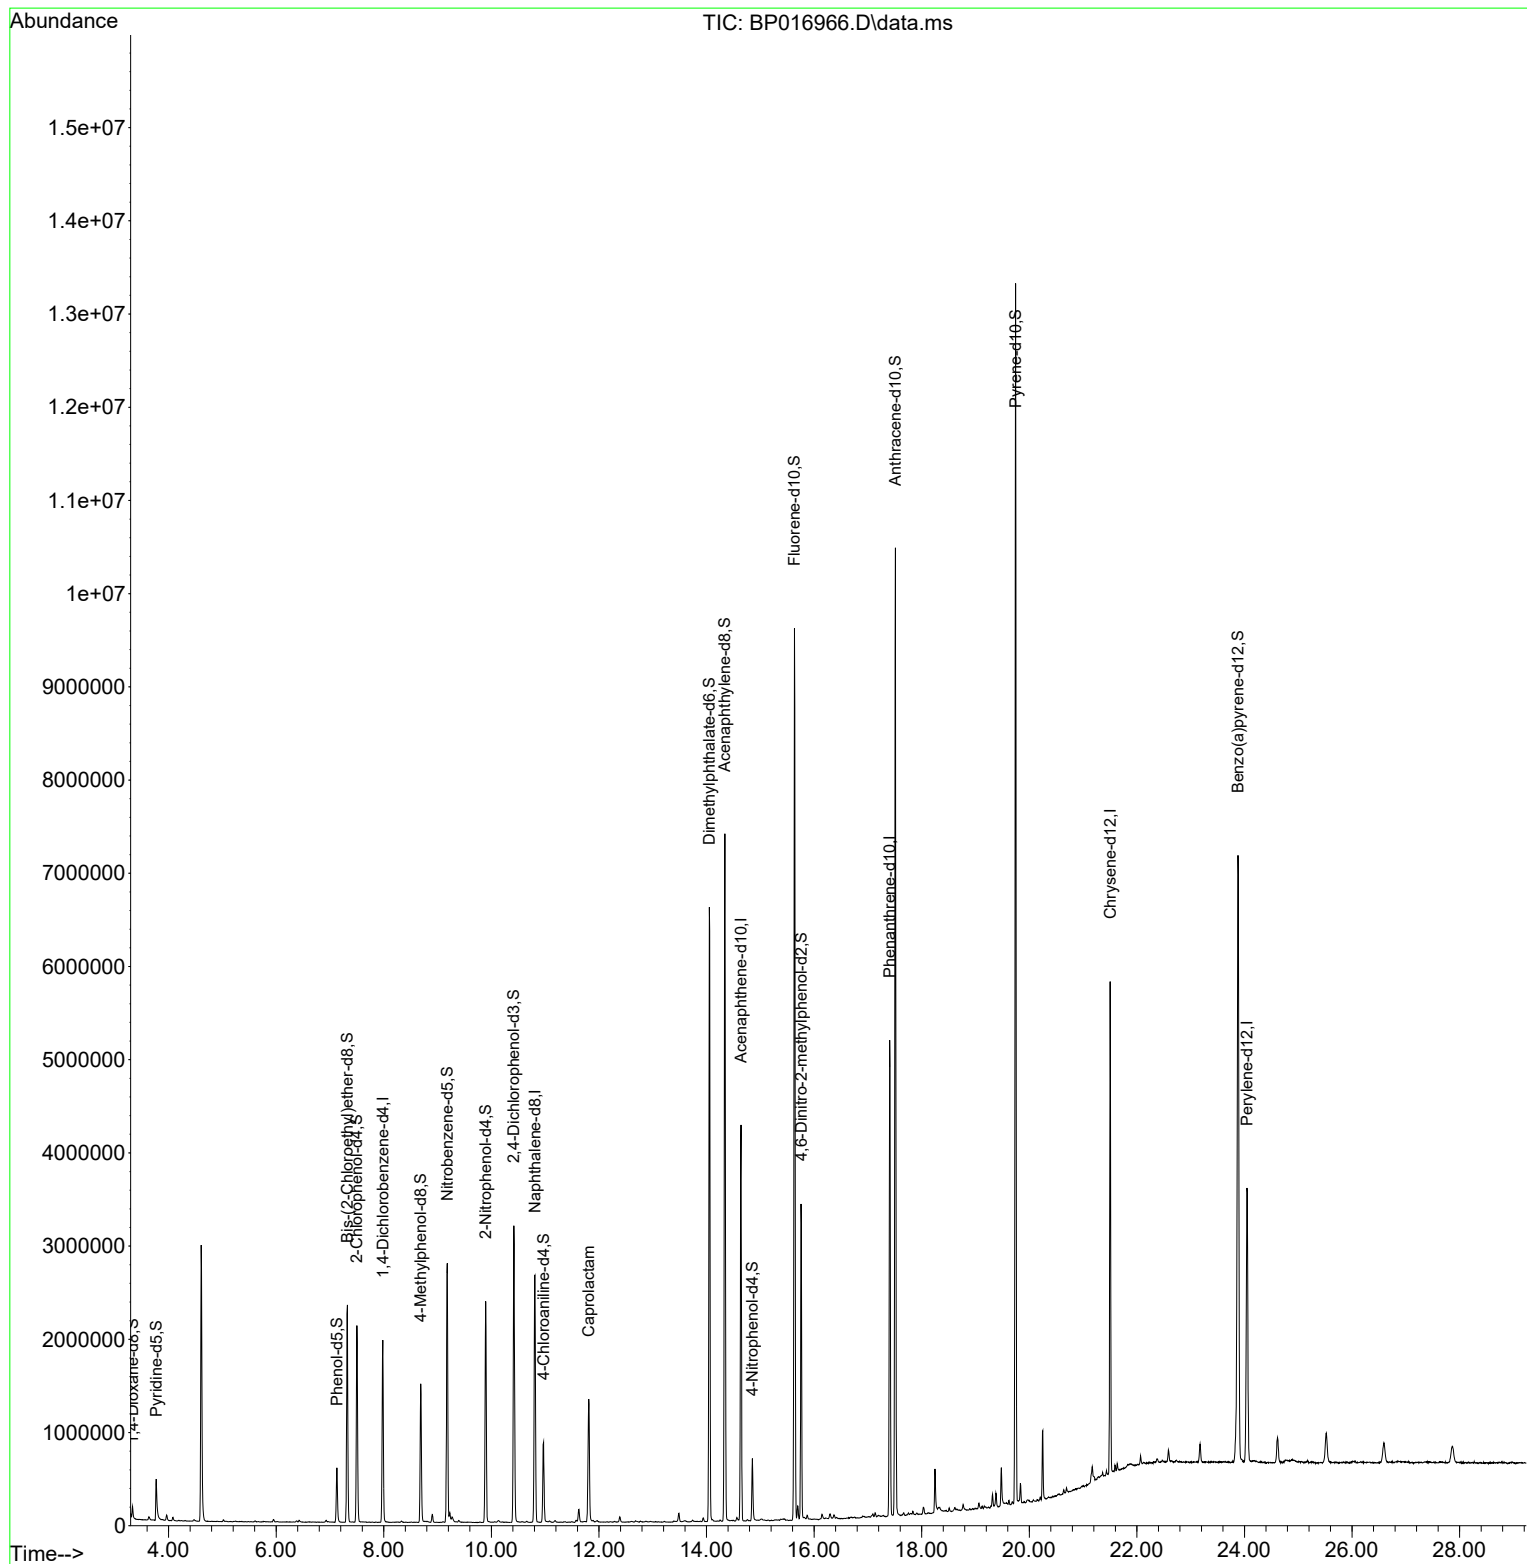

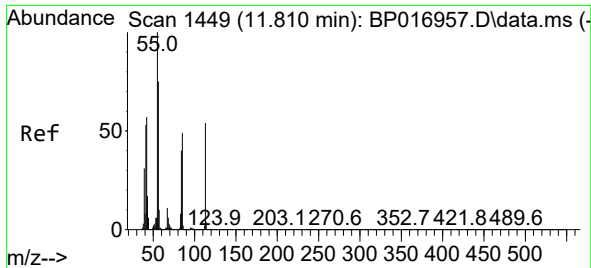

#34
Caprolactam
Concen: 21.623 ng/ul
RT: 11.810 min Scan# 1449
Delta R.T. 0.000 min
Lab File: BP016966.D
Acq: 06 Sep 2023 21:54

Instrument :
BNA_P
ClientSampleId :
BBK25

Tgt Ion:113 Resp: 242803
Ion Ratio Lower Upper
113 100
55 185.8 142.3 213.5
56 132.0 102.2 153.2

