

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090623\
 Data File : BP016965.D
 Acq On : 06 Sep 2023 21:20
 Operator : MA/JU
 Sample : 04148-16
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBK16

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016965.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.328	3	7	12	rBV	125893	163823	0.98%	0.108%
2	3.770	78	82	96	rBV	400749	642564	3.85%	0.422%
3	3.964	109	115	124	rVB	65435	108675	0.65%	0.071%
4	4.081	130	135	142	rBV	47762	69881	0.42%	0.046%
5	4.470	198	201	210	rVB5	10544	21021	0.13%	0.014%
6	5.023	291	295	300	rBV	17834	24988	0.15%	0.016%
7	5.605	388	394	401	rBV4	10304	19335	0.12%	0.013%
8	6.922	615	618	623	rBV3	13163	23558	0.14%	0.015%
9	7.128	646	653	666	rBV	551791	856559	5.13%	0.562%
10	7.322	678	686	700	rBV	2441331	3801930	22.79%	2.496%
11	7.499	709	716	726	rBV	2180831	3411284	20.45%	2.240%
12	7.981	789	798	810	rBV	2165696	3323588	19.92%	2.182%
13	8.687	911	918	931	rBV	1619683	2607576	15.63%	1.712%
14	9.181	993	1002	1016	rBV	2947366	4800287	28.77%	3.152%
15	9.393	1033	1038	1045	rVB	14032	23746	0.14%	0.016%
16	9.893	1115	1123	1139	rBV	2360294	3819576	22.89%	2.508%
17	10.016	1139	1144	1149	rVV	21713	39260	0.24%	0.026%
18	10.416	1204	1212	1231	rBV	3162641	5253027	31.48%	3.449%
19	10.810	1270	1279	1291	rBV	3003259	4921626	29.50%	3.232%
20	10.969	1297	1306	1318	rBV	1340832	2247882	13.47%	1.476%
21	11.493	1388	1395	1401	rBV5	10293	17828	0.11%	0.012%
22	11.557	1401	1406	1412	rVV8	12862	25048	0.15%	0.016%
23	12.387	1541	1547	1559	rBV2	56846	104917	0.63%	0.069%
24	13.393	1714	1718	1726	rBV3	18333	29689	0.18%	0.019%
25	13.481	1726	1733	1740	rBV2	57252	122793	0.74%	0.081%
26	13.604	1748	1754	1760	rVB4	10076	17473	0.10%	0.011%
27	14.051	1821	1830	1843	rBV	6586255	9027083	54.10%	5.928%
28	14.340	1872	1879	1888	rBV	7487178	10694359	64.10%	7.022%
29	14.640	1923	1930	1939	rVB	4617892	6515814	39.05%	4.279%
30	14.757	1947	1950	1960	rBV	12830	29473	0.18%	0.019%
31	14.851	1960	1966	1979	rVV	500353	769098	4.61%	0.505%
32	15.022	1989	1995	2001	rBV9	12681	33677	0.20%	0.022%
33	15.381	2051	2056	2060	rVB2	14203	20570	0.12%	0.014%
34	15.457	2060	2069	2075	rVB5	9419	22538	0.14%	0.015%
35	15.634	2091	2099	2108	rBV	9385187	13516580	81.01%	8.875%
36	15.757	2114	2120	2131	rBV	3384332	4656771	27.91%	3.058%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090623\
 Data File : BP016965.D
 Acq On : 06 Sep 2023 21:20
 Operator : MA/JU
 Sample : 04148-16
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBK16

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
 Title : SVOA CALIBRATION

37	15.869	2135	2139	2151	rVB	46886	92440	0.55%	0.061%
38	16.363	2218	2223	2229	rVB5	22219	38331	0.23%	0.025%
39	17.069	2340	2343	2351	rVB6	13759	26321	0.16%	0.017%
40	17.410	2394	2401	2411	rBV	5551437	7784874	46.66%	5.112%
41	17.510	2411	2418	2432	rVV	10786161	14828542	88.88%	9.737%
42	17.663	2441	2444	2450	rVB2	14311	21607	0.13%	0.014%
43	18.034	2504	2507	2511	rBV6	18027	21718	0.13%	0.014%
44	18.245	2539	2543	2552	rBV	236697	336133	2.01%	0.221%
45	18.339	2556	2559	2566	rVB	27418	39666	0.24%	0.026%
46	18.645	2607	2611	2620	rBV	79586	147328	0.88%	0.097%
47	19.316	2721	2725	2729	rBV	128739	154728	0.93%	0.102%
48	19.381	2732	2736	2742	rVB	121265	175015	1.05%	0.115%
49	19.481	2749	2753	2762	rBV	173374	262037	1.57%	0.172%
50	19.622	2774	2777	2780	rVB3	42434	45403	0.27%	0.030%
51	19.745	2792	2798	2804	rBV	13061405	16684564	100.00%	10.956%
52	21.504	3092	3097	3107	rBV	5892140	7617896	45.66%	5.002%
53	23.886	3492	3502	3514	rVB	7181364	15136737	90.72%	9.939%
54	24.045	3522	3529	3538	rVB	3429167	7094053	42.52%	4.658%




Sum of corrected areas: 152291290

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090623\
Data File : BP016965.D
Acq On : 06 Sep 2023 21:20
Operator : MA/JU
Sample : 04148-16
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBK16

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

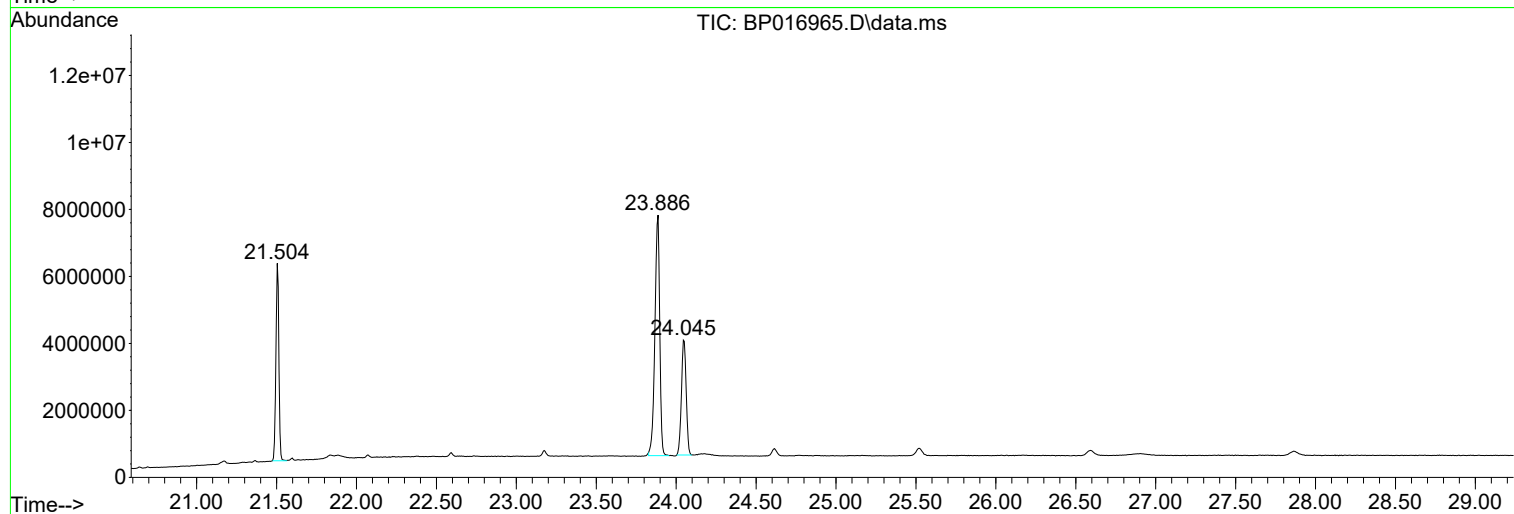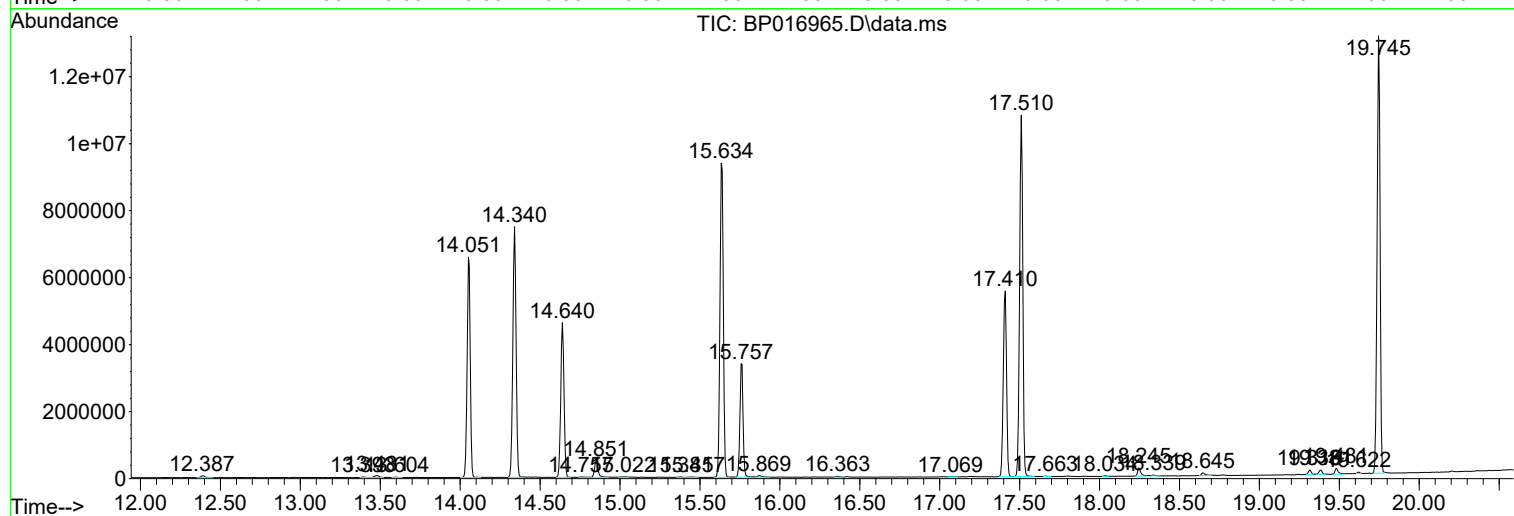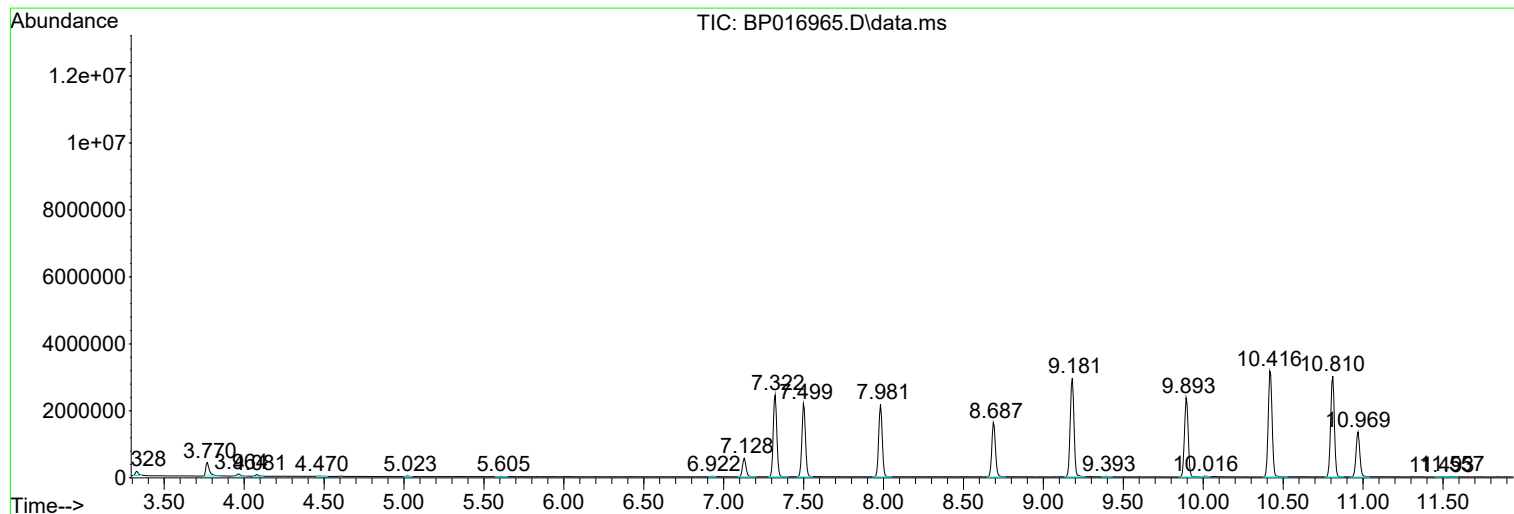

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090623\
Data File : BP016965.D
Acq On : 06 Sep 2023 21:20
Operator : MA/JU
Sample : 04148-16
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBK16

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090623\
Data File : BP016965.D
Acq On : 06 Sep 2023 21:20
Operator : MA/JU
Sample : 04148-16
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBK16

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------