

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090723\
 Data File : BP016999.D
 Acq On : 07 Sep 2023 21:38
 Operator : MA/JU
 Sample : 04123-16
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHAL9

Quant Time: Sep 08 00:41:19 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 06 01:52:05 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.975	152	318060	20.000	ng/ul	0.00
20) Naphthalene-d8	10.804	136	1401469	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.634	164	871515	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.404	188	1880705	20.000	ng/ul	0.00
79) Chrysene-d12	21.498	240	1520328	20.000	ng/ul	-0.01
88) Perylene-d12	24.039	264	1521364	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.328	96	52108	6.197	ng/uL	0.00
4) Pyridine-d5	3.770	84	129594	5.394	ng/ul	0.00
7) Phenol-d5	7.128	99	225133	7.748	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.316	67	740708	40.752	ng/ul	0.00
11) 2-Chlorophenol-d4	7.499	132	637470	30.312	ng/ul	0.00
15) 4-Methylphenol-d8	8.687	113	426710	19.276	ng/ul	0.00
21) Nitrobenzene-d5	9.175	128	434126	39.928	ng/ul	0.00
24) 2-Nitrophenol-d4	9.893	143	442071	37.508	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.416	165	731657	33.625	ng/ul	0.00
31) 4-Chloroaniline-d4	10.963	131	845616	26.936	ng/ul	0.00
46) Dimethylphthalate-d6	14.051	166	2752792	42.433	ng/ul	0.00
49) Acenaphthylene-d8	14.334	160	3030912	40.483	ng/ul	0.00
54) 4-Nitrophenol-d4	14.845	143	78720	6.212	ng/ul	-0.01
60) Fluorene-d10	15.634	176	2397586	43.166	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.757	200	360032	31.811	ng/ul	0.00
73) Anthracene-d10	17.504	188	4046653	46.853	ng/ul	0.00
81) Pyrene-d10	19.739	212	4491120	48.499	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.874	264	3750997	48.600	ng/ul	0.00


Target Compounds					Qvalue
35) 4-Chloro-3-methylphenol	12.087	107	46525	1.915 ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090723\
Data File : BP016999.D
Acq On : 07 Sep 2023 21:38
Operator : MA/JU
Sample : 04123-16
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHAL9

Quant Time: Sep 08 00:41:19 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 06 01:52:05 2023
Response via : Initial Calibration

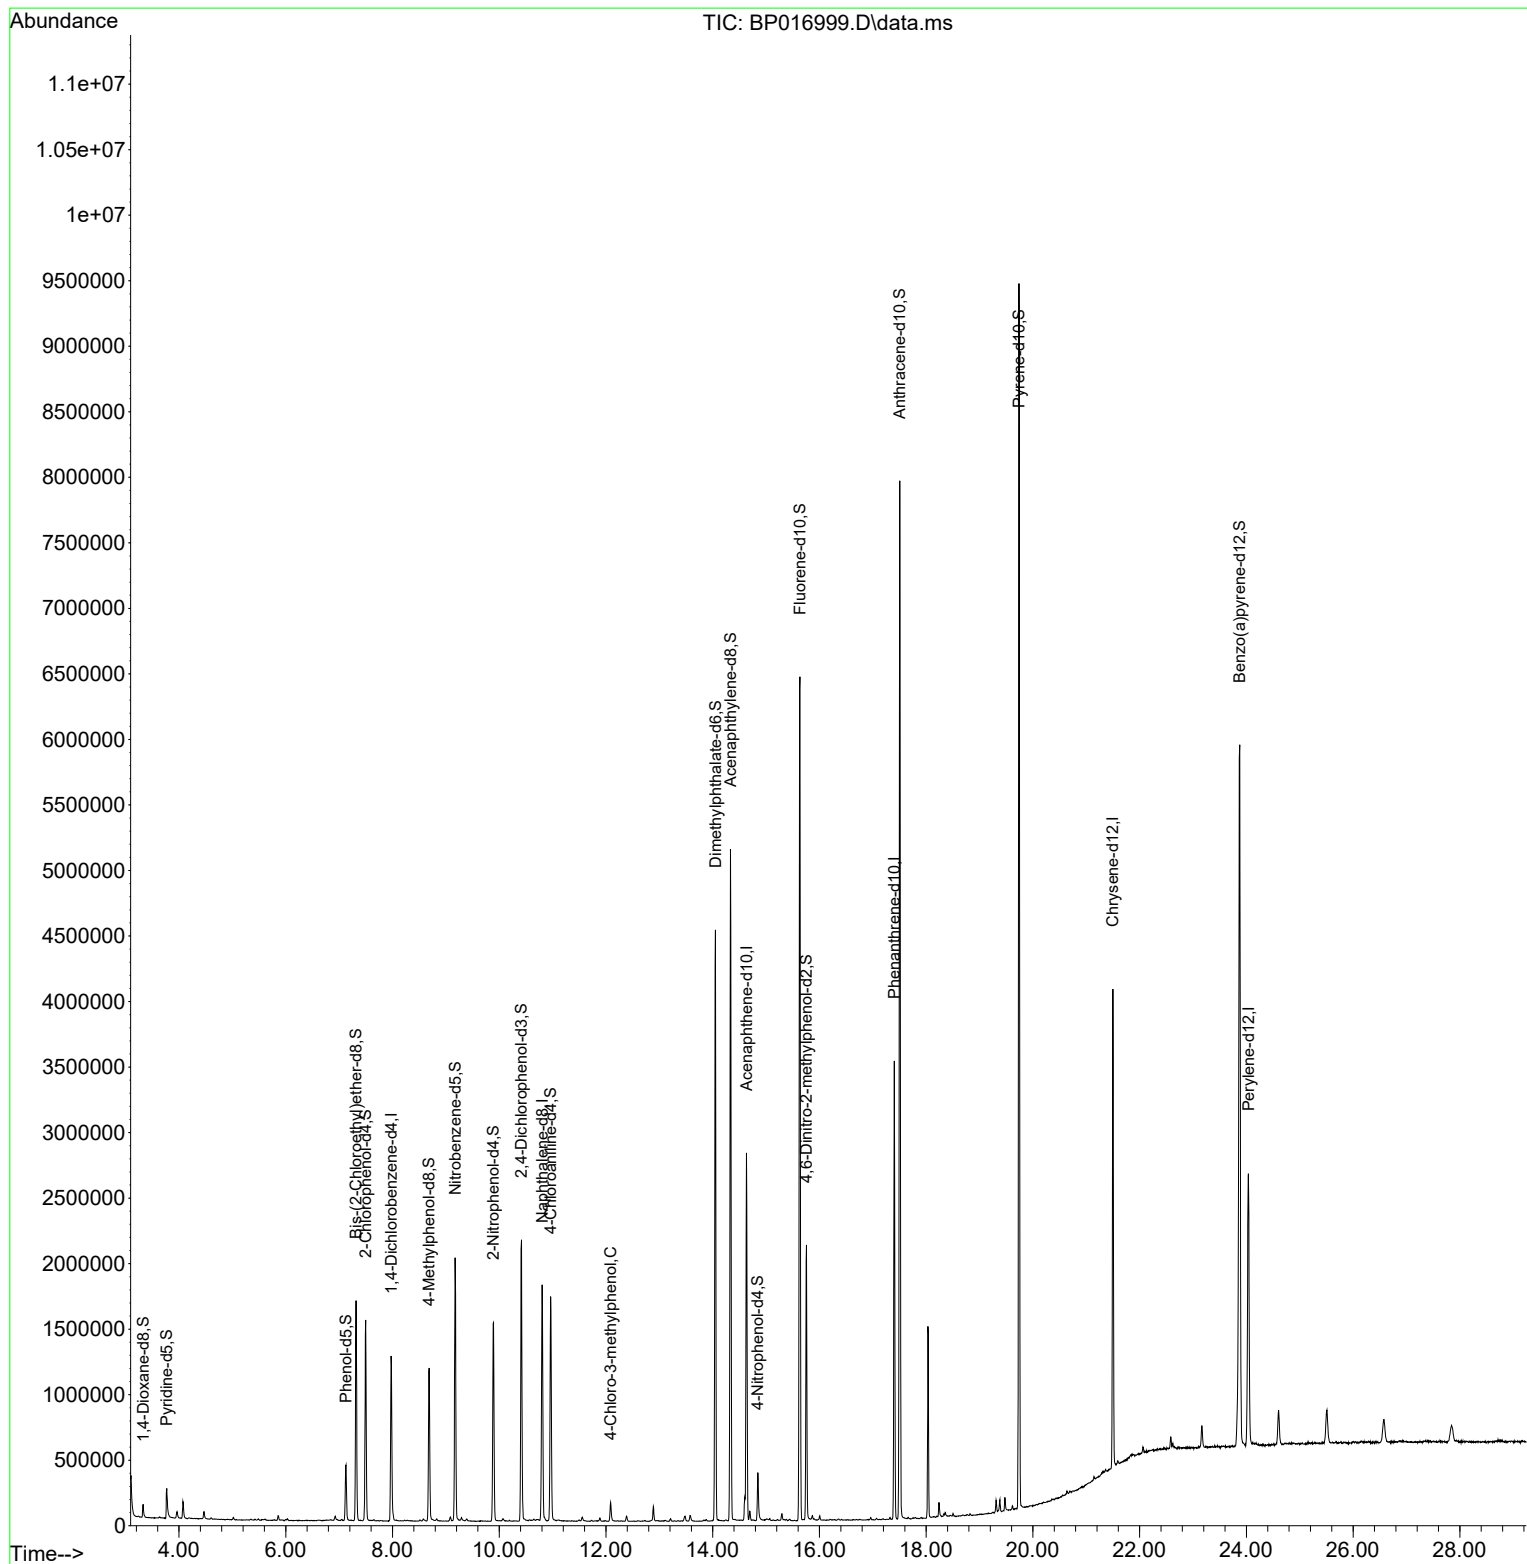

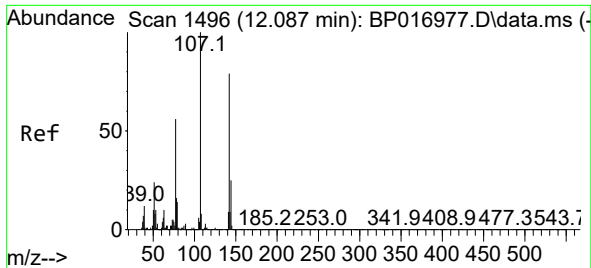

#35
 4-Chloro-3-methylphenol
 Concen: 1.915 ng/ul
 RT: 12.087 min Scan# 11
 Delta R.T. -0.006 min
 Lab File: BP016999.D
 Acq: 07 Sep 2023 21:38

Instrument :
 BNA_P
 ClientSampleId :
 BHAL9

Tgt Ion:	107	Resp:	46525
Ion	Ratio	Lower	Upper
107	100		
144	25.8	20.3	30.5
142	81.3	63.8	95.8

