

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090723\
 Data File : BP017002.D
 Acq On : 07 Sep 2023 23:21
 Operator : MA/JU
 Sample : 04166-17
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBJX4

Quant Time: Sep 08 00:41:51 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 06 01:52:05 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.975	152	330106	20.000	ng/ul	0.00
20) Naphthalene-d8	10.804	136	1440791	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.634	164	886316	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.404	188	1922430	20.000	ng/ul	0.00
79) Chrysene-d12	21.498	240	1588649	20.000	ng/ul	-0.01
88) Perylene-d12	24.033	264	1582242	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.328	96	60259	6.905	ng/uL	0.00
4) Pyridine-d5	3.764	84	285420	11.446	ng/ul	0.00
7) Phenol-d5	7.122	99	314228	10.419	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.316	67	872443	46.249	ng/ul	0.00
11) 2-Chlorophenol-d4	7.499	132	800819	36.689	ng/ul	0.00
15) 4-Methylphenol-d8	8.687	113	559820	24.366	ng/ul	0.00
21) Nitrobenzene-d5	9.175	128	500840	44.807	ng/ul	0.00
24) 2-Nitrophenol-d4	9.893	143	531108	43.832	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.416	165	894056	39.967	ng/ul	0.00
31) 4-Chloroaniline-d4	10.963	131	1116607	34.597	ng/ul	0.00
46) Dimethylphthalate-d6	14.051	166	3112379	47.175	ng/ul	0.00
49) Acenaphthylene-d8	14.334	160	3442630	45.215	ng/ul	0.00
54) 4-Nitrophenol-d4	14.845	143	110380	8.565	ng/ul	-0.01
60) Fluorene-d10	15.628	176	2648093	46.880	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.757	200	444236	38.399	ng/ul	0.00
73) Anthracene-d10	17.504	188	4199570	47.568	ng/ul	0.00
81) Pyrene-d10	19.739	212	4806137	49.668	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.868	264	3954341	49.263	ng/ul	-0.01
Target Compounds						
34) Caprolactam	11.798	113	16825	2.228	ng/ul	Qvalue 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090723\
Data File : BP017002.D
Acq On : 07 Sep 2023 23:21
Operator : MA/JU
Sample : 04166-17
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJX4

Quant Time: Sep 08 00:41:51 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 06 01:52:05 2023
Response via : Initial Calibration

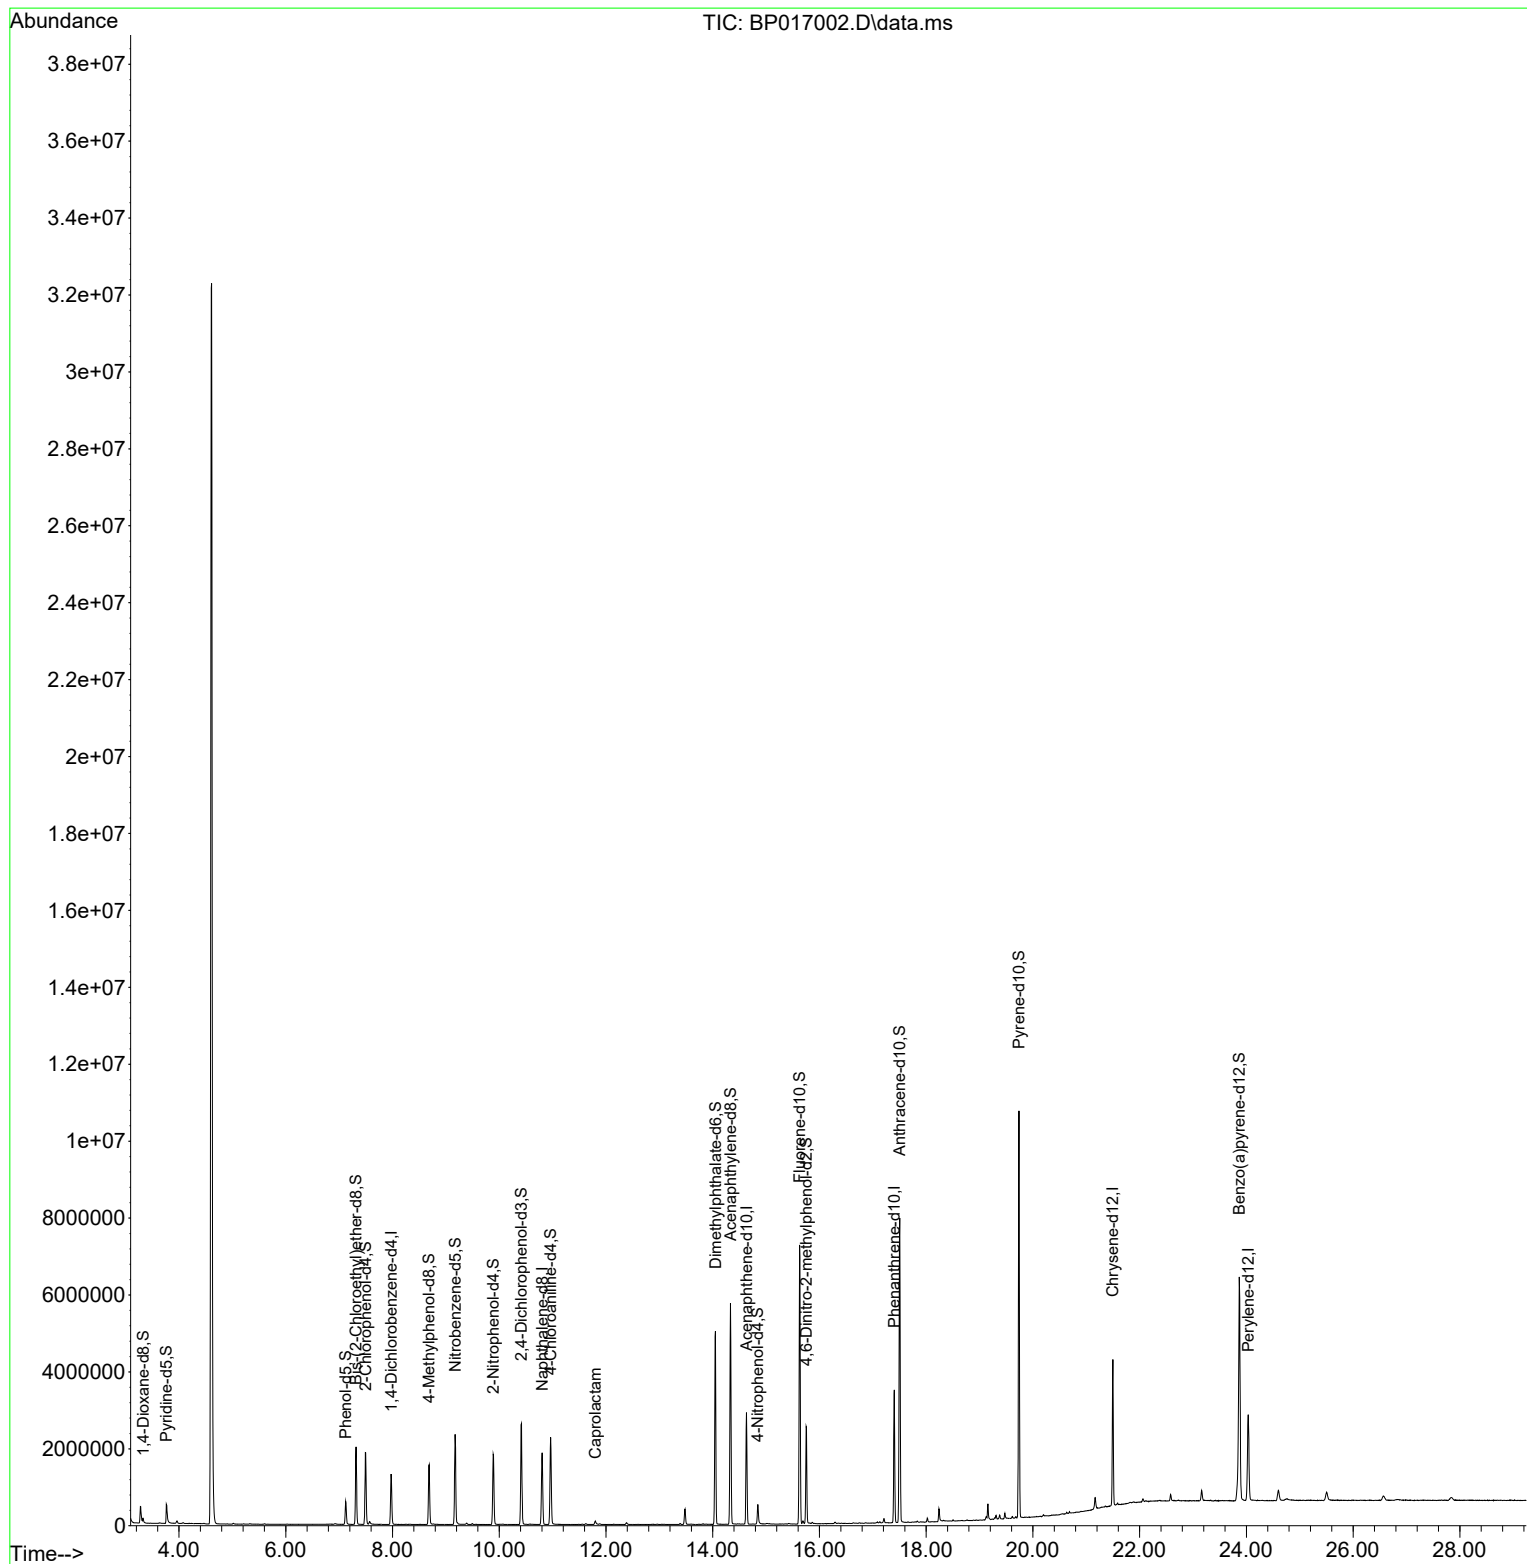

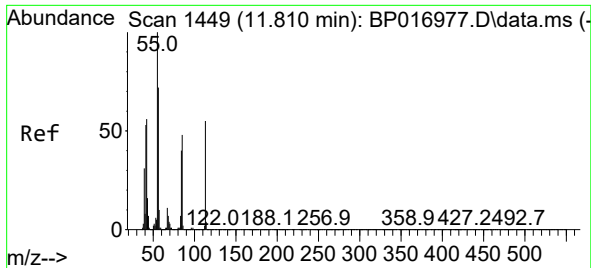

#34
Caprolactam
Concen: 2.228 ng/ul
RT: 11.798 min Scan# 14
Delta R.T. -0.011 min
Lab File: BP017002.D
Acq: 07 Sep 2023 23:21

Instrument :
BNA_P
ClientSampleId :
BBJX4

Tgt Ion:113 Resp: 16825
Ion Ratio Lower Upper
113 100
55 185.0 142.3 213.5
56 139.3 102.2 153.2

