

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090723\
 Data File : BP017000.D
 Acq On : 07 Sep 2023 22:12
 Operator : MA/JU
 Sample : 04123-17
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH9F9

Quant Time: Sep 08 01:34:31 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 06 01:52:05 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.975	152	390869	20.000	ng/ul	0.00
20) Naphthalene-d8	10.804	136	1713007	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.633	164	1050640	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.404	188	2209840	20.000	ng/ul	0.00
79) Chrysene-d12	21.498	240	1728663	20.000	ng/ul	-0.01
88) Perylene-d12	24.039	264	1670319	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.328	96	65809	6.369	ng/uL	0.00
4) Pyridine-d5	3.763	84	279237	9.457	ng/ul	0.00
7) Phenol-d5	7.122	99	304610	8.530	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.316	67	892364	39.951	ng/ul	0.00
11) 2-Chlorophenol-d4	7.498	132	792727	30.673	ng/ul	0.00
15) 4-Methylphenol-d8	8.687	113	554018	20.365	ng/ul	0.00
21) Nitrobenzene-d5	9.175	128	518449	39.011	ng/ul	0.00
24) 2-Nitrophenol-d4	9.892	143	541065	37.558	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.416	165	893536	33.596	ng/ul	0.00
31) 4-Chloroaniline-d4	10.963	131	1231771	32.101	ng/ul	0.00
46) Dimethylphthalate-d6	14.051	166	3084112	39.435	ng/ul	0.00
49) Acenaphthylene-d8	14.333	160	3515586	38.951	ng/ul	0.00
54) 4-Nitrophenol-d4	14.845	143	95785	6.270	ng/ul	-0.01
60) Fluorene-d10	15.633	176	2654170	39.638	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.757	200	411105	30.913	ng/ul	0.00
73) Anthracene-d10	17.504	188	4135345	40.748	ng/ul	0.00
81) Pyrene-d10	19.739	212	4489059	42.634	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.874	264	3549372	41.886	ng/ul	0.00
Target Compounds						
34) Caprolactam	11.798	113	20356	2.268	ng/ul	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090723\
Data File : BP017000.D
Acq On : 07 Sep 2023 22:12
Operator : MA/JU
Sample : 04123-17
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH9F9

Quant Time: Sep 08 01:34:31 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 06 01:52:05 2023
Response via : Initial Calibration

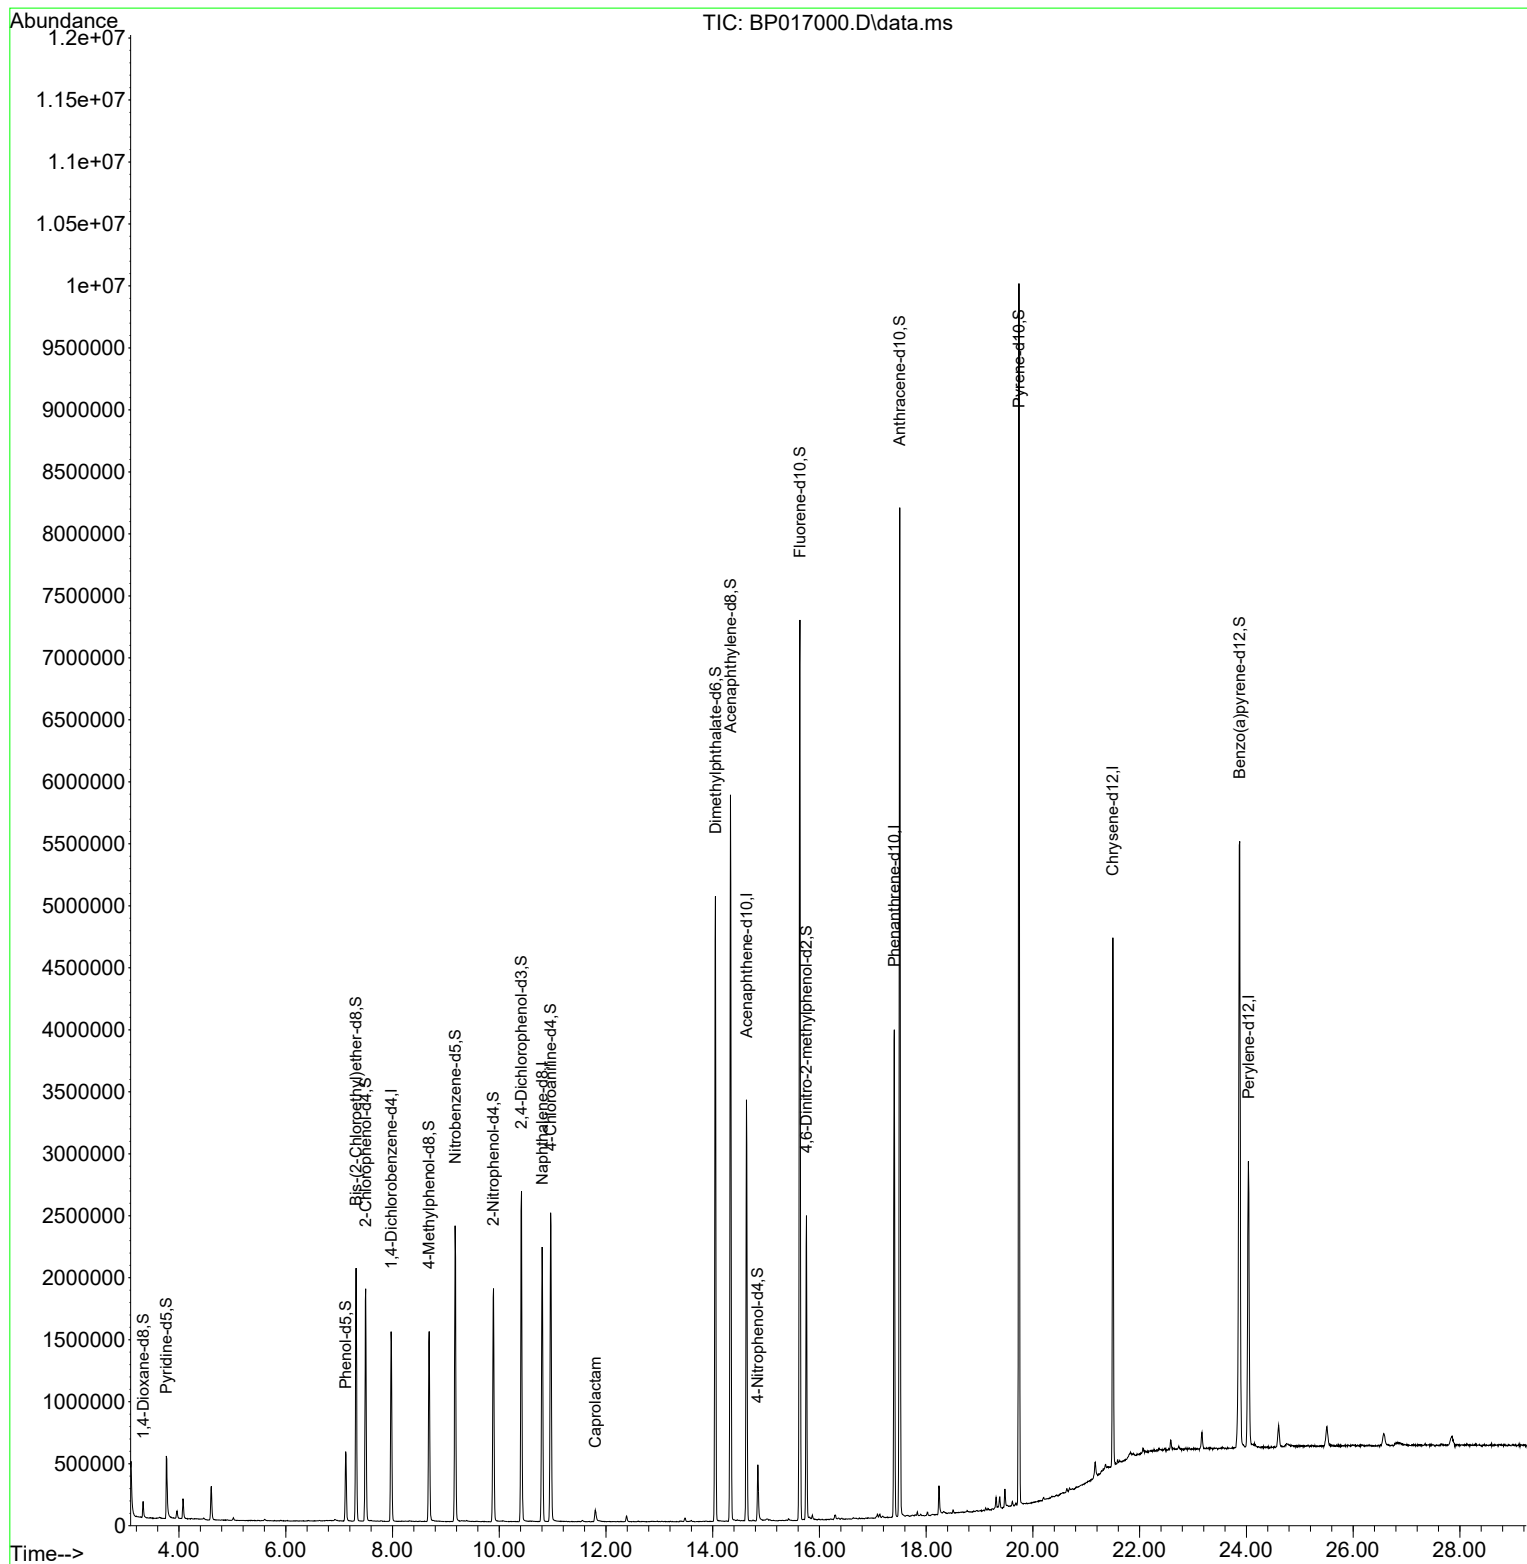

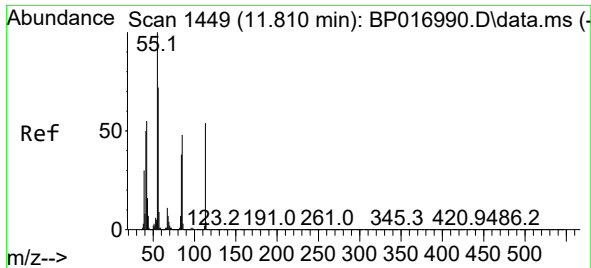

#34

Caprolactam

Concen: 2.268 ng/ul

RT: 11.798 min Scan# 14

Delta R.T. -0.012 min

Lab File: BP017000.D

Acq: 07 Sep 2023 22:12

Instrument :

BNA_P

ClientSampleId :

BH9F9

Tgt Ion:113 Resp: 20356

Ion Ratio Lower Upper

113 100

55 181.9 142.3 213.5

56 138.3 102.2 153.2

