

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090723\
 Data File : BP016985.D
 Acq On : 07 Sep 2023 13:30
 Operator : MA/JU
 Sample : 04148-16
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBK16

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016985.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.328	3	7	19	rVB	78480	121597	1.32%	0.146%
2	3.770	79	82	92	rBV	238693	388385	4.23%	0.465%
3	3.964	111	115	125	rVB2	40266	62572	0.68%	0.075%
4	4.075	131	134	141	rVB	26890	40971	0.45%	0.049%
5	4.605	221	224	228	rVB6	8849	12271	0.13%	0.015%
6	5.017	290	294	299	rBV2	13435	18895	0.21%	0.023%
7	5.605	388	394	399	rBV6	7471	13739	0.15%	0.016%
8	6.922	615	618	623	rBV6	7434	12546	0.14%	0.015%
9	7.128	646	653	665	rBV	295504	478662	5.21%	0.573%
10	7.317	676	685	695	rBV	1408009	2202861	23.97%	2.639%
11	7.499	710	716	726	rVB	1242862	1920321	20.90%	2.300%
12	7.981	790	798	809	rBV	1135605	1815194	19.75%	2.174%
13	8.687	911	918	929	rBV	904745	1455410	15.84%	1.743%
14	9.175	994	1001	1012	rBV	1682434	2698729	29.37%	3.233%
15	9.387	1034	1037	1042	rVB4	8065	12140	0.13%	0.015%
16	9.893	1115	1123	1134	rBV	1320381	2135653	23.24%	2.558%
17	10.005	1139	1142	1150	rVV5	12208	27008	0.29%	0.032%
18	10.069	1150	1153	1161	rVB9	7335	14193	0.15%	0.017%
19	10.416	1204	1212	1226	rBV	1868448	2997781	32.62%	3.591%
20	10.805	1269	1278	1288	rBV	1627903	2668073	29.03%	3.196%
21	10.963	1298	1305	1316	rBV	755087	1277705	13.90%	1.531%
22	11.493	1390	1395	1399	rBV8	7103	13229	0.14%	0.016%
23	11.557	1402	1406	1413	rVB10	5258	11193	0.12%	0.013%
24	12.387	1541	1547	1553	rBV2	31295	55729	0.61%	0.067%
25	12.963	1640	1645	1649	rBV8	4938	9778	0.11%	0.012%
26	13.393	1713	1718	1722	rBV5	11101	17061	0.19%	0.020%
27	13.475	1726	1732	1738	rBV3	27453	61562	0.67%	0.074%
28	14.051	1823	1830	1839	rBV	3823299	5094452	55.43%	6.103%
29	14.334	1872	1878	1889	rBV	4063318	5938501	64.62%	7.114%
30	14.640	1923	1930	1938	rBV	2344537	3504044	38.13%	4.197%
31	14.763	1947	1951	1955	rVB7	5884	9514	0.10%	0.011%
32	14.851	1959	1966	1977	rBV	214623	363911	3.96%	0.436%
33	15.028	1991	1996	2001	rVB8	8700	16978	0.18%	0.020%
34	15.381	2052	2056	2059	rVB5	9985	13926	0.15%	0.017%
35	15.445	2065	2067	2072	rVB4	8788	12823	0.14%	0.015%
36	15.634	2091	2099	2106	rBV	5558090	7662487	83.38%	9.179%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090723\
 Data File : BP016985.D
 Acq On : 07 Sep 2023 13:30
 Operator : MA/JU
 Sample : 04148-16
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBK16

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
 Title : SVOA CALIBRATION

37	15.757	2114	2120	2128	rBV	1766105	2264819	24.64%	2.713%
38	15.875	2135	2140	2144	rBV2	20558	28714	0.31%	0.034%
39	16.363	2220	2223	2228	rVB7	9756	15112	0.16%	0.018%
40	17.075	2340	2344	2350	rVB9	8575	14035	0.15%	0.017%
41	17.192	2359	2364	2367	rBV5	8203	14490	0.16%	0.017%
42	17.404	2393	2400	2411	rBV	2893899	4179918	45.48%	5.007%
43	17.510	2411	2418	2429	rBV	5957868	8362408	90.99%	10.017%
44	18.245	2539	2543	2549	rBV	108921	145373	1.58%	0.174%
45	18.651	2609	2612	2619	rBV5	26112	57511	0.63%	0.069%
46	19.316	2721	2725	2729	rBV2	70473	92466	1.01%	0.111%
47	19.386	2733	2737	2742	rVB	68712	95804	1.04%	0.115%
48	19.481	2749	2753	2760	rBV5	77484	118298	1.29%	0.142%
49	19.622	2775	2777	2781	rVB4	26980	27116	0.30%	0.032%
50	19.745	2792	2798	2804	rBV	7536866	9190156	100.00%	11.009%
51	21.504	3092	3097	3104	rBV	3003112	3907869	42.52%	4.681%
52	23.880	3493	3501	3520	rVB2	3775674	8129461	88.46%	9.738%
53	24.051	3523	3530	3541	rVB	1800319	3676833	40.01%	4.404%




Sum of corrected areas: 83480277

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090723\
Data File : BP016985.D
Acq On : 07 Sep 2023 13:30
Operator : MA/JU
Sample : 04148-16
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBK16

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

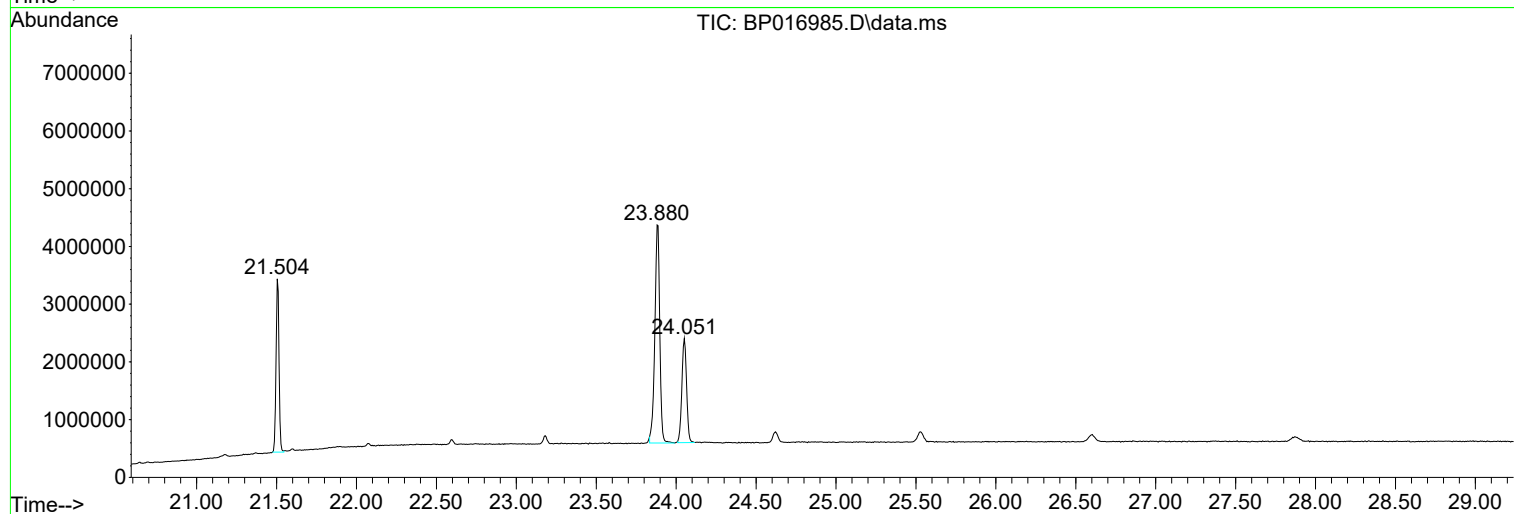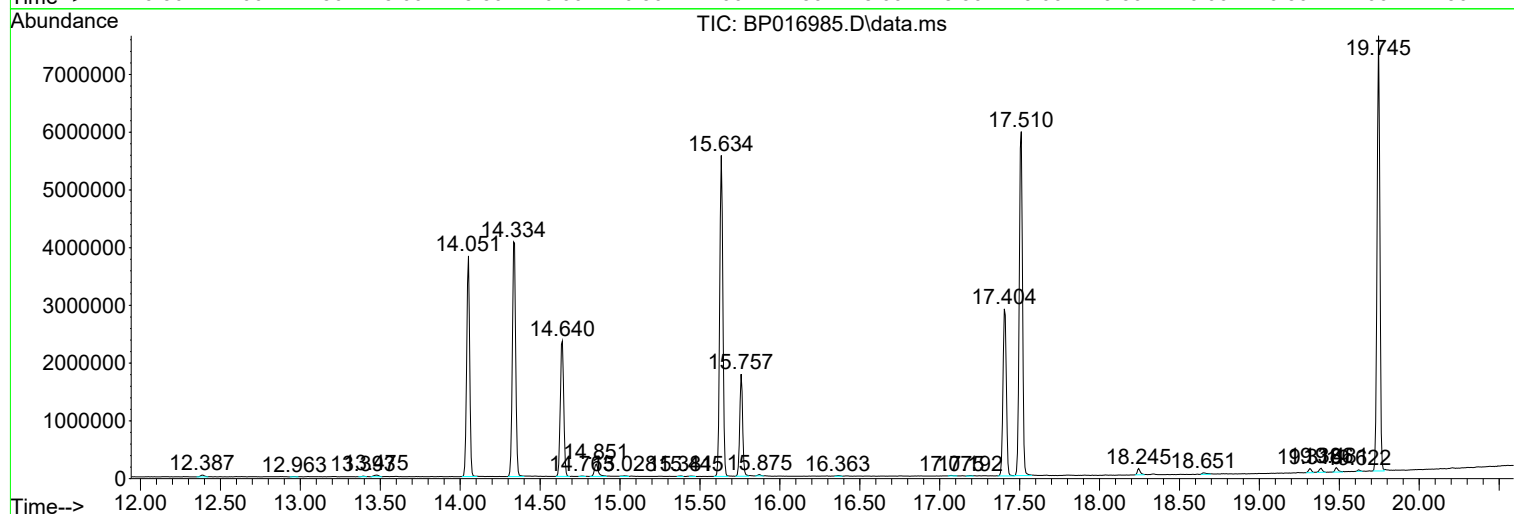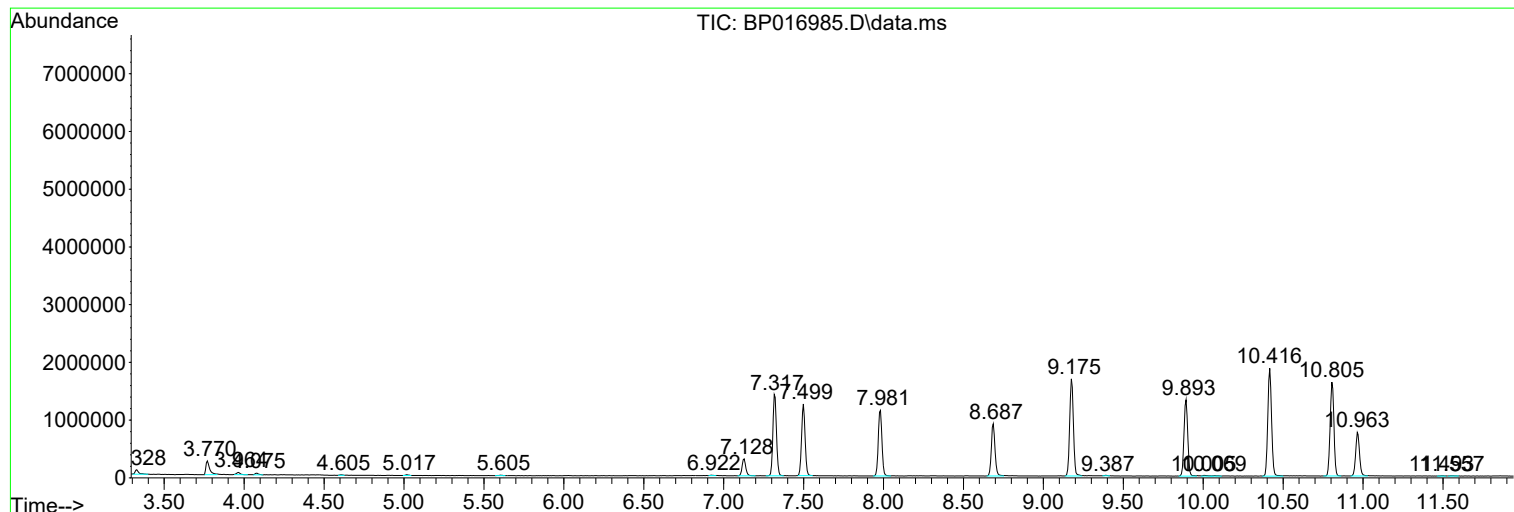

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090723\
Data File : BP016985.D
Acq On : 07 Sep 2023 13:30
Operator : MA/JU
Sample : 04148-16
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBK16

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090723\
Data File : BP016985.D
Acq On : 07 Sep 2023 13:30
Operator : MA/JU
Sample : 04148-16
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBK16

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc