

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090723\
 Data File : BP016991.D
 Acq On : 07 Sep 2023 17:00
 Operator : MA/JU
 Sample : PB155065BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK065

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016991.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.323	36	40	52	rVB	142655	201580	2.26%	0.211%
2	3.758	110	114	132	rBV	1477546	2349527	26.38%	2.454%
3	4.075	164	168	172	rBV	21644	29627	0.33%	0.031%
4	7.122	679	686	700	rBV	1716576	2720554	30.54%	2.841%
5	7.316	713	719	729	rBV	1459708	2180706	24.48%	2.278%
6	7.499	742	750	759	rBV	1679414	2641373	29.65%	2.759%
7	7.975	824	831	840	rBV	1332181	2109237	23.68%	2.203%
8	8.687	942	952	964	rBV	2030118	3264881	36.65%	3.410%
9	9.175	1025	1035	1048	rBV	1656806	2635724	29.59%	2.753%
10	9.893	1148	1157	1168	rBV	1321376	2177916	24.45%	2.275%
11	10.416	1238	1246	1257	rBV	1984807	3219914	36.15%	3.363%
12	10.804	1301	1312	1320	rBV	1911217	3109694	34.91%	3.248%
13	10.963	1332	1339	1352	rBV	1986662	3396930	38.14%	3.548%
14	12.387	1576	1581	1587	rBV	32026	49602	0.56%	0.052%
15	13.481	1762	1767	1772	rBV	25027	39864	0.45%	0.042%
16	13.593	1782	1786	1793	rVB8	7171	13181	0.15%	0.014%
17	14.051	1856	1864	1876	rBV	3771230	4954289	55.62%	5.174%
18	14.340	1905	1913	1928	rBV	3937962	5771200	64.79%	6.028%
19	14.640	1957	1964	1972	rBV	2847340	4144556	46.53%	4.329%
20	14.851	1993	2000	2019	rBV	1796791	2674563	30.03%	2.793%
21	15.634	2126	2133	2140	rBV	5290052	7267273	81.59%	7.590%
22	15.757	2148	2154	2170	rBV	1687991	2142675	24.06%	2.238%
23	15.875	2170	2174	2181	rVB5	22996	36221	0.41%	0.038%
24	16.416	2263	2266	2270	rBV6	7246	9522	0.11%	0.010%
25	17.069	2373	2377	2382	rBV8	7959	11926	0.13%	0.012%
26	17.192	2394	2398	2403	rBV4	6931	10982	0.12%	0.011%
27	17.404	2428	2434	2444	rBV	3532701	4913730	55.17%	5.132%
28	17.510	2445	2452	2463	rBV	5566697	7956713	89.33%	8.310%
29	18.245	2573	2577	2582	rBV8	9844	18166	0.20%	0.019%
30	19.316	2755	2759	2764	rBV3	67352	88093	0.99%	0.092%
31	19.381	2767	2770	2776	rVB	60639	77194	0.87%	0.081%
32	19.745	2826	2832	2842	rBV	6764115	8907285	100.00%	9.303%
33	21.504	3126	3131	3140	rBV	3574291	4574981	51.36%	4.778%
34	23.874	3526	3534	3546	rVB2	3783215	7777748	87.32%	8.123%
35	24.045	3556	3563	3574	rVB	2010331	4267537	47.91%	4.457%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090723\
Data File : BP016991.D
Acq On : 07 Sep 2023 17:00
Operator : MA/JU
Sample : PB155065BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK065

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 95744964

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090723\
Data File : BP016991.D
Acq On : 07 Sep 2023 17:00
Operator : MA/JU
Sample : PB155065BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK065

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

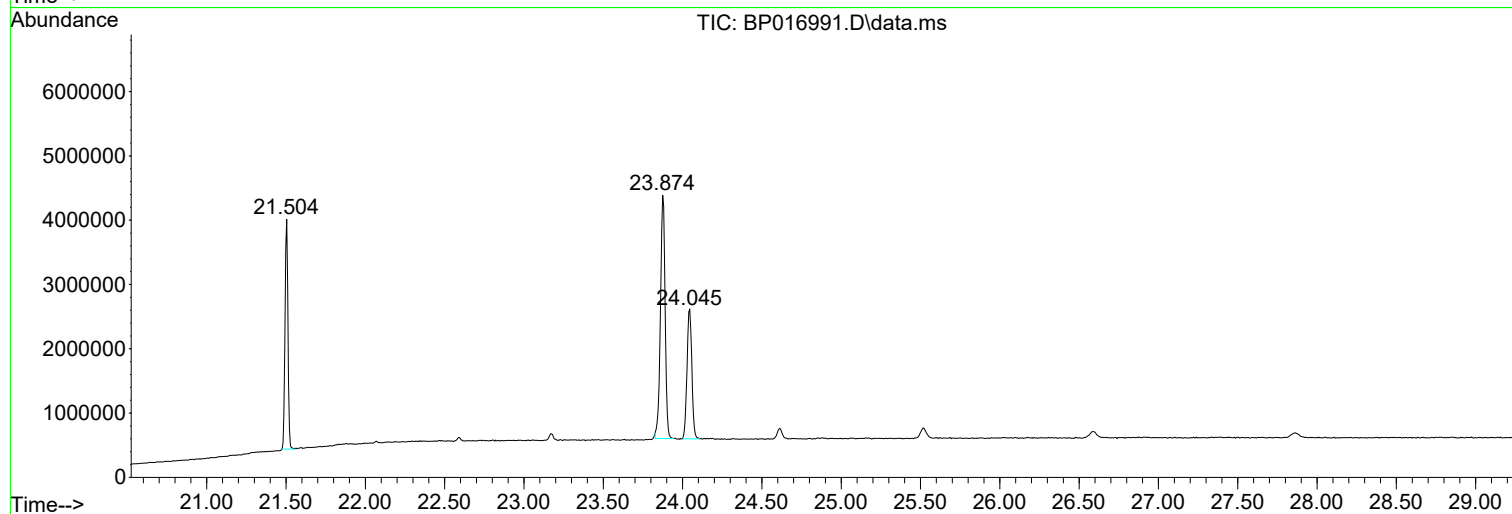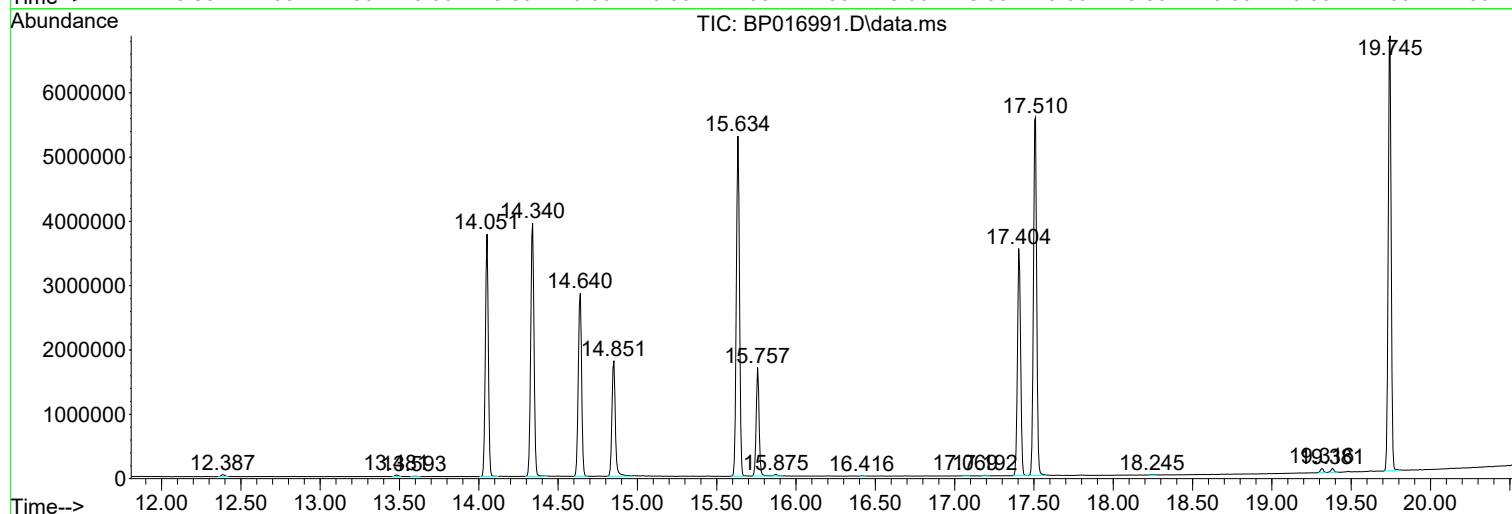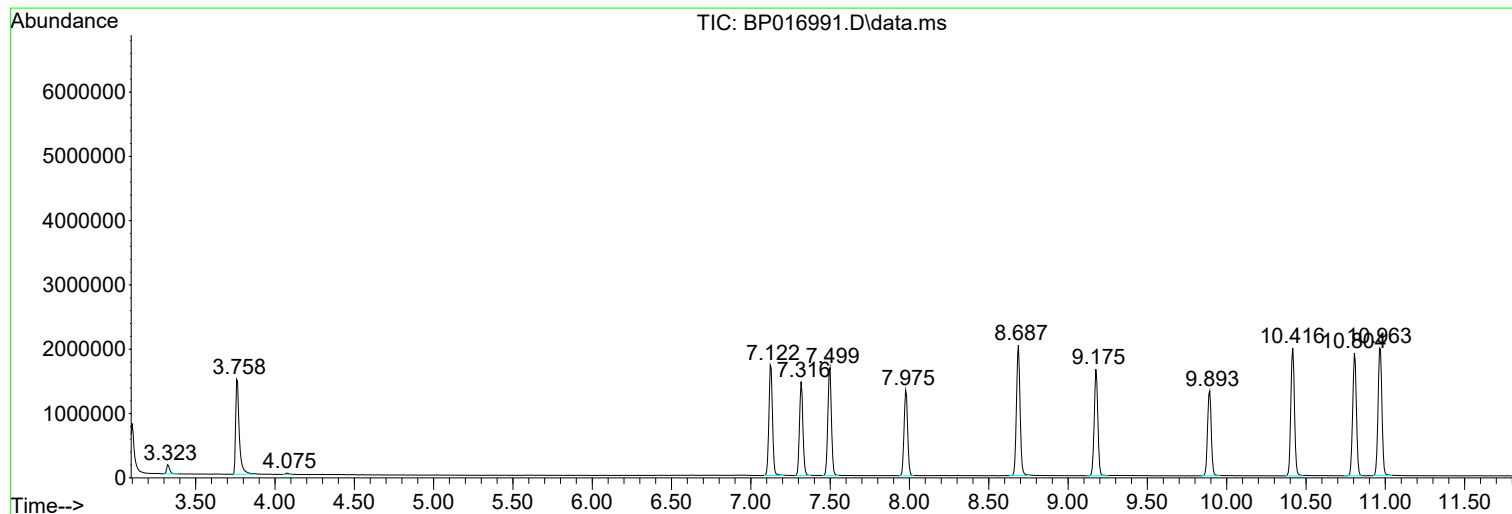

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090723\
Data File : BP016991.D
Acq On : 07 Sep 2023 17:00
Operator : MA/JU
Sample : PB155065BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK065

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090723\
Data File : BP016991.D
Acq On : 07 Sep 2023 17:00
Operator : MA/JU
Sample : PB155065BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK065

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc