

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090723\
 Data File : BP016992.D
 Acq On : 07 Sep 2023 17:35
 Operator : MA/JU
 Sample : PB155068BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK068

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016992.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.322	36	40	47	rBV	133049	176066	2.05%	0.196%
2	3.640	90	94	97	rBV5	6279	8828	0.10%	0.010%
3	3.758	111	114	139	rBV	1390959	2239174	26.10%	2.494%
4	4.075	164	168	172	rBV	17277	25114	0.29%	0.028%
5	7.128	679	687	702	rBV	1628759	2595368	30.25%	2.891%
6	7.316	713	719	728	rBV	1338286	2056488	23.97%	2.291%
7	7.499	743	750	760	rBV	1610336	2496592	29.10%	2.781%
8	7.981	824	832	841	rBV	1090839	1721641	20.06%	1.918%
9	8.687	944	952	965	rBV	1969882	3143327	36.63%	3.501%
10	9.175	1027	1035	1044	rBV	1590080	2531011	29.50%	2.819%
11	9.893	1150	1157	1166	rBV	1301486	2079923	24.24%	2.317%
12	10.416	1236	1246	1258	rBV	1905407	3103942	36.17%	3.458%
13	10.804	1303	1312	1323	rBV	1596577	2621089	30.55%	2.920%
14	10.963	1332	1339	1357	rBV	1937386	3302783	38.49%	3.679%
15	12.387	1575	1581	1590	rVB	29786	51174	0.60%	0.057%
16	13.481	1761	1767	1771	rBV3	20976	33869	0.39%	0.038%
17	13.598	1782	1787	1793	rVB9	6251	12284	0.14%	0.014%
18	14.051	1857	1864	1873	rBV	3539010	4769230	55.58%	5.313%
19	14.334	1905	1912	1926	rBV2	3755729	5582927	65.06%	6.219%
20	14.634	1956	1963	1972	rVB	2396407	3498555	40.77%	3.897%
21	14.851	1993	2000	2013	rBV	1706834	2582068	30.09%	2.876%
22	15.633	2126	2133	2141	rBV	5101466	7033958	81.97%	7.835%
23	15.757	2147	2154	2167	rBV	1645679	2091569	24.38%	2.330%
24	15.869	2169	2173	2178	rVB2	21587	34272	0.40%	0.038%
25	16.204	2222	2230	2234	rVB10	6081	10337	0.12%	0.012%
26	17.404	2427	2434	2443	rBV	3023854	4160401	48.49%	4.634%
27	17.504	2445	2451	2469	rVV2	5426805	7703208	89.77%	8.581%
28	19.316	2755	2759	2763	rVB3	59914	77530	0.90%	0.086%
29	19.380	2766	2770	2776	rVB	54067	75094	0.88%	0.084%
30	19.745	2826	2832	2840	rBV	6777944	8580669	100.00%	9.558%
31	21.504	3126	3131	3140	rBV	3086724	3930076	45.80%	4.378%
32	23.880	3526	3535	3547	rVB2	3756118	7754315	90.37%	8.638%
33	24.045	3556	3563	3573	rVB	1806307	3690173	43.01%	4.111%




Sum of corrected areas: 89773055

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090723\
Data File : BP016992.D
Acq On : 07 Sep 2023 17:35
Operator : MA/JU
Sample : PB155068BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK068

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

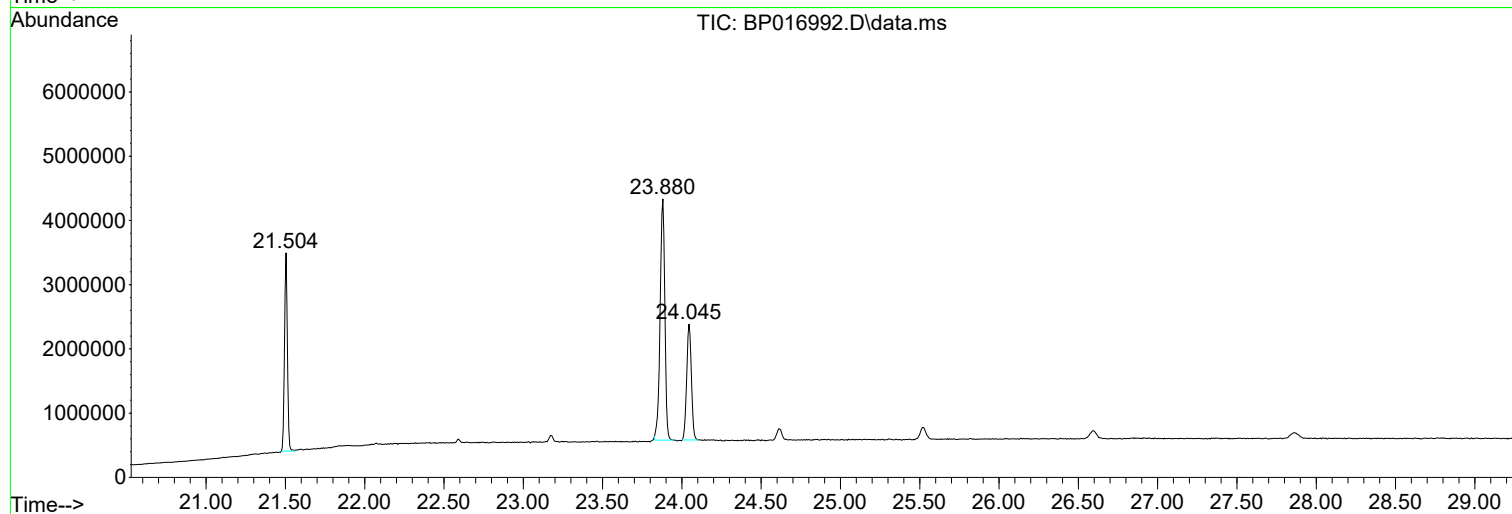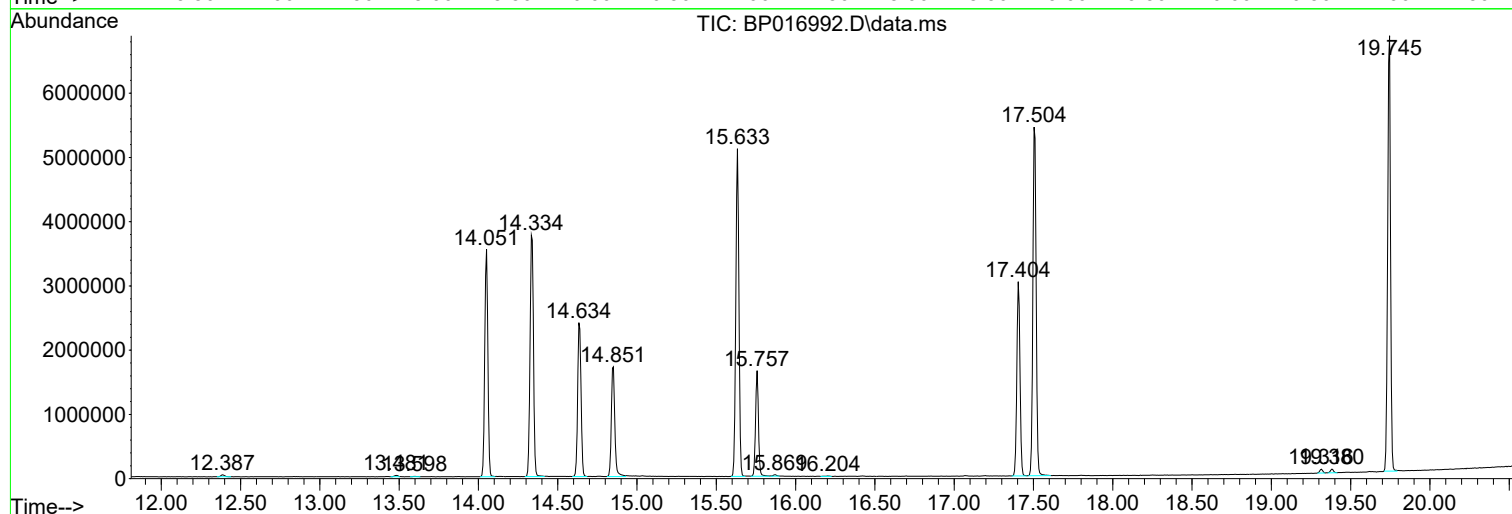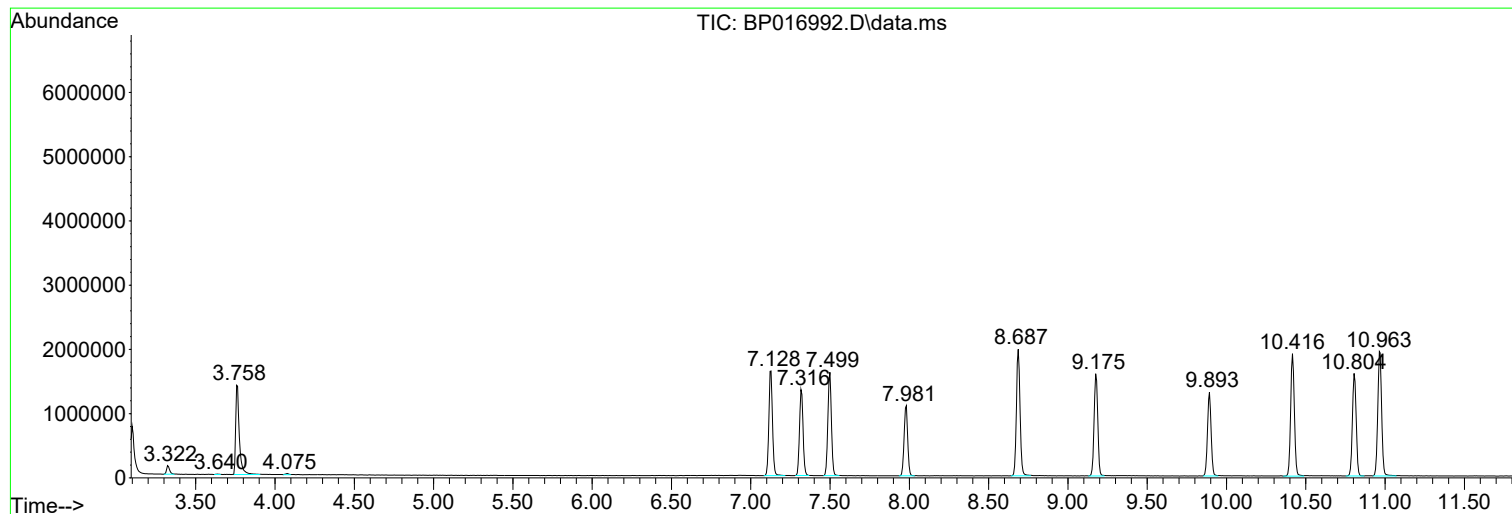

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090723\
Data File : BP016992.D
Acq On : 07 Sep 2023 17:35
Operator : MA/JU
Sample : PB155068BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK068

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090723\
Data File : BP016992.D
Acq On : 07 Sep 2023 17:35
Operator : MA/JU
Sample : PB155068BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK068

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc