

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090723\
 Data File : BP016993.D
 Acq On : 07 Sep 2023 18:10
 Operator : MA/JU
 Sample : 04123-10
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH930

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016993.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.281	30	33	36	rVB3	13277	16714	0.16%	0.018%
2	3.328	36	41	48	rBV	102802	136491	1.32%	0.144%
3	3.764	111	115	129	rBV	658163	1027522	9.97%	1.087%
4	3.964	144	149	161	rVB	46995	84996	0.82%	0.090%
5	4.075	165	168	173	rVB	15612	21810	0.21%	0.023%
6	4.605	253	258	265	rVB	68534	102699	1.00%	0.109%
7	5.016	324	328	333	rBV	16187	24253	0.24%	0.026%
8	6.928	648	653	657	rBV7	6976	17121	0.17%	0.018%
9	7.128	679	687	703	rBV	463008	744167	7.22%	0.787%
10	7.316	712	719	729	rBV	1532187	2358911	22.88%	2.496%
11	7.499	743	750	763	rBV	1477710	2307467	22.39%	2.441%
12	7.981	824	832	844	rBV	1198527	1901480	18.45%	2.012%
13	8.687	944	952	970	rBV	1246822	1991964	19.32%	2.108%
14	9.175	1027	1035	1045	rBV	1810370	2914369	28.27%	3.084%
15	9.393	1068	1072	1079	rVB	29601	44467	0.43%	0.047%
16	9.893	1149	1157	1168	rBV	1451288	2317978	22.49%	2.453%
17	10.416	1237	1246	1257	rBV	2039793	3323576	32.24%	3.516%
18	10.804	1304	1312	1323	rBV	1722799	2844092	27.59%	3.009%
19	10.963	1331	1339	1356	rBV	1941593	3308617	32.10%	3.501%
20	11.887	1490	1496	1502	rVB	35715	54267	0.53%	0.057%
21	12.387	1575	1581	1589	rBV2	34539	59093	0.57%	0.063%
22	13.481	1761	1767	1776	rVB2	26855	49187	0.48%	0.052%
23	13.881	1829	1835	1840	rVB2	18562	27133	0.26%	0.029%
24	14.051	1853	1864	1874	rBV	4096104	5423315	52.61%	5.738%
25	14.340	1905	1913	1933	rBV	4351668	6368361	61.78%	6.738%
26	14.639	1957	1964	1974	rVB	2595576	3765221	36.53%	3.984%
27	14.757	1981	1984	1992	rVB9	7421	14320	0.14%	0.015%
28	14.845	1992	1999	2020	rBV	399974	667829	6.48%	0.707%
29	15.439	2097	2100	2105	rVB5	9068	13610	0.13%	0.014%
30	15.634	2126	2133	2140	rBV	6007549	8139021	78.96%	8.611%
31	15.757	2148	2154	2169	rBV	2013152	2581141	25.04%	2.731%
32	15.869	2169	2173	2177	rVB2	25498	33132	0.32%	0.035%
33	17.069	2372	2377	2383	rBV10	10768	22762	0.22%	0.024%
34	17.404	2428	2434	2444	rBV	3278280	4488374	43.54%	4.749%
35	17.504	2445	2451	2464	rBV2	6427260	8935730	86.69%	9.454%
36	18.033	2537	2541	2544	rBV6	9921	14169	0.14%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090723\
Data File : BP016993.D
Acq On : 07 Sep 2023 18:10
Operator : MA/JU
Sample : 04123-10
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH930

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Title : SVOA CALIBRATION

37	18.239	2572	2576	2584	rBV2	81630	119554	1.16%	0.126%
38	19.316	2755	2759	2763	rBV	71366	94705	0.92%	0.100%
39	19.380	2766	2770	2775	rVV	72791	93594	0.91%	0.099%
40	19.480	2783	2787	2794	rBV5	53468	76107	0.74%	0.081%
41	19.622	2808	2811	2814	rBV2	24874	27634	0.27%	0.029%
42	19.745	2825	2832	2842	rBV	7863517	10307852	100.00%	10.906%
43	21.504	3126	3131	3137	rBV	3437098	4314821	41.86%	4.565%
44	23.874	3527	3534	3548	rVB2	4577624	9216213	89.41%	9.751%
45	24.045	3556	3563	3574	rVB	1989139	4118882	39.96%	4.358%




Sum of corrected areas: 94514721

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090723\
Data File : BP016993.D
Acq On : 07 Sep 2023 18:10
Operator : MA/JU
Sample : 04123-10
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH930

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

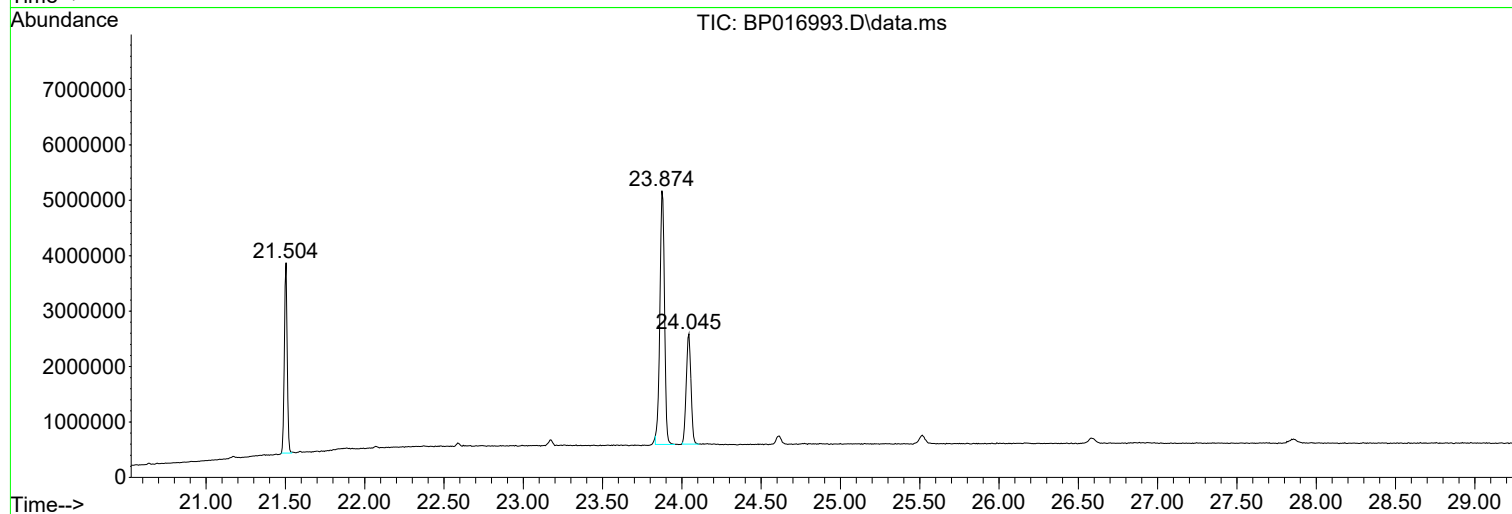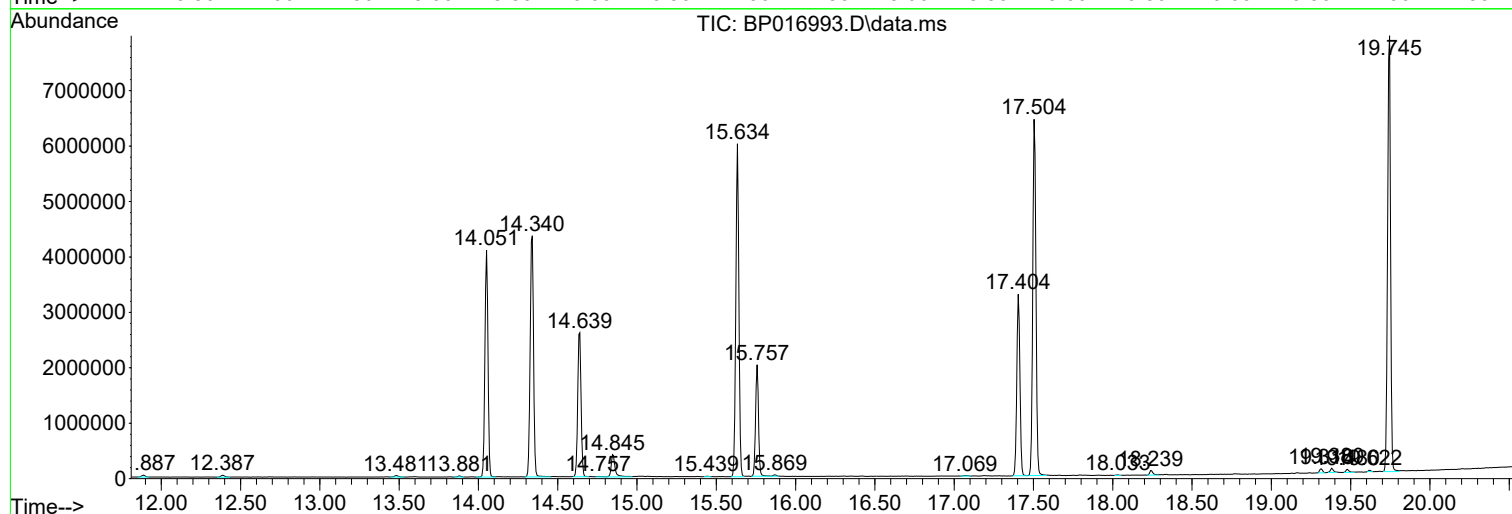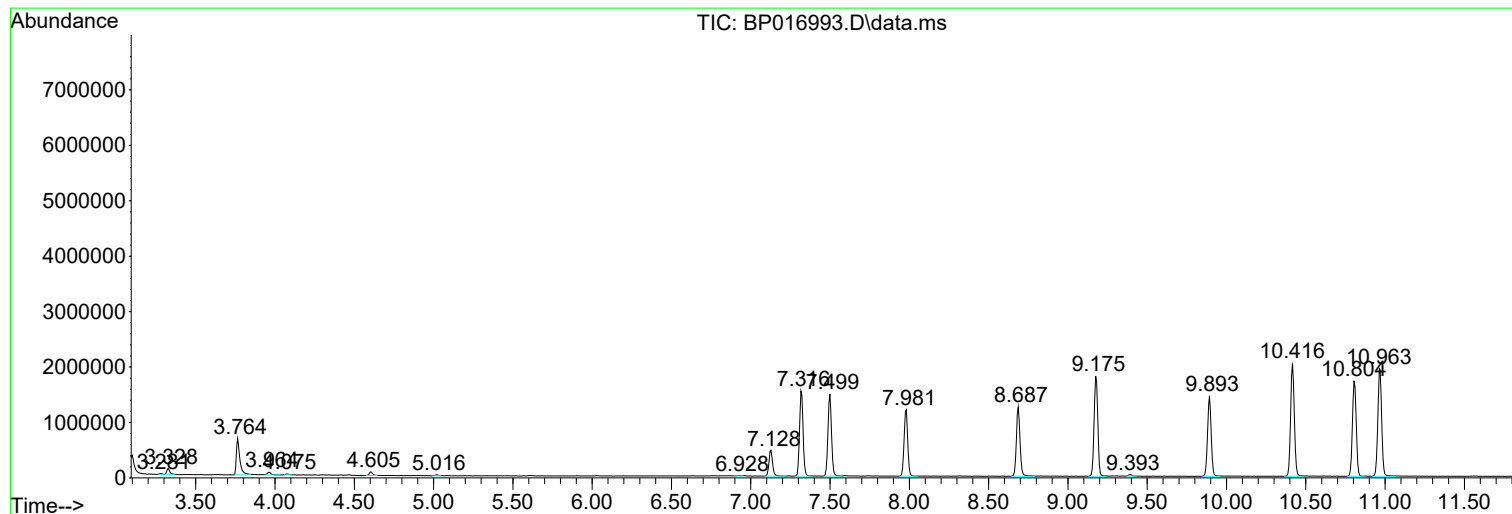

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090723\
Data File : BP016993.D
Acq On : 07 Sep 2023 18:10
Operator : MA/JU
Sample : 04123-10
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH930

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090723\
Data File : BP016993.D
Acq On : 07 Sep 2023 18:10
Operator : MA/JU
Sample : 04123-10
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH930

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------