

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090723\
 Data File : BP016994.D
 Acq On : 07 Sep 2023 18:45
 Operator : MA/JU
 Sample : 04123-11
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH9H3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016994.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.323	36	40	54	rVB	129583	197950	1.51%	0.168%
2	3.764	111	115	132	rBV	611855	959867	7.31%	0.815%
3	3.964	144	149	156	rVB	58929	96360	0.73%	0.082%
4	4.076	164	168	172	rBV	20368	26110	0.20%	0.022%
5	4.605	253	258	266	rVB	77477	116109	0.88%	0.099%
6	5.017	323	328	333	rBV	21896	33759	0.26%	0.029%
7	5.611	424	429	433	rBV3	9558	16110	0.12%	0.014%
8	6.922	646	652	662	rVB8	14844	37072	0.28%	0.031%
9	7.122	677	686	700	rBV	573641	910248	6.93%	0.772%
10	7.317	712	719	730	rBV	1827432	2804893	21.35%	2.380%
11	7.499	742	750	761	rBV	1794601	2772318	21.10%	2.353%
12	7.593	761	766	772	rVB3	9554	20686	0.16%	0.018%
13	7.975	824	831	844	rVB	1321541	2124497	16.17%	1.803%
14	8.687	944	952	968	rBV	1529182	2472769	18.82%	2.099%
15	9.052	1008	1014	1019	rBV6	11387	22064	0.17%	0.019%
16	9.175	1027	1035	1047	rBV	2194694	3506926	26.69%	2.976%
17	9.346	1059	1064	1068	rBV3	33510	53768	0.41%	0.046%
18	9.393	1068	1072	1079	rVB6	14038	21793	0.17%	0.018%
19	9.640	1108	1114	1117	rBV2	12344	17392	0.13%	0.015%
20	9.763	1129	1135	1142	rVB2	22741	37725	0.29%	0.032%
21	9.893	1150	1157	1169	rVB	1781625	2809511	21.38%	2.384%
22	10.046	1178	1183	1190	rVB4	12890	25981	0.20%	0.022%
23	10.146	1194	1200	1204	rBV3	12412	25197	0.19%	0.021%
24	10.416	1238	1246	1260	rBV	2547939	4112020	31.30%	3.490%
25	10.575	1268	1273	1276	rBV7	6115	13241	0.10%	0.011%
26	10.658	1282	1287	1292	rVB6	12164	23580	0.18%	0.020%
27	10.805	1300	1312	1321	rBV	1994449	3251777	24.75%	2.760%
28	10.963	1331	1339	1352	rBV	2039038	3525860	26.84%	2.992%
29	11.552	1433	1439	1446	rBV	9949	23044	0.18%	0.020%
30	11.622	1447	1451	1458	rVB4	13941	22709	0.17%	0.019%
31	11.916	1497	1501	1505	rBV2	16853	27173	0.21%	0.023%
32	11.957	1505	1508	1515	rVB7	13947	22929	0.17%	0.019%
33	12.075	1520	1528	1538	rBV2	50685	108467	0.83%	0.092%
34	12.257	1555	1559	1564	rBV2	9148	17325	0.13%	0.015%
35	12.387	1576	1581	1587	rVB2	49072	79398	0.60%	0.067%
36	12.728	1635	1639	1641	rBV5	10337	14034	0.11%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090723\
 Data File : BP016994.D
 Acq On : 07 Sep 2023 18:45
 Operator : MA/JU
 Sample : 04123-11
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH9H3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
 Title : SVOA CALIBRATION

37	12.875	1658	1664	1668	rBV9	12572	29006	0.22%	0.025%
38	12.916	1668	1671	1676	rVB7	13956	20085	0.15%	0.017%
39	13.093	1697	1701	1706	rVB2	31502	51527	0.39%	0.044%
40	13.175	1708	1715	1717	rBV6	12455	25000	0.19%	0.021%
41	13.304	1734	1737	1742	rVB6	13201	17607	0.13%	0.015%
42	13.481	1762	1767	1774	rBV3	27811	53872	0.41%	0.046%
43	13.628	1788	1792	1801	rVB5	21985	39474	0.30%	0.033%
44	13.751	1808	1813	1821	rVB5	9679	21922	0.17%	0.019%
45	13.969	1847	1850	1857	rVB9	9649	17002	0.13%	0.014%
46	14.051	1857	1864	1870	rBV	4947650	6551917	49.87%	5.560%
47	14.257	1894	1899	1904	rBV3	30103	50423	0.38%	0.043%
48	14.340	1906	1913	1924	rVV	5304174	7913394	60.23%	6.716%
49	14.634	1956	1963	1973	rBV	2902287	4283718	32.60%	3.635%
50	14.757	1980	1984	1991	rBV10	13180	30401	0.23%	0.026%
51	14.851	1994	2000	2015	rVV	531613	854561	6.50%	0.725%
52	15.587	2120	2125	2126	rBV4	15165	22165	0.17%	0.019%
53	15.634	2126	2133	2139	rVV	7208578	9882389	75.22%	8.387%
54	15.693	2139	2143	2148	rVB	126659	175088	1.33%	0.149%
55	15.757	2148	2154	2163	rBV	2610726	3357724	25.56%	2.850%
56	15.869	2169	2173	2178	rVV2	29255	42091	0.32%	0.036%
57	15.922	2180	2182	2190	rVB7	20920	29642	0.23%	0.025%
58	16.422	2263	2267	2271	rVB5	19797	28332	0.22%	0.024%
59	17.404	2428	2434	2444	rBV	3787571	5214123	39.69%	4.425%
60	17.504	2445	2451	2460	rBV	7742642	11046425	84.08%	9.375%
61	18.245	2573	2577	2583	rBV	188219	269071	2.05%	0.228%
62	19.310	2755	2758	2763	rBV	96745	123835	0.94%	0.105%
63	19.381	2766	2770	2775	rVB	95562	131614	1.00%	0.112%
64	19.481	2783	2787	2798	rBV2	134219	195756	1.49%	0.166%
65	19.616	2808	2810	2814	rVB	47908	47454	0.36%	0.040%
66	19.745	2826	2832	2841	rBV	9855167	13138340	100.00%	11.150%
67	21.504	3125	3131	3137	rBV	4125412	5510245	41.94%	4.676%
68	23.874	3524	3534	3549	rVB2	6159415	13006248	98.99%	11.038%
69	24.045	3555	3563	3574	rVB	2540115	5302799	40.36%	4.500%




Sum of corrected areas: 117833912

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090723\
Data File : BP016994.D
Acq On : 07 Sep 2023 18:45
Operator : MA/JU
Sample : 04123-11
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH9H3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

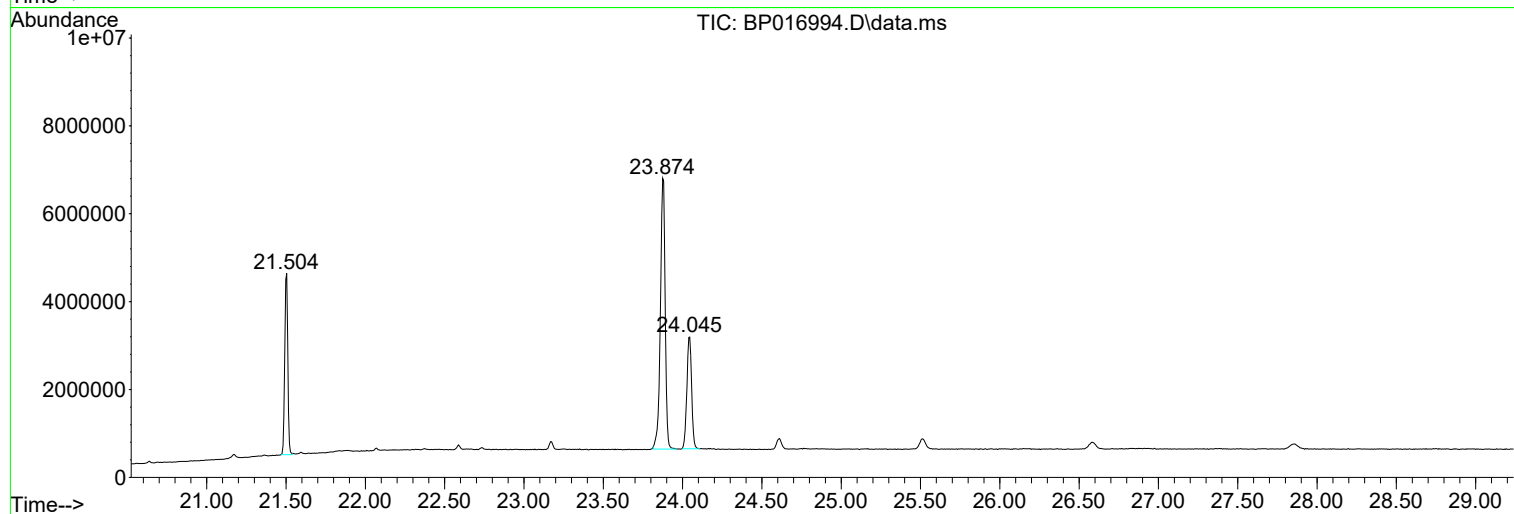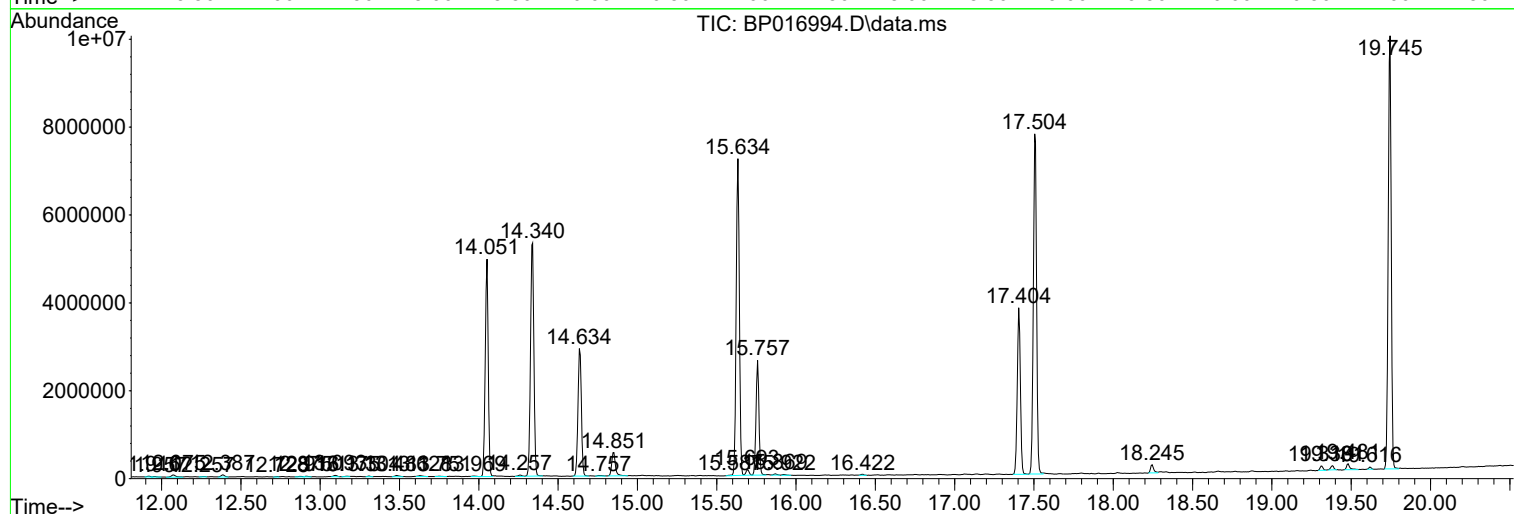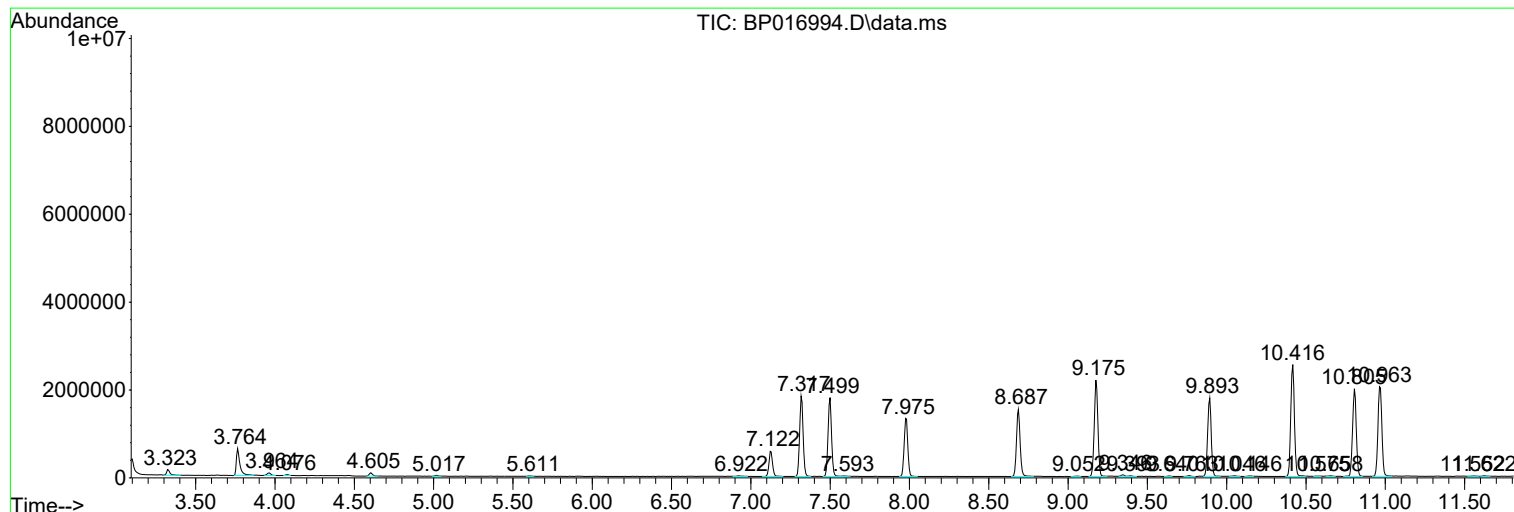

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090723\
Data File : BP016994.D
Acq On : 07 Sep 2023 18:45
Operator : MA/JU
Sample : 04123-11
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH9H3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090723\
Data File : BP016994.D
Acq On : 07 Sep 2023 18:45
Operator : MA/JU
Sample : 04123-11
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH9H3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc