

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090723\
 Data File : BP016995.D
 Acq On : 07 Sep 2023 19:20
 Operator : MA/JU
 Sample : 04123-12
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH8W9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016995.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.281	28	33	37	rBV	95256	145687	0.79%	0.110%
2	3.328	37	41	51	rVB	115879	181981	0.99%	0.137%
3	3.764	111	115	130	rBV	666825	1071593	5.83%	0.808%
4	3.964	144	149	156	rVB	52674	86064	0.47%	0.065%
5	4.075	163	168	180	rVB	119105	187773	1.02%	0.142%
6	4.605	251	258	275	rBV	11644987	18374191	100.00%	13.847%
7	5.017	325	328	334	rBV	18264	25012	0.14%	0.019%
8	6.499	573	580	588	rVB	419091	647086	3.52%	0.488%
9	7.122	679	686	698	rBV	562507	901061	4.90%	0.679%
10	7.317	712	719	729	rBV	1735704	2699811	14.69%	2.035%
11	7.499	741	750	759	rBV	1743028	2702812	14.71%	2.037%
12	7.587	761	765	774	rVB3	11024	20988	0.11%	0.016%
13	7.981	824	832	845	rBV	1504564	2383227	12.97%	1.796%
14	8.687	942	952	965	rBV	1514410	2435899	13.26%	1.836%
15	9.175	1027	1035	1047	rBV	2050858	3330317	18.12%	2.510%
16	9.893	1150	1157	1175	rBV	1680400	2703717	14.71%	2.038%
17	10.416	1237	1246	1259	rBV	2463266	3998914	21.76%	3.014%
18	10.805	1305	1312	1323	rBV	2184412	3612386	19.66%	2.722%
19	10.963	1331	1339	1358	rBV	1925543	3291955	17.92%	2.481%
20	11.622	1446	1451	1457	rVB7	9361	19820	0.11%	0.015%
21	12.387	1576	1581	1588	rVB2	39315	61076	0.33%	0.046%
22	13.481	1761	1767	1775	rVB2	28232	45660	0.25%	0.034%
23	14.051	1857	1864	1877	rBV	4642848	6235984	33.94%	4.700%
24	14.334	1905	1912	1929	rBV2	5047825	7470209	40.66%	5.630%
25	14.634	1957	1963	1971	rBV	3310067	4827607	26.27%	3.638%
26	14.846	1993	1999	2016	rBV	496515	818617	4.46%	0.617%
27	15.034	2022	2031	2035	rBV	11518	32338	0.18%	0.024%
28	15.634	2126	2133	2139	rBV	6827057	9405041	51.19%	7.088%
29	15.693	2139	2143	2148	rVV	167340	245937	1.34%	0.185%
30	15.757	2148	2154	2168	rVV	2384571	3136199	17.07%	2.364%
31	15.869	2169	2173	2177	rVB2	25798	35099	0.19%	0.026%
32	17.404	2427	2434	2444	rBV	4179926	5829969	31.73%	4.394%
33	17.504	2445	2451	2464	rVV2	7574144	10332007	56.23%	7.787%
34	18.239	2572	2576	2582	rBV	179968	260541	1.42%	0.196%
35	19.310	2755	2758	2762	rVB2	87994	105674	0.58%	0.080%
36	19.381	2767	2770	2774	rVB	91887	115463	0.63%	0.087%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090723\
Data File : BP016995.D
Acq On : 07 Sep 2023 19:20
Operator : MA/JU
Sample : 04123-12
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH8W9

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Title : SVOA CALIBRATION

37	19.475	2783	2786	2796	rBV	107414	149307	0.81%	0.113%
38	19.739	2825	2831	2838	rBV	9000513	11826364	64.36%	8.913%
39	20.045	2879	2883	2888	rBV	162928	202012	1.10%	0.152%
40	21.498	3125	3130	3137	rBV	4596345	5928436	32.27%	4.468%
41	23.874	3526	3534	3546	rVB2	5341419	11143706	60.65%	8.398%
42	24.039	3555	3562	3575	rVB	2701730	5662960	30.82%	4.268%




Sum of corrected areas: 132690500

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090723\
Data File : BP016995.D
Acq On : 07 Sep 2023 19:20
Operator : MA/JU
Sample : 04123-12
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH8W9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

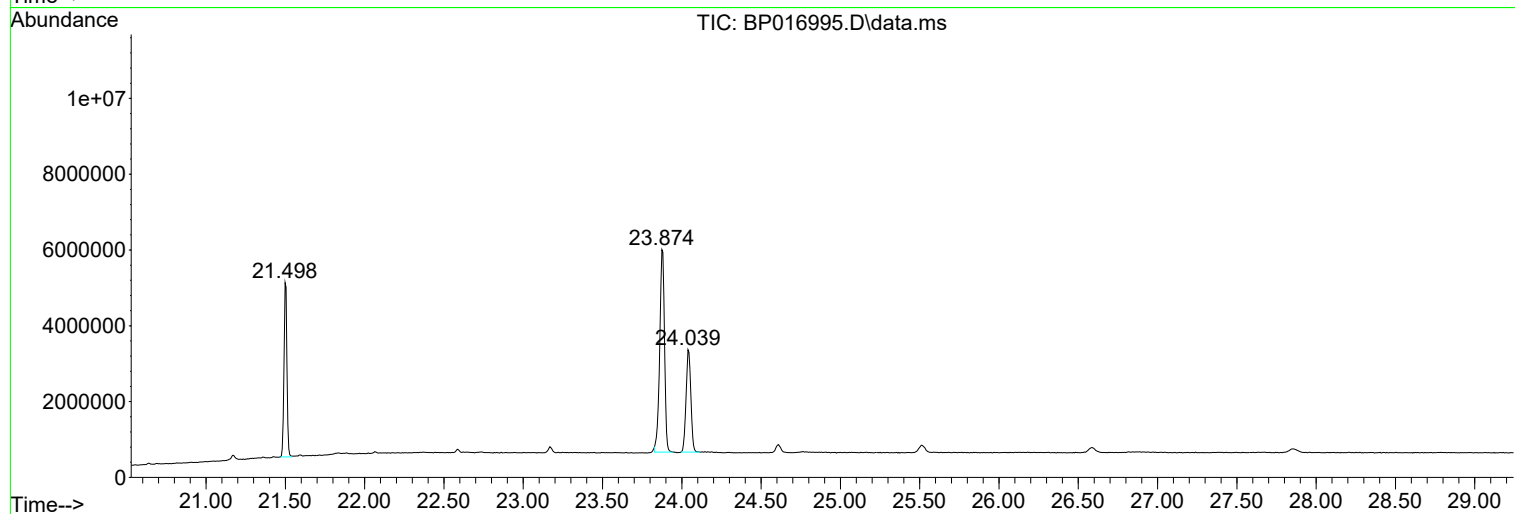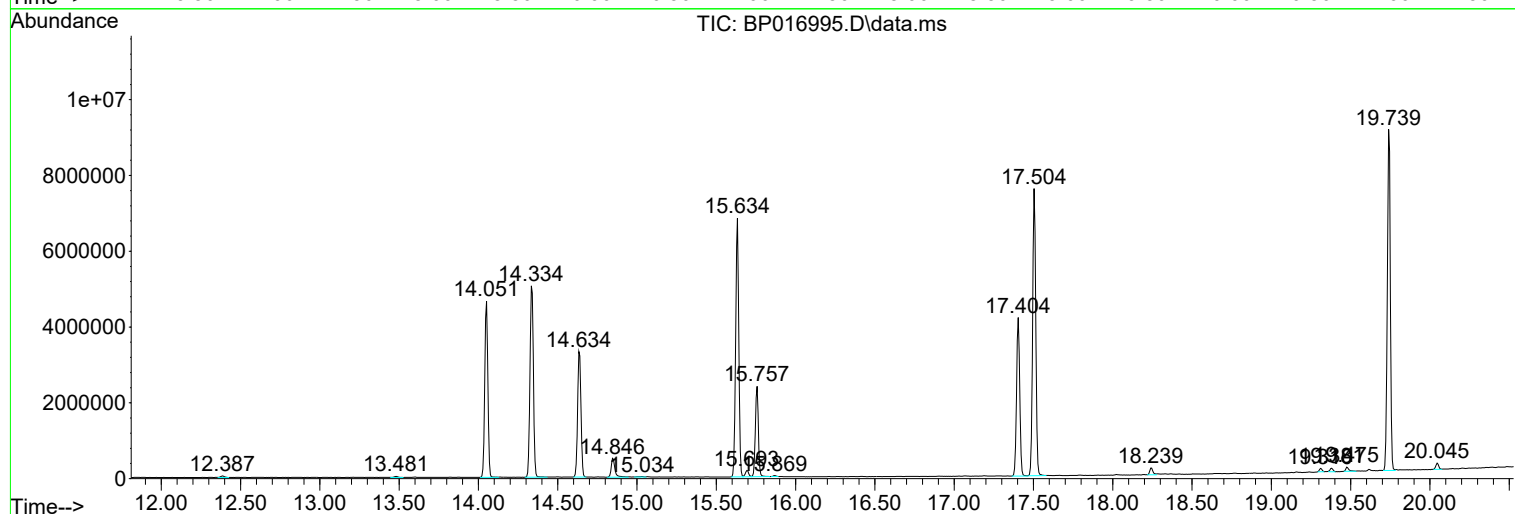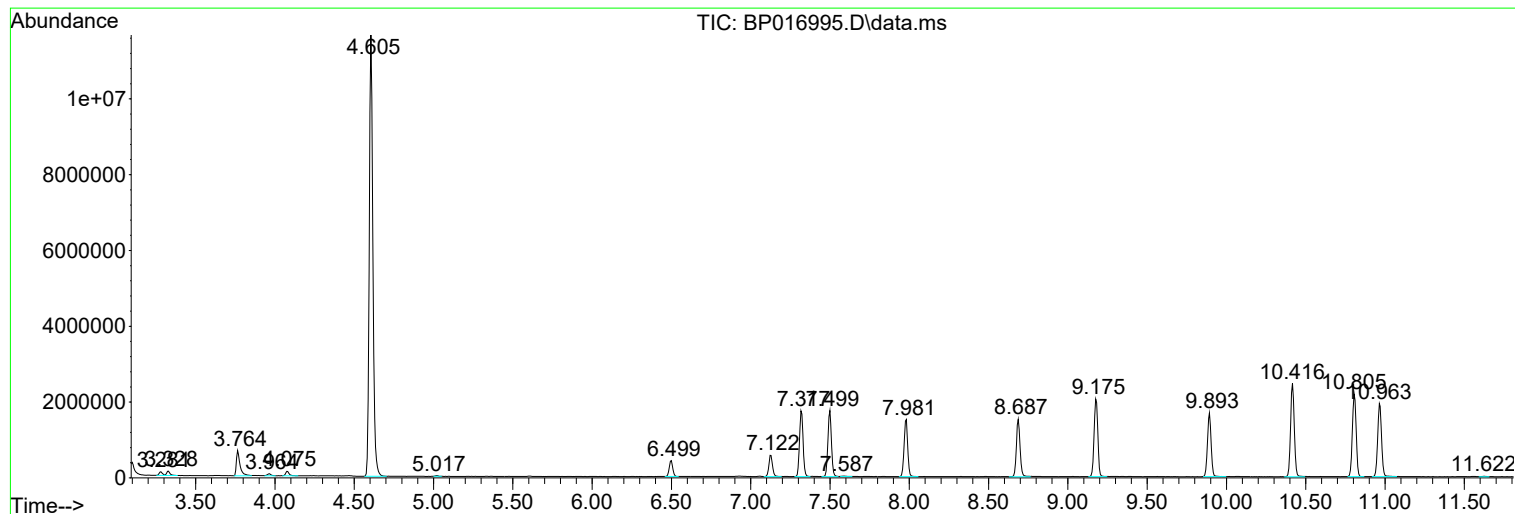

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090723\
Data File : BP016995.D
Acq On : 07 Sep 2023 19:20
Operator : MA/JU
Sample : 04123-12
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH8W9









Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.605	154.20 ng/ul	18374200	1,4-Dichlorobenzene-d4	7.981

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	99
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	99
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	94
5			Pyrimidine, 5-fluoro-2,4-dichloro-	166	C4HC12FN2	002927-71-1	35

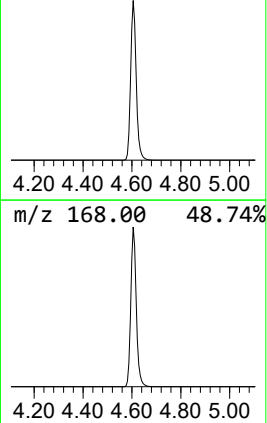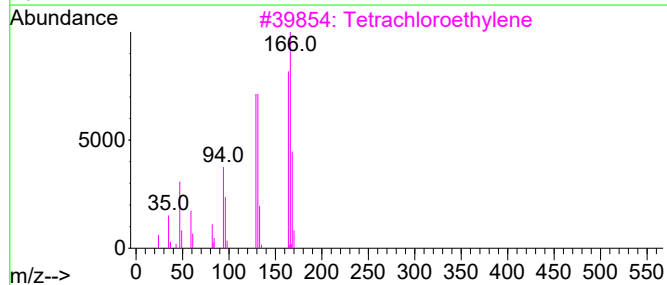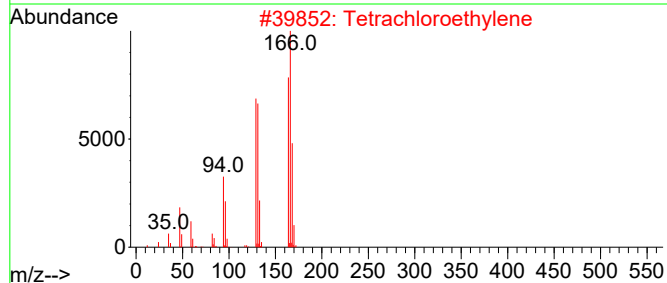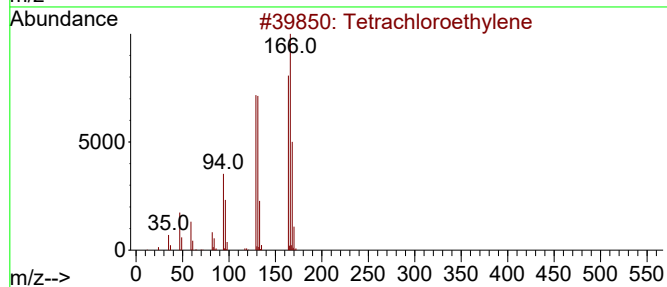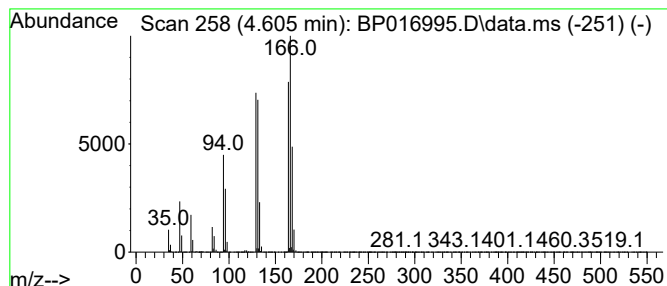

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090723\
Data File : BP016995.D
Acq On : 07 Sep 2023 19:20
Operator : MA/JU
Sample : 04123-12
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH8W9










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Propane, 1,2,3-trichloro- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.499	5.43 ng/ul	647086	1,4-Dichlorobenzene-d4	7.981

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Propane, 1,2,3-trichloro-	146	C3H5Cl3	000096-18-4	91
2			Propane, 1,2,3-trichloro-	146	C3H5Cl3	000096-18-4	91
3			1-Propene, 1,3-dichloro-, (Z)-	110	C3H4Cl2	010061-01-5	86
4			Propane, 1,2,3-trichloro-	146	C3H5Cl3	000096-18-4	86
5			Propane, 1,2,3-trichloro-	146	C3H5Cl3	000096-18-4	74

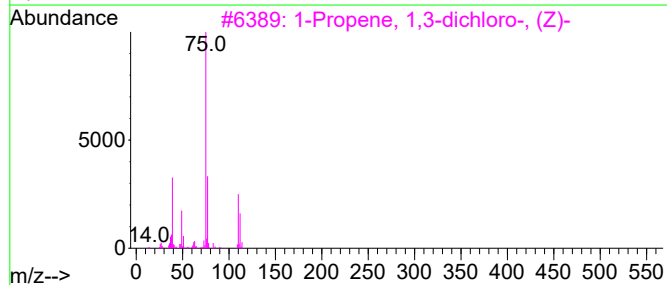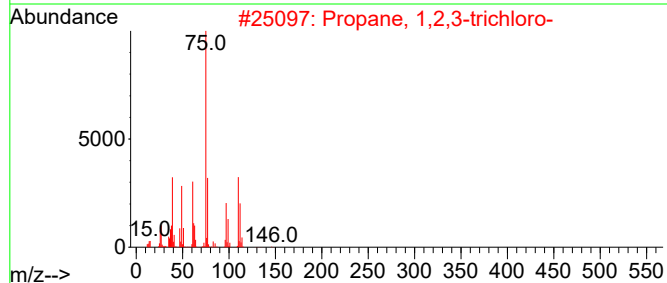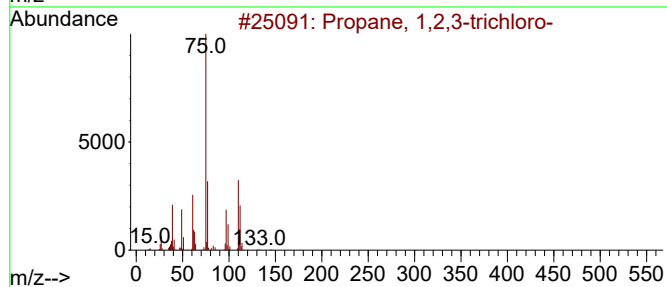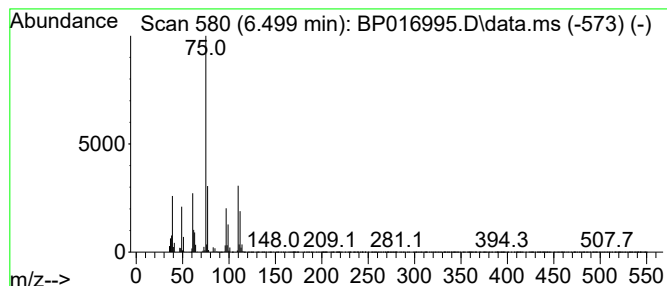

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090723\
Data File : BP016995.D
Acq On : 07 Sep 2023 19:20
Operator : MA/JU
Sample : 04123-12
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH8W9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.605	154.2	ng/ul	18374200	1	7.981	2383230	20.0
Propane, 1,2,3-...	6.499	5.4	ng/ul	647086	1	7.981	2383230	20.0