

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090723\
 Data File : BP016997.D
 Acq On : 07 Sep 2023 20:29
 Operator : MA/JU
 Sample : 04123-14
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH9Y0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016997.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.328	36	41	49	rVB	120636	163660	1.36%	0.142%
2	3.764	111	115	131	rBV	593063	952090	7.91%	0.828%
3	3.964	144	149	160	rVB	63190	100296	0.83%	0.087%
4	4.075	164	168	180	rVB	140196	213643	1.77%	0.186%
5	4.464	232	234	240	rVB5	12594	16358	0.14%	0.014%
6	4.605	255	258	263	rVB5	11241	14571	0.12%	0.013%
7	5.017	323	328	333	rBV	18895	27767	0.23%	0.024%
8	5.605	424	428	435	rVB2	13228	23846	0.20%	0.021%
9	6.922	648	652	657	rBV5	12905	24051	0.20%	0.021%
10	7.128	679	687	703	rBV	534615	875362	7.27%	0.762%
11	7.316	712	719	730	rBV	1962837	3031270	25.18%	2.638%
12	7.499	742	750	759	rBV	1814136	2868881	23.83%	2.496%
13	7.587	760	765	770	rVB2	13071	25947	0.22%	0.023%
14	7.975	824	831	844	rBV	1479236	2329373	19.35%	2.027%
15	8.687	945	952	964	rBV	1500803	2375682	19.73%	2.067%
16	9.175	1027	1035	1048	rBV	2304976	3761063	31.24%	3.273%
17	9.387	1066	1071	1080	rVB	23312	42764	0.36%	0.037%
18	9.893	1147	1157	1170	rBV	1838504	2983865	24.79%	2.596%
19	10.416	1238	1246	1255	rBV	2657866	4290727	35.64%	3.734%
20	10.804	1304	1312	1323	rBV	2162949	3534381	29.36%	3.075%
21	10.963	1332	1339	1360	rBV	1983153	3351115	27.84%	2.916%
22	11.557	1433	1440	1444	rBV6	9045	20455	0.17%	0.018%
23	11.622	1446	1451	1457	rVV4	21281	38908	0.32%	0.034%
24	11.887	1491	1496	1502	rVB	15418	22710	0.19%	0.020%
25	12.387	1574	1581	1588	rBV2	43281	73425	0.61%	0.064%
26	13.387	1746	1751	1755	rBV4	9286	16241	0.13%	0.014%
27	13.481	1761	1767	1772	rBV	24199	41012	0.34%	0.036%
28	13.593	1780	1786	1793	rBV8	9305	18272	0.15%	0.016%
29	13.822	1819	1825	1829	rBV8	8472	12161	0.10%	0.011%
30	13.875	1829	1834	1839	rBV5	8456	15069	0.13%	0.013%
31	14.051	1857	1864	1870	rBV	5141714	6870293	57.07%	5.978%
32	14.334	1905	1912	1921	rBV	5810331	8227773	68.34%	7.159%
33	14.634	1957	1963	1971	rVB	3232083	4648859	38.62%	4.045%
34	14.845	1993	1999	2019	rBV	459309	720908	5.99%	0.627%
35	15.375	2082	2089	2094	rBV5	9097	15236	0.13%	0.013%
36	15.445	2094	2101	2105	rBV5	8429	13178	0.11%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090723\
 Data File : BP016997.D
 Acq On : 07 Sep 2023 20:29
 Operator : MA/JU
 Sample : 04123-14
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH9Y0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
 Title : SVOA CALIBRATION

37	15.634	2125	2133	2139	rBV	7383111	10222669	84.92%	8.895%
38	15.692	2139	2143	2148	rVV	137429	207150	1.72%	0.180%
39	15.757	2148	2154	2167	rVV	2424702	3207568	26.64%	2.791%
40	15.869	2168	2173	2178	rVB	31802	50951	0.42%	0.044%
41	17.069	2373	2377	2385	rBV9	10806	21660	0.18%	0.019%
42	17.404	2427	2434	2444	rBV	4000900	5461906	45.37%	4.753%
43	17.504	2444	2451	2468	rVV2	7994286	10858769	90.20%	9.449%
44	18.022	2537	2539	2544	rVB6	17728	20810	0.17%	0.018%
45	18.239	2572	2576	2588	rBV	251429	408503	3.39%	0.355%
46	18.333	2589	2592	2597	rVB	26913	37957	0.32%	0.033%
47	19.310	2754	2758	2762	rBV2	93009	125823	1.05%	0.109%
48	19.380	2766	2770	2775	rVB	90932	131938	1.10%	0.115%
49	19.475	2782	2786	2793	rBV	179700	268358	2.23%	0.234%
50	19.616	2807	2810	2813	rBV	44716	49883	0.41%	0.043%
51	19.739	2825	2831	2838	rBV	9372241	12038695	100.00%	10.475%
52	21.498	3125	3130	3137	rBV	3904016	5098979	42.35%	4.437%
53	23.868	3525	3533	3546	rVB2	4904207	10348874	85.96%	9.005%
54	24.039	3555	3562	3572	rVB	2217121	4603277	38.24%	4.005%




Sum of corrected areas: 114924982

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090723\
Data File : BP016997.D
Acq On : 07 Sep 2023 20:29
Operator : MA/JU
Sample : 04123-14
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH9Y0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

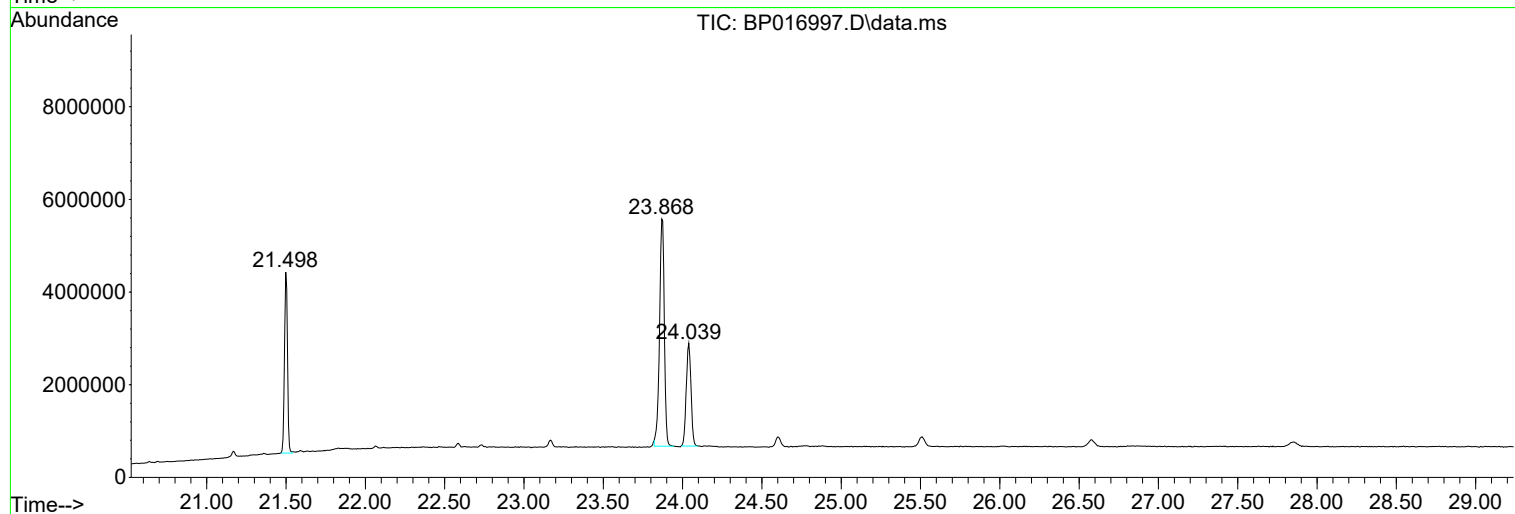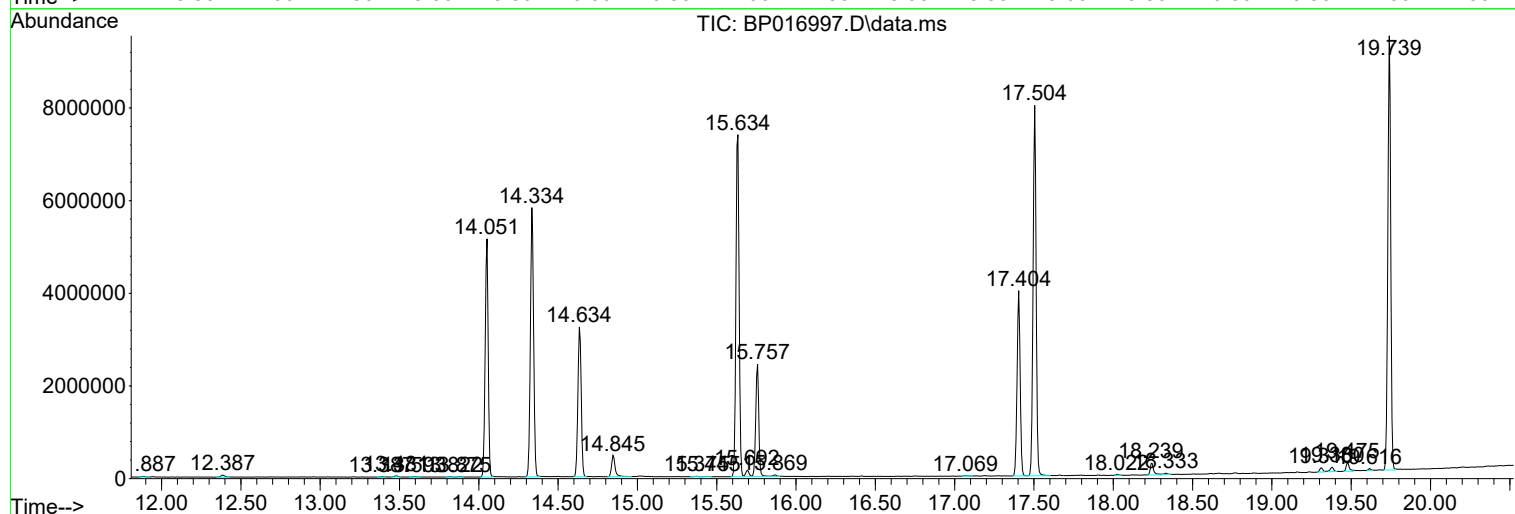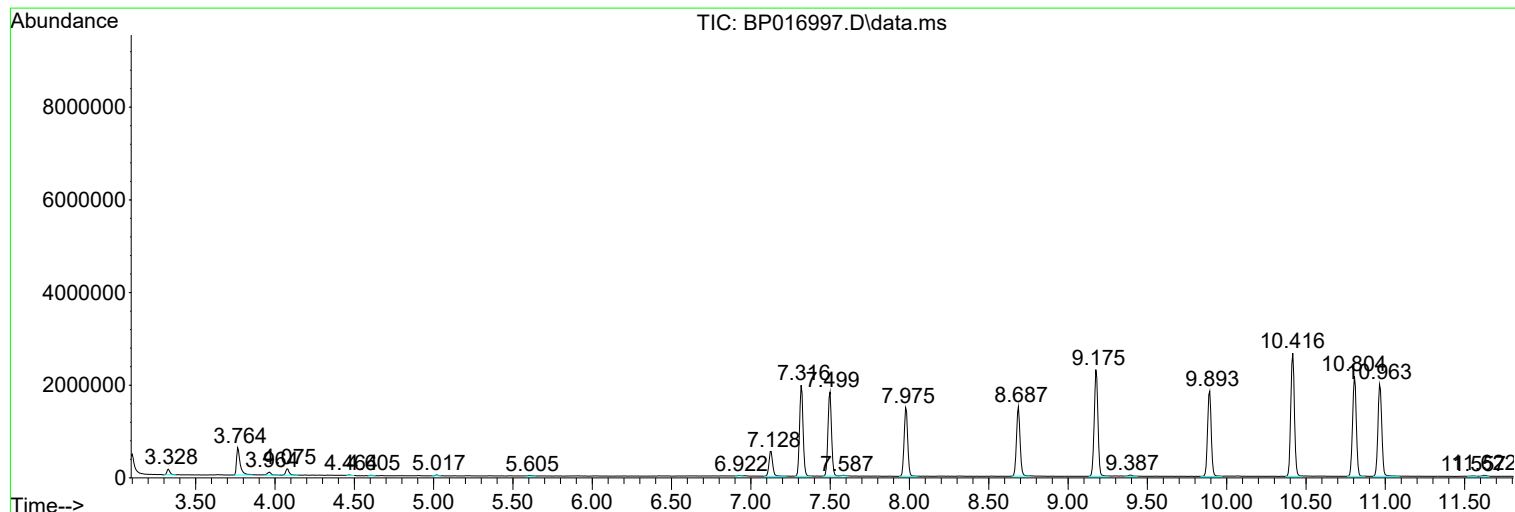

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090723\
Data File : BP016997.D
Acq On : 07 Sep 2023 20:29
Operator : MA/JU
Sample : 04123-14
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH9Y0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090723\
Data File : BP016997.D
Acq On : 07 Sep 2023 20:29
Operator : MA/JU
Sample : 04123-14
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH9Y0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------