

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090723\
 Data File : BP016998.D
 Acq On : 07 Sep 2023 21:03
 Operator : MA/JU
 Sample : 04123-15
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH931

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016998.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.328	37	41	49	rVB	113358	153958	1.31%	0.141%
2	3.764	112	115	130	rBV	581326	918284	7.79%	0.840%
3	3.964	144	149	157	rVB	54034	83438	0.71%	0.076%
4	4.075	163	168	177	rVB	137971	196932	1.67%	0.180%
5	4.605	253	258	265	rVB	80826	123382	1.05%	0.113%
6	5.022	324	329	332	rBV2	20829	29415	0.25%	0.027%
7	5.611	424	429	434	rVB2	8002	13624	0.12%	0.012%
8	6.928	647	653	656	rBV5	10511	19443	0.16%	0.018%
9	7.128	680	687	702	rBV	483874	786323	6.67%	0.719%
10	7.316	712	719	732	rVB	1785176	2713467	23.02%	2.482%
11	7.499	742	750	761	rBV	1637524	2598842	22.05%	2.377%
12	7.975	824	831	843	rVB	1347685	2159358	18.32%	1.975%
13	8.687	943	952	969	rBV	1378119	2250053	19.09%	2.058%
14	9.175	1027	1035	1045	rBV	2101947	3367964	28.57%	3.080%
15	9.893	1145	1157	1167	rBV	1685121	2742941	23.27%	2.509%
16	10.416	1238	1246	1260	rBV	2427893	3947866	33.49%	3.611%
17	10.804	1303	1312	1322	rBV	2041814	3316741	28.14%	3.034%
18	10.963	1330	1339	1356	rBV	2163903	3661429	31.06%	3.349%
19	11.557	1433	1440	1448	rVB8	12097	23119	0.20%	0.021%
20	12.387	1573	1581	1587	rBV2	42607	69473	0.59%	0.064%
21	13.481	1762	1767	1775	rVB	33855	52818	0.45%	0.048%
22	13.593	1782	1786	1792	rVB4	8429	15264	0.13%	0.014%
23	14.051	1857	1864	1873	rBV	4839494	6615435	56.13%	6.051%
24	14.334	1905	1912	1928	rBV	5546217	7751290	65.76%	7.090%
25	14.634	1956	1963	1972	rBV	3044511	4402581	37.35%	4.027%
26	14.751	1978	1983	1987	rBV8	7303	12762	0.11%	0.012%
27	14.845	1993	1999	2012	rBV	431691	693799	5.89%	0.635%
28	15.069	2034	2037	2041	rVB5	10957	14463	0.12%	0.013%
29	15.451	2096	2102	2106	rVB2	15512	21967	0.19%	0.020%
30	15.634	2124	2133	2141	rBV	7023972	9874256	83.77%	9.031%
31	15.757	2147	2154	2167	rBV	2425319	3149718	26.72%	2.881%
32	15.869	2169	2173	2180	rVB	31965	45058	0.38%	0.041%
33	16.363	2250	2257	2262	rBV7	11828	23864	0.20%	0.022%
34	17.075	2373	2378	2382	rBV8	9564	20197	0.17%	0.018%
35	17.192	2393	2398	2403	rBV6	9192	15980	0.14%	0.015%
36	17.404	2427	2434	2444	rBV	3822335	5168509	43.85%	4.727%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090723\
Data File : BP016998.D
Acq On : 07 Sep 2023 21:03
Operator : MA/JU
Sample : 04123-15
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH931

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Title : SVOA CALIBRATION

37	17.504	2444	2451	2466	rVV2	7738737	10717767	90.93%	9.803%
38	18.239	2572	2576	2584	rBV	97610	140129	1.19%	0.128%
39	19.310	2754	2758	2763	rBV2	87248	119879	1.02%	0.110%
40	19.380	2766	2770	2775	rVB	93024	129629	1.10%	0.119%
41	19.475	2783	2786	2791	rBV	96621	128289	1.09%	0.117%
42	19.616	2807	2810	2814	rBV	44885	52089	0.44%	0.048%
43	19.739	2825	2831	2837	rBV	9007772	11786675	100.00%	10.780%
44	21.504	3125	3131	3140	rBV	3602106	4782875	40.58%	4.375%
45	23.874	3526	3534	3545	rVB2	4918070	10092147	85.62%	9.231%
46	24.039	3555	3562	3572	rVB	2079058	4330538	36.74%	3.961%




Sum of corrected areas: 109334030

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090723\
Data File : BP016998.D
Acq On : 07 Sep 2023 21:03
Operator : MA/JU
Sample : 04123-15
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH931

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

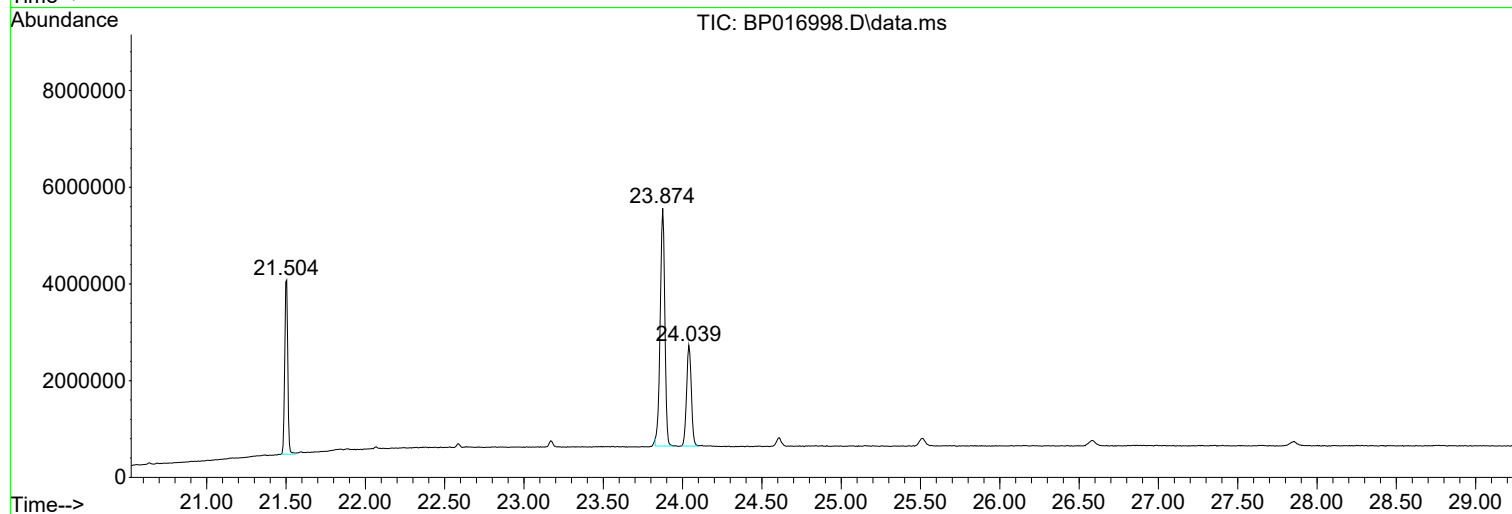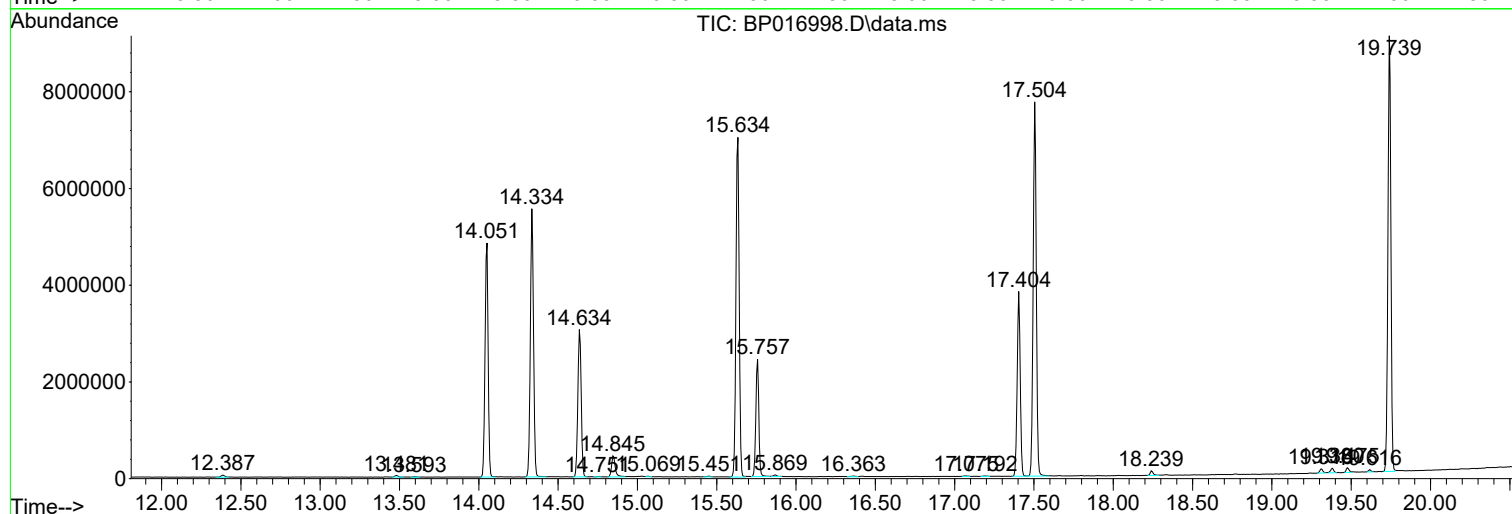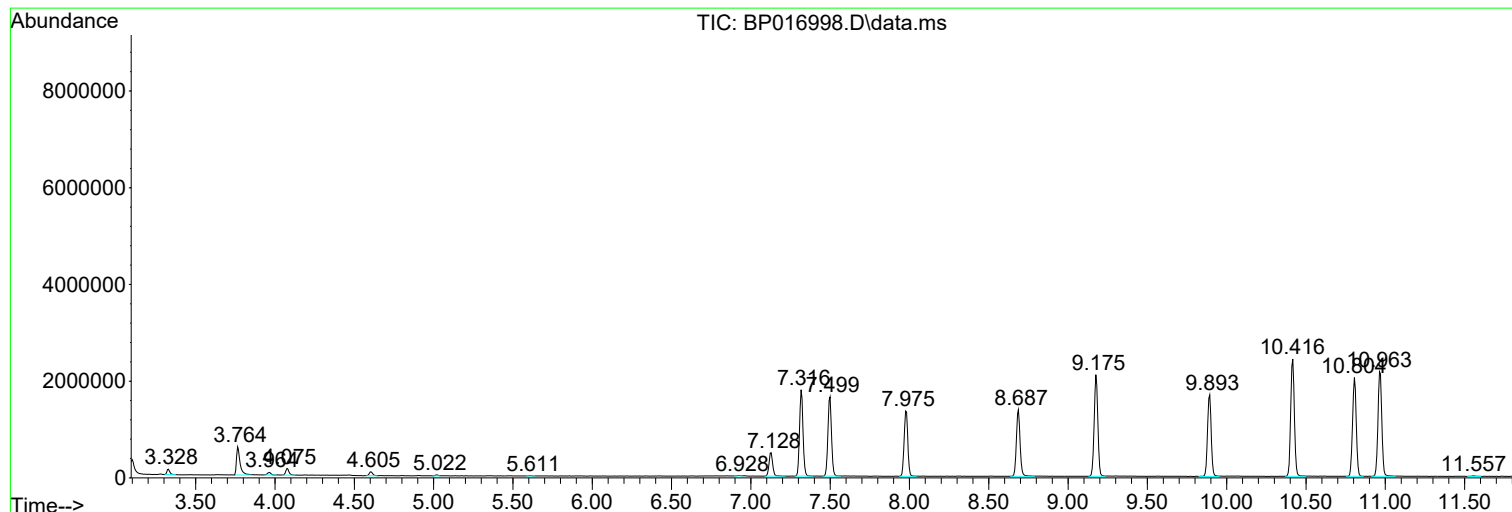

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090723\
Data File : BP016998.D
Acq On : 07 Sep 2023 21:03
Operator : MA/JU
Sample : 04123-15
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH931

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090723\
Data File : BP016998.D
Acq On : 07 Sep 2023 21:03
Operator : MA/JU
Sample : 04123-15
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH931

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc