

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090723\
 Data File : BP017000.D
 Acq On : 07 Sep 2023 22:12
 Operator : MA/JU
 Sample : 04123-17
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH9F9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017000.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.328	37	41	53	rVB	133713	194187	1.58%	0.164%
2	3.763	111	115	129	rBV	504323	811715	6.60%	0.686%
3	3.963	144	149	154	rBV	59866	90313	0.73%	0.076%
4	4.075	163	168	179	rVB	160788	232105	1.89%	0.196%
5	4.463	232	234	241	rVB7	12921	19335	0.16%	0.016%
6	4.604	252	258	269	rBV	270501	413564	3.36%	0.349%
7	5.016	324	328	333	rVB	18917	24840	0.20%	0.021%
8	5.604	423	428	434	rBV5	10719	17356	0.14%	0.015%
9	6.922	646	652	658	rBV6	10670	23333	0.19%	0.020%
10	7.122	680	686	699	rBV	559797	885621	7.20%	0.748%
11	7.316	712	719	731	rVB	2039633	3094076	25.16%	2.614%
12	7.498	742	750	762	rBV	1873989	2970411	24.15%	2.510%
13	7.975	824	831	841	rBV	1530054	2414688	19.63%	2.040%
14	8.687	944	952	964	rBV	1533042	2473489	20.11%	2.090%
15	9.175	1027	1035	1048	rBV	2386332	3817842	31.04%	3.226%
16	9.892	1148	1157	1172	rBV	1881586	3086614	25.10%	2.608%
17	10.416	1238	1246	1264	rBV	2667840	4376857	35.59%	3.698%
18	10.804	1304	1312	1322	rBV	2214306	3646817	29.65%	3.081%
19	10.963	1331	1339	1354	rBV	2490569	4154406	33.78%	3.510%
20	11.557	1434	1440	1449	rBV9	10770	22894	0.19%	0.019%
21	11.798	1475	1481	1494	rBV	93849	223816	1.82%	0.189%
22	12.386	1575	1581	1591	rVB2	46729	79452	0.65%	0.067%
23	13.481	1761	1767	1774	rBV2	29509	47840	0.39%	0.040%
24	13.598	1779	1787	1792	rBV5	9034	16687	0.14%	0.014%
25	14.051	1857	1864	1872	rBV	5040952	6860129	55.78%	5.796%
26	14.333	1904	1912	1922	rBV	5859530	8348721	67.88%	7.054%
27	14.633	1956	1963	1971	rBV	3394977	4820087	39.19%	4.073%
28	14.845	1993	1999	2014	rBV	452316	710104	5.77%	0.600%
29	15.016	2022	2028	2033	rVV9	10641	27929	0.23%	0.024%
30	15.069	2034	2037	2044	rVB8	8720	14720	0.12%	0.012%
31	15.422	2093	2097	2109	rVB4	16128	30839	0.25%	0.026%
32	15.633	2124	2133	2142	rBV	7263741	10334914	84.03%	8.732%
33	15.757	2148	2154	2163	rBV	2451952	3178997	25.85%	2.686%
34	15.869	2169	2173	2180	rVB	35450	49269	0.40%	0.042%
35	16.292	2239	2245	2253	rBV2	36445	82648	0.67%	0.070%
36	16.357	2253	2256	2262	rVV7	11072	19286	0.16%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090723\
 Data File : BP017000.D
 Acq On : 07 Sep 2023 22:12
 Operator : MA/JU
 Sample : 04123-17
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH9F9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
 Title : SVOA CALIBRATION

37	16.416	2262	2266	2270	rVV7	8632	13850	0.11%	0.012%
38	16.639	2300	2304	2309	rBV7	7635	13385	0.11%	0.011%
39	17.086	2373	2380	2383	rBV6	33258	59987	0.49%	0.051%
40	17.133	2383	2388	2392	rVB3	29417	45144	0.37%	0.038%
41	17.404	2427	2434	2443	rBV	3931480	5672928	46.12%	4.793%
42	17.504	2444	2451	2469	rVV	8137042	11151857	90.67%	9.422%
43	17.833	2504	2507	2512	rVB2	31960	34856	0.28%	0.029%
44	18.021	2536	2539	2545	rVB2	28626	37572	0.31%	0.032%
45	18.239	2572	2576	2586	rBV	233179	352530	2.87%	0.298%
46	18.504	2618	2621	2626	rBV3	28266	38804	0.32%	0.033%
47	19.310	2755	2758	2761	rBV2	80598	93907	0.76%	0.079%
48	19.374	2766	2769	2776	rVB	89243	128786	1.05%	0.109%
49	19.474	2782	2786	2792	rBV2	147667	195786	1.59%	0.165%
50	19.615	2807	2810	2815	rVB3	37873	48112	0.39%	0.041%
51	19.739	2825	2831	2843	rBV	9852967	12299557	100.00%	10.392%
52	21.168	3071	3074	3081	rVB2	106660	163592	1.33%	0.138%
53	21.498	3125	3130	3137	rBV	4256815	5251585	42.70%	4.437%
54	23.874	3525	3534	3545	rVB2	4869625	10398644	84.54%	8.786%
55	24.039	3555	3562	3571	rVB	2283116	4739711	38.54%	4.005%




Sum of corrected areas: 118356494

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090723\
Data File : BP017000.D
Acq On : 07 Sep 2023 22:12
Operator : MA/JU
Sample : 04123-17
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH9F9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

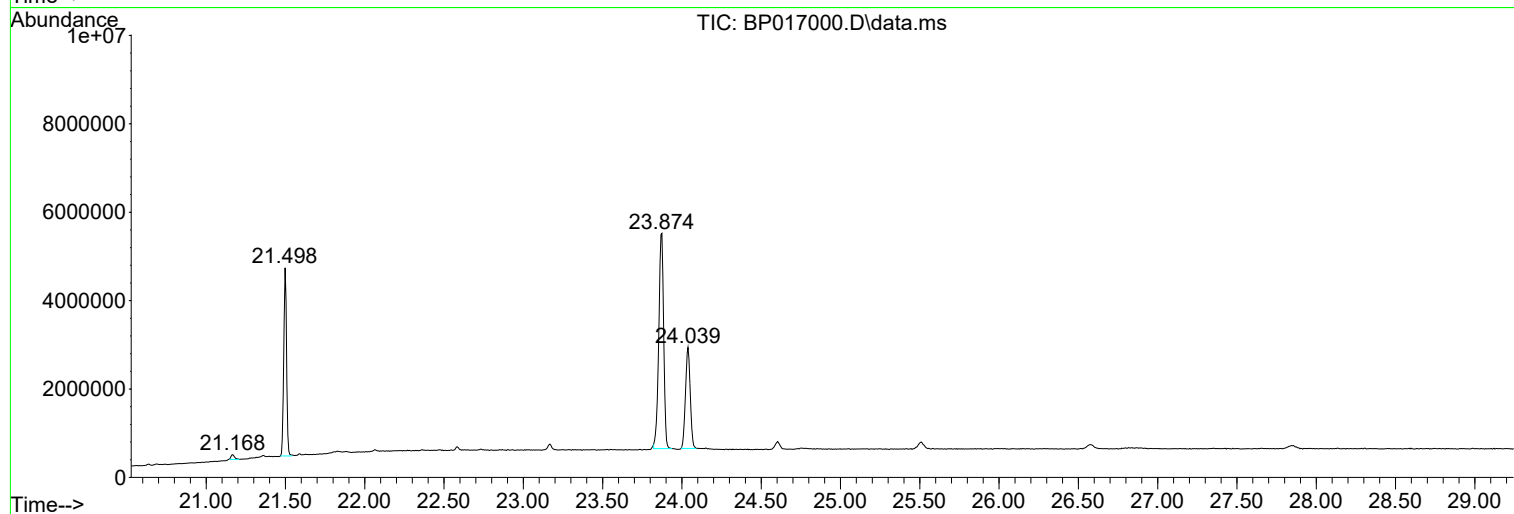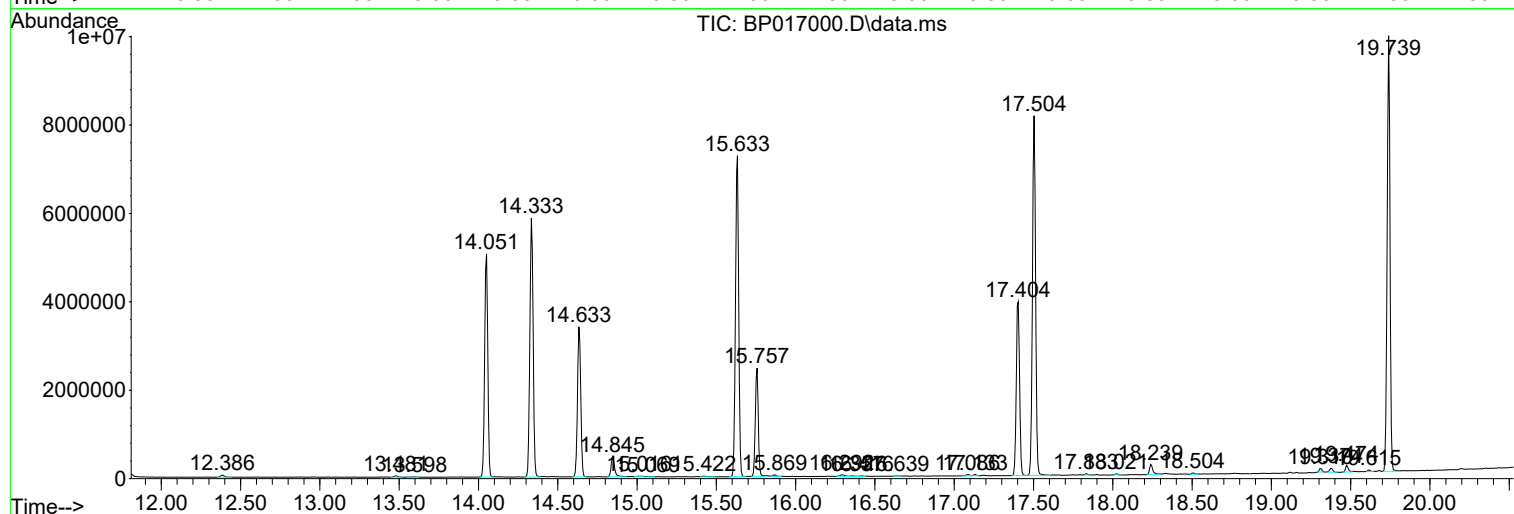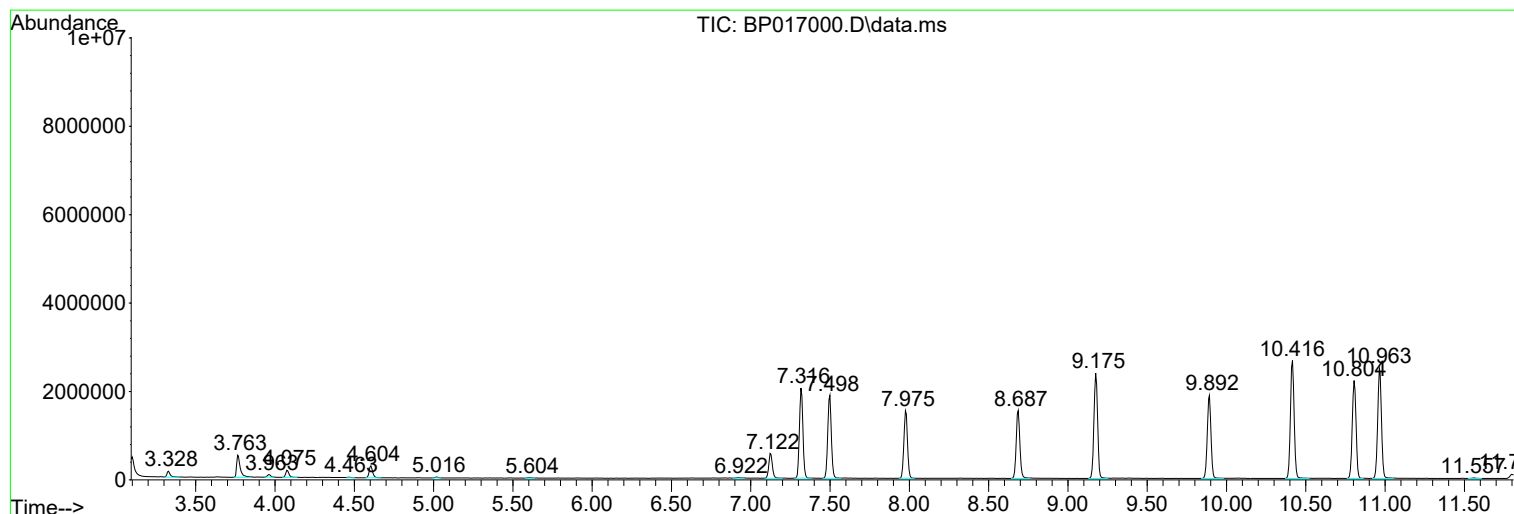

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090723\
Data File : BP017000.D
Acq On : 07 Sep 2023 22:12
Operator : MA/JU
Sample : 04123-17
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH9F9










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.604	3.43 ng/ul	413564	1,4-Dichlorobenzene-d4	7.975

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
5			Pyrimidine, 5-fluoro-2,4-dichloro-	166	C4HC12FN2	002927-71-1	38

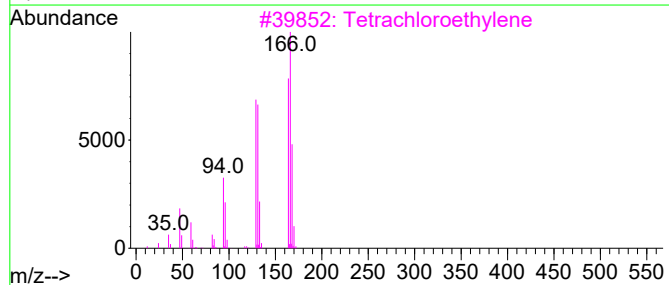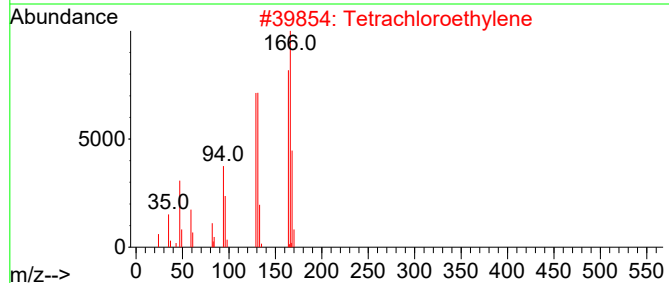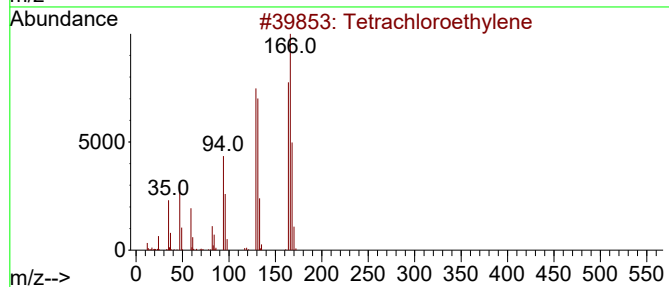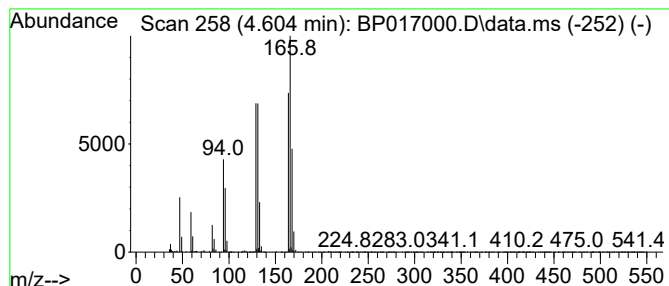

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090723\
Data File : BP017000.D
Acq On : 07 Sep 2023 22:12
Operator : MA/JU
Sample : 04123-17
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH9F9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.604	3.4	ng/ul	413564	1	7.975	2414690	20.0