

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090723\
 Data File : BP017001.D
 Acq On : 07 Sep 2023 22:47
 Operator : MA/JU
 Sample : 04166-16
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBJP0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017001.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.281	29	33	37	rVB2	36557	49612	0.47%	0.046%
2	3.328	37	41	45	rBV	115238	142685	1.34%	0.132%
3	3.640	90	94	97	rBV6	7589	13385	0.13%	0.012%
4	3.764	111	115	133	rBV	467198	729510	6.86%	0.673%
5	3.964	144	149	156	rVB	70378	106959	1.01%	0.099%
6	4.075	164	168	174	rVB	24637	37174	0.35%	0.034%
7	4.240	192	196	202	rBV9	5047	11105	0.10%	0.010%
8	4.464	230	234	240	rVB7	9423	17732	0.17%	0.016%
9	4.605	251	258	270	rBV	4286906	6101422	57.36%	5.629%
10	5.016	324	328	332	rVB	21750	29031	0.27%	0.027%
11	5.605	424	428	431	rBV3	8552	12503	0.12%	0.012%
12	6.928	648	653	654	rBV4	8369	12813	0.12%	0.012%
13	7.122	680	686	696	rBV	558829	861473	8.10%	0.795%
14	7.316	711	719	730	rBV	1893368	2833407	26.64%	2.614%
15	7.499	742	750	760	rBV	1741464	2757520	25.92%	2.544%
16	7.587	760	765	770	rVB5	12476	22091	0.21%	0.020%
17	7.975	824	831	842	rBV	1471823	2279820	21.43%	2.103%
18	8.687	943	952	963	rBV	1391811	2320230	21.81%	2.141%
19	9.175	1027	1035	1047	rBV	2165041	3453443	32.47%	3.186%
20	9.393	1066	1072	1079	rVB	91587	142653	1.34%	0.132%
21	9.887	1149	1156	1167	rBV	1648390	2717043	25.54%	2.507%
22	10.416	1236	1246	1260	rBV	2333434	3895393	36.62%	3.594%
23	10.804	1304	1312	1322	rBV	2069636	3363256	31.62%	3.103%
24	10.963	1330	1339	1351	rBV	2308746	3769862	35.44%	3.478%
25	11.557	1434	1440	1448	rBV7	9773	18028	0.17%	0.017%
26	11.887	1490	1496	1502	rVB	78301	121066	1.14%	0.112%
27	12.387	1574	1581	1588	rVB	41596	67888	0.64%	0.063%
28	13.392	1747	1752	1755	rBV4	9942	14538	0.14%	0.013%
29	13.481	1759	1767	1772	rBV3	51476	89503	0.84%	0.083%
30	13.598	1782	1787	1792	rVB7	8944	15305	0.14%	0.014%
31	13.816	1819	1824	1828	rBV8	7116	12258	0.12%	0.011%
32	13.875	1828	1834	1838	rBV2	26298	39491	0.37%	0.036%
33	14.045	1857	1863	1873	rBV	4377625	6168657	57.99%	5.691%
34	14.334	1905	1912	1927	rBV	5209079	7268928	68.33%	6.706%
35	14.528	1937	1945	1954	rBV	106268	155377	1.46%	0.143%
36	14.634	1956	1963	1971	rVB	3017299	4308081	40.50%	3.974%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090723\
 Data File : BP017001.D
 Acq On : 07 Sep 2023 22:47
 Operator : MA/JU
 Sample : 04166-16
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBJP0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
 Title : SVOA CALIBRATION

37	14.845	1993	1999	2012	rBV	451530	713474	6.71%	0.658%
38	15.063	2033	2036	2041	rVB6	13174	19009	0.18%	0.018%
39	15.445	2096	2101	2105	rVB6	11981	18840	0.18%	0.017%
40	15.634	2125	2133	2140	rBV	6390460	9210943	86.59%	8.497%
41	15.757	2147	2154	2162	rBV	2125348	2918319	27.43%	2.692%
42	15.863	2168	2172	2177	rVB	26917	37322	0.35%	0.034%
43	16.345	2247	2254	2259	rBV	62620	96430	0.91%	0.089%
44	17.069	2372	2377	2382	rBV8	10194	18178	0.17%	0.017%
45	17.186	2393	2397	2404	rBV6	10727	23903	0.22%	0.022%
46	17.404	2427	2434	2444	rBV	3369832	4785802	44.99%	4.415%
47	17.504	2444	2451	2464	rBV	7384606	10152550	95.44%	9.366%
48	17.898	2514	2518	2522	rBV3	10038	16278	0.15%	0.015%
49	18.022	2536	2539	2544	rVB3	25552	34736	0.33%	0.032%
50	18.239	2572	2576	2584	rBV	124162	171154	1.61%	0.158%
51	19.157	2729	2732	2739	rVB4	59948	72553	0.68%	0.067%
52	19.310	2754	2758	2762	rBV	79467	103596	0.97%	0.096%
53	19.375	2766	2769	2774	rVB	75338	102470	0.96%	0.095%
54	19.475	2782	2786	2793	rBV2	91497	123388	1.16%	0.114%
55	19.616	2807	2810	2815	rBV2	34494	38632	0.36%	0.036%
56	19.739	2825	2831	2843	rBV	8704490	10637288	100.00%	9.813%
57	21.498	3125	3130	3137	rBV	3007231	3805942	35.78%	3.511%
58	23.868	3526	3533	3550	rVB2	4019731	8021723	75.41%	7.400%
59	24.033	3555	3561	3570	rVB	1566298	3314157	31.16%	3.057%




Sum of corrected areas: 108395929

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090723\
Data File : BP017001.D
Acq On : 07 Sep 2023 22:47
Operator : MA/JU
Sample : 04166-16
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJP0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

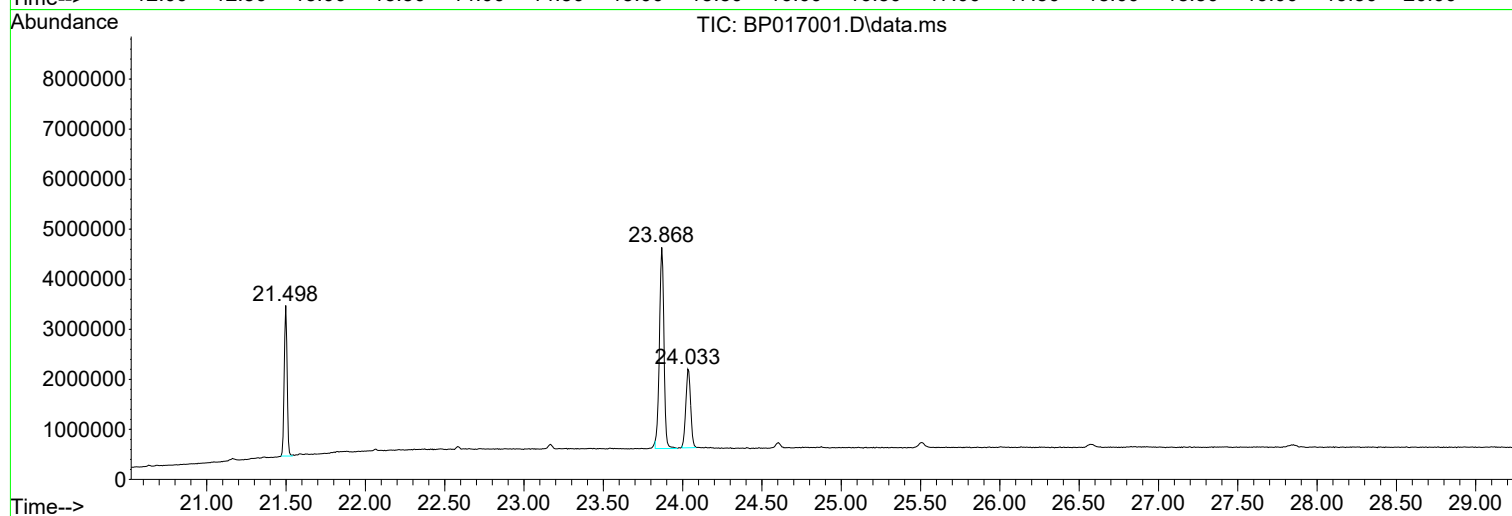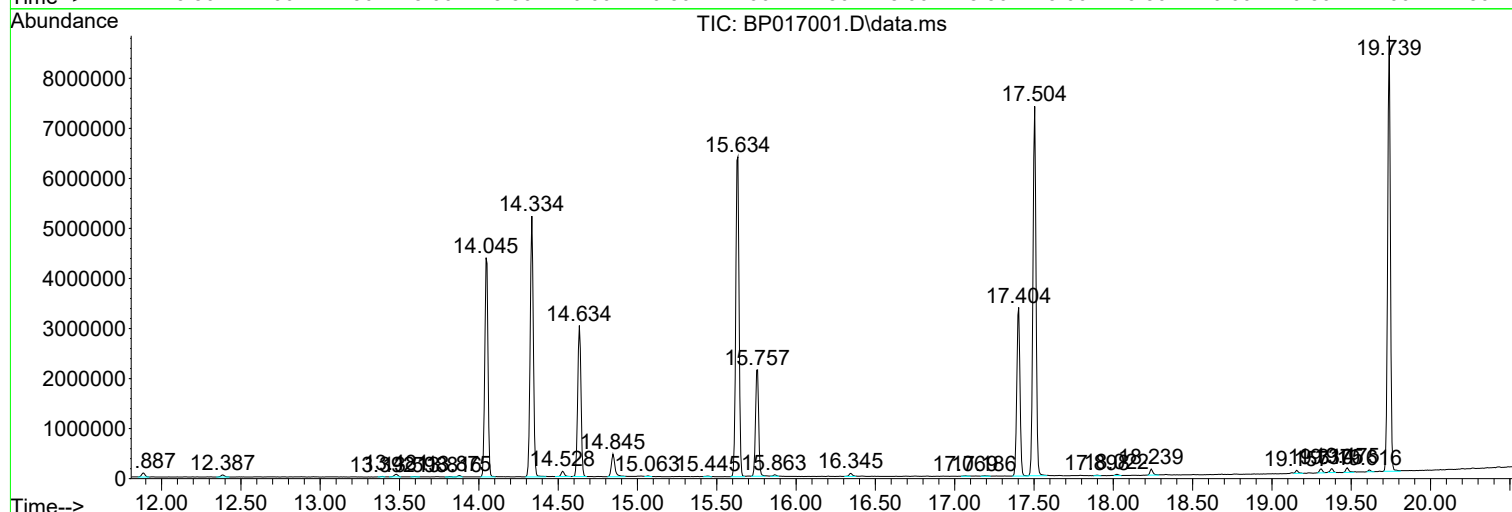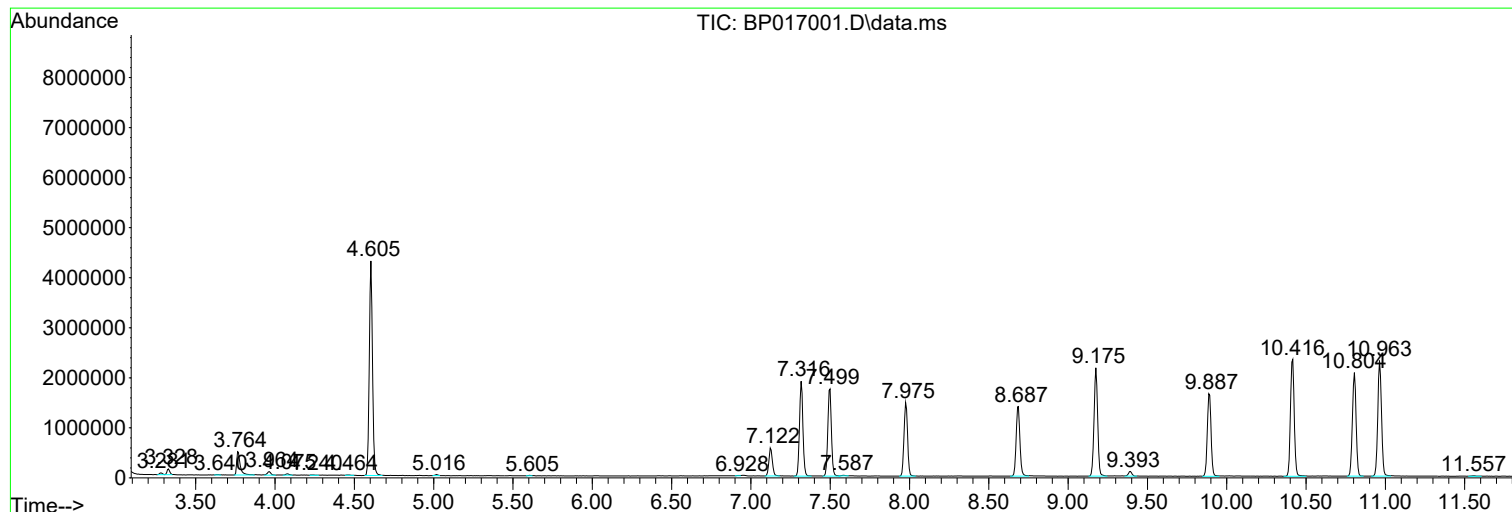

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090723\
Data File : BP017001.D
Acq On : 07 Sep 2023 22:47
Operator : MA/JU
Sample : 04166-16
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJP0










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.605	53.53 ng/ul	6101420	1,4-Dichlorobenzene-d4	7.975

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	95
5			Pyrimidine, 5-fluoro-2,4-dichloro-	166	C4HC12FN2	002927-71-1	35

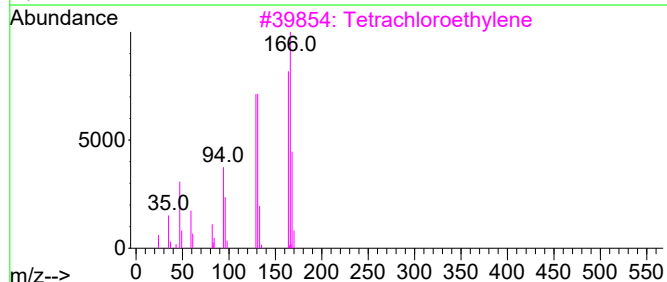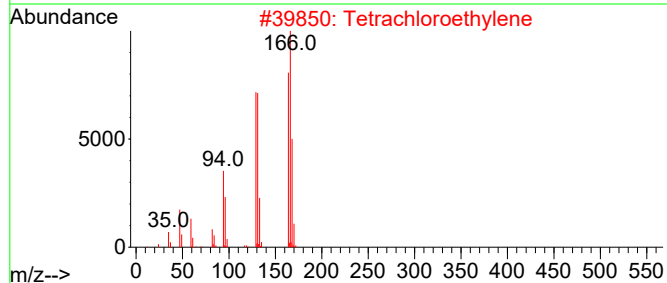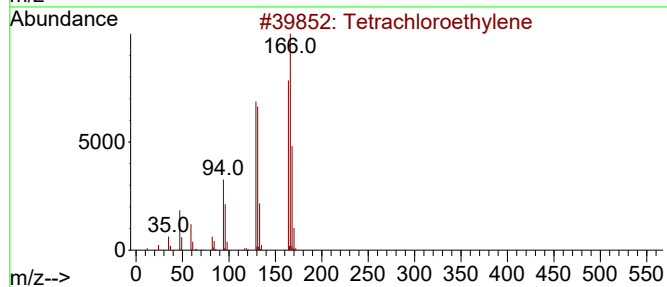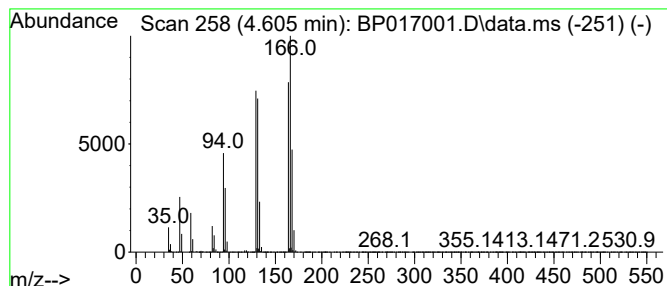

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090723\
Data File : BP017001.D
Acq On : 07 Sep 2023 22:47
Operator : MA/JU
Sample : 04166-16
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJP0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.605	53.5	ng/ul	6101420	1	7.975	2279820	20.0