

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
 Data File : BP017017.D
 Acq On : 08 Sep 2023 17:57
 Operator : MA/JU
 Sample : 04166-17
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBJX4

Quant Time: Sep 09 00:45:12 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 06 01:52:05 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.975	152	432077	20.000	ng/ul	0.00
20) Naphthalene-d8	10.804	136	1876133	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.634	164	1121137	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.398	188	2287773	20.000	ng/ul	-0.01
79) Chrysene-d12	21.498	240	1654019	20.000	ng/ul	-0.01
88) Perylene-d12	24.033	264	1484449	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.328	96	76230	6.673	ng/uL	0.00
4) Pyridine-d5	3.764	84	371782	11.391	ng/ul	0.00
7) Phenol-d5	7.122	99	415513	10.526	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.316	67	1153642	46.722	ng/ul	0.00
11) 2-Chlorophenol-d4	7.493	132	1057086	37.001	ng/ul	-0.01
15) 4-Methylphenol-d8	8.681	113	732733	24.365	ng/ul	-0.01
21) Nitrobenzene-d5	9.175	128	665328	45.711	ng/ul	0.00
24) 2-Nitrophenol-d4	9.887	143	702835	44.545	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.410	165	1160207	39.830	ng/ul	-0.01
31) 4-Chloroaniline-d4	10.963	131	1414912	33.667	ng/ul	0.00
46) Dimethylphthalate-d6	14.045	166	3896573	46.691	ng/ul	0.00
49) Acenaphthylene-d8	14.334	160	4371278	45.387	ng/ul	0.00
54) 4-Nitrophenol-d4	14.845	143	135635	8.320	ng/ul	-0.01
60) Fluorene-d10	15.628	176	3290092	46.046	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.751	200	540374	39.249	ng/ul	-0.01
73) Anthracene-d10	17.504	188	4973423	47.337	ng/ul	0.00
81) Pyrene-d10	19.739	212	5351623	53.120	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.868	264	3744695	49.724	ng/ul	-0.01
Target Compounds						
34) Caprolactam	11.798	113	20731	2.109	ng/ul	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017017.D
Acq On : 08 Sep 2023 17:57
Operator : MA/JU
Sample : 04166-17
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJX4

Quant Time: Sep 09 00:45:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 06 01:52:05 2023
Response via : Initial Calibration

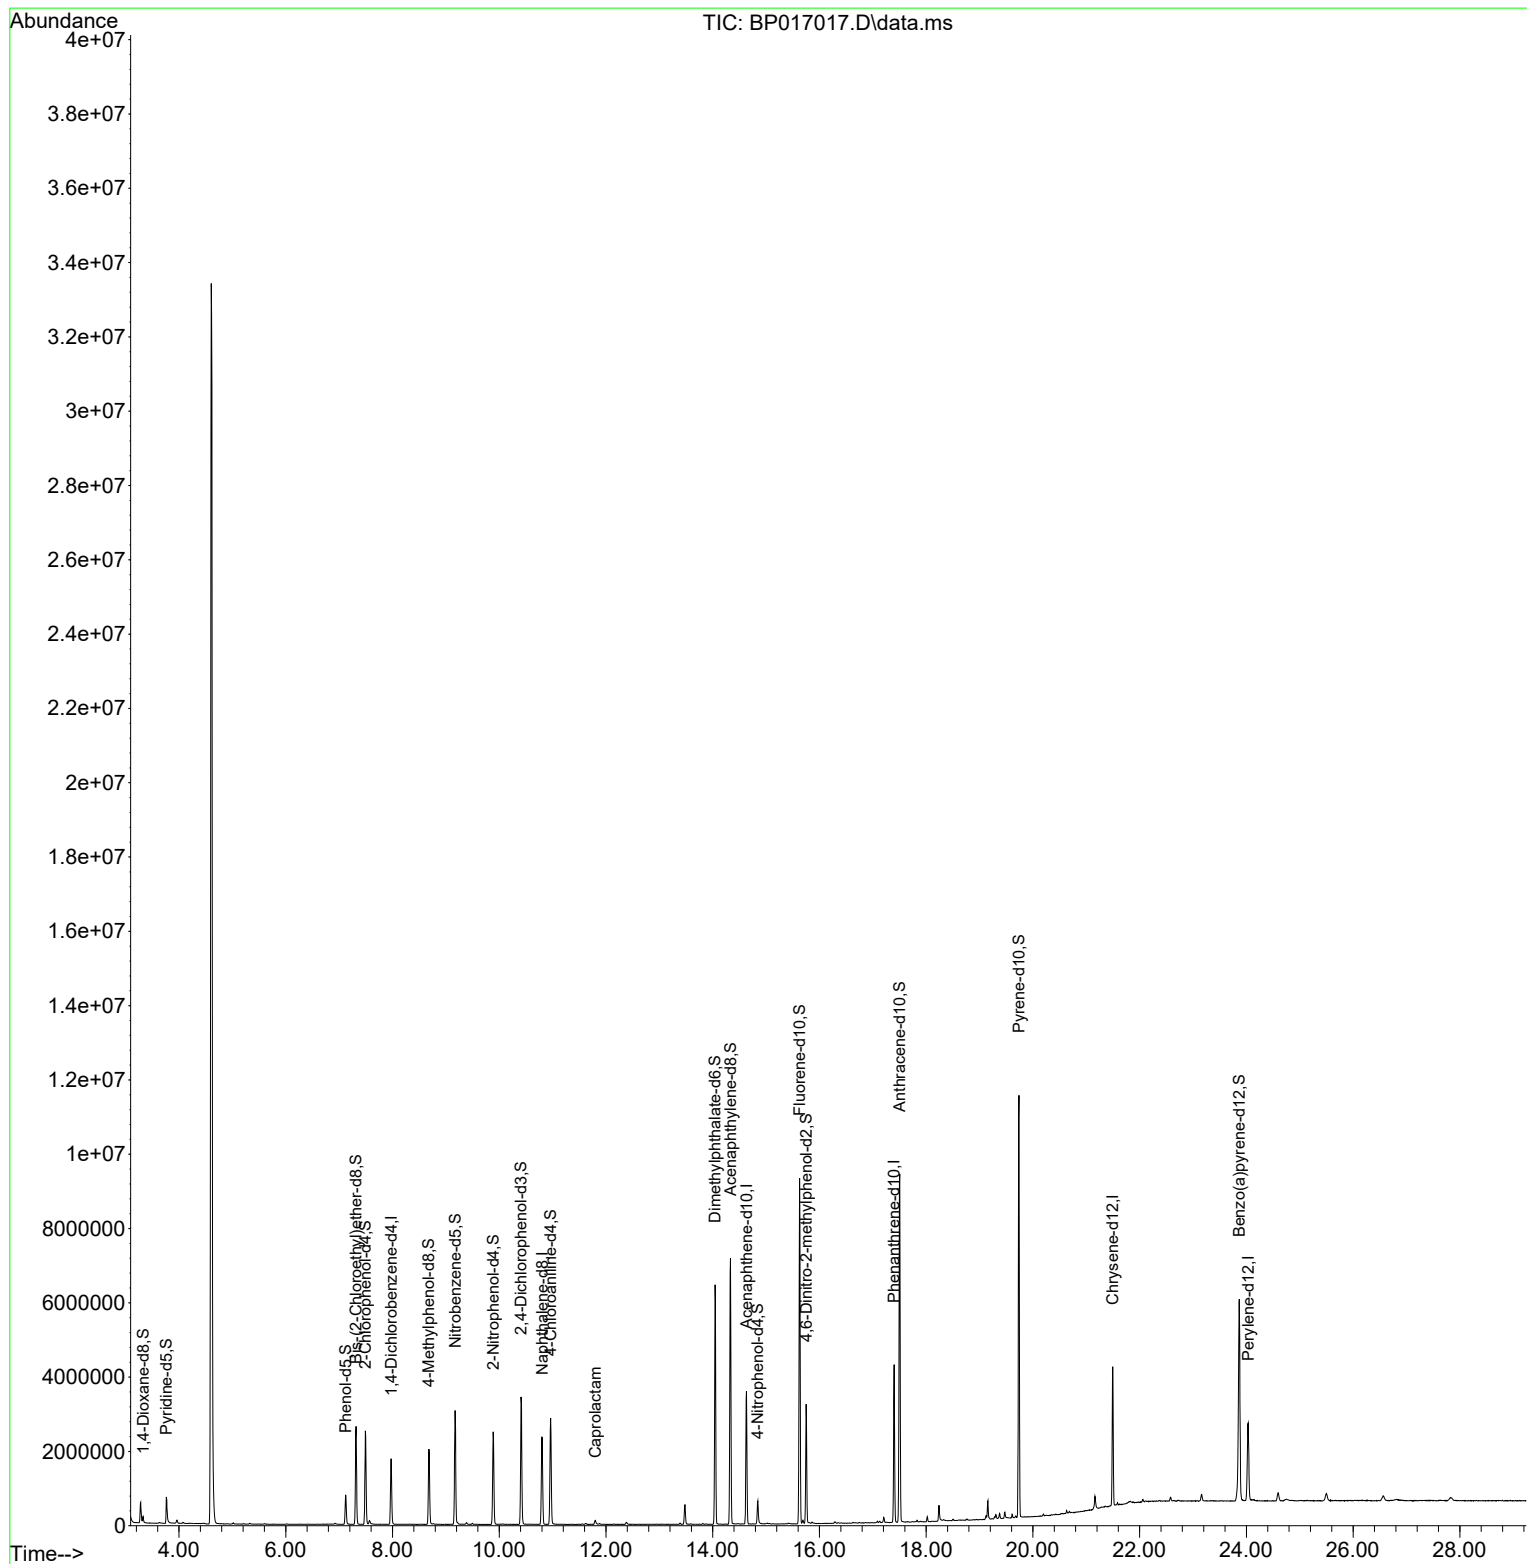

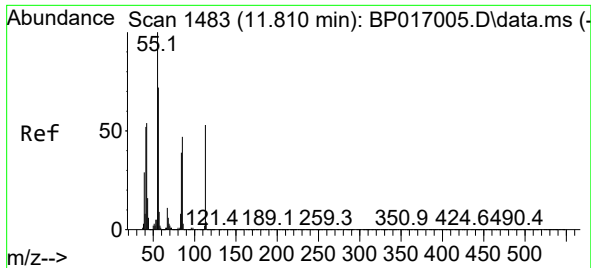

#34
Caprolactam
Concen: 2.109 ng/ul
RT: 11.798 min Scan# 14
Delta R.T. -0.011 min
Lab File: BP017017.D
Acq: 08 Sep 2023 17:57

Instrument :
BNA_P
ClientSampleId :
BBJX4

Tgt Ion:113 Resp: 20731
Ion Ratio Lower Upper
113 100
55 176.9 142.3 213.5
56 124.6 102.2 153.2

