

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
 Data File : BP017047.D
 Acq On : 09 Sep 2023 12:17
 Operator : MA/JU
 Sample : 04227-07
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH9X8

Quant Time: Sep 09 23:05:04 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 09 01:41:21 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.969	152	335378	20.000	ng/u1	0.00
20) Naphthalene-d8	10.799	136	1462755	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.628	164	890081	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.392	188	1917060	20.000	ng/u1	0.00
79) Chrysene-d12	21.492	240	1580397	20.000	ng/u1	0.00
88) Perylene-d12	24.021	264	1646702	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.322	96	50911	5.742	ng/uL	0.00
4) Pyridine-d5	3.764	84	329512	13.006	ng/u1	0.00
7) Phenol-d5	7.116	99	222492	7.261	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.310	67	753882	39.335	ng/u1	0.00
11) 2-Chlorophenol-d4	7.493	132	641619	28.934	ng/u1	0.00
15) 4-Methylphenol-d8	8.675	113	435090	18.639	ng/u1	-0.01
21) Nitrobenzene-d5	9.169	128	432215	38.087	ng/u1	0.00
24) 2-Nitrophenol-d4	9.881	143	441837	35.917	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.404	165	751016	33.068	ng/u1	0.00
31) 4-Chloroaniline-d4	10.957	131	1040033	31.741	ng/u1	0.00
46) Dimethylphthalate-d6	14.045	166	3042912	45.927	ng/u1	0.00
49) Acenaphthylene-d8	14.328	160	3214836	42.044	ng/u1	0.00
54) 4-Nitrophenol-d4	14.845	143	79303	6.128	ng/u1	0.00
60) Fluorene-d10	15.622	176	2554547	45.032	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.751	200	416125	36.069	ng/u1	0.00
73) Anthracene-d10	17.498	188	4227426	48.017	ng/u1	0.00
81) Pyrene-d10	19.733	212	4753154	49.377	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.863	264	4081304	48.854	ng/u1	0.00
Target Compounds						
2) 1,4-Dioxane	3.364	88	9658	1.009	ng/uL	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017047.D
Acq On : 09 Sep 2023 12:17
Operator : MA/JU
Sample : 04227-07
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH9X8

Quant Time: Sep 09 23:05:04 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 09 01:41:21 2023
Response via : Initial Calibration

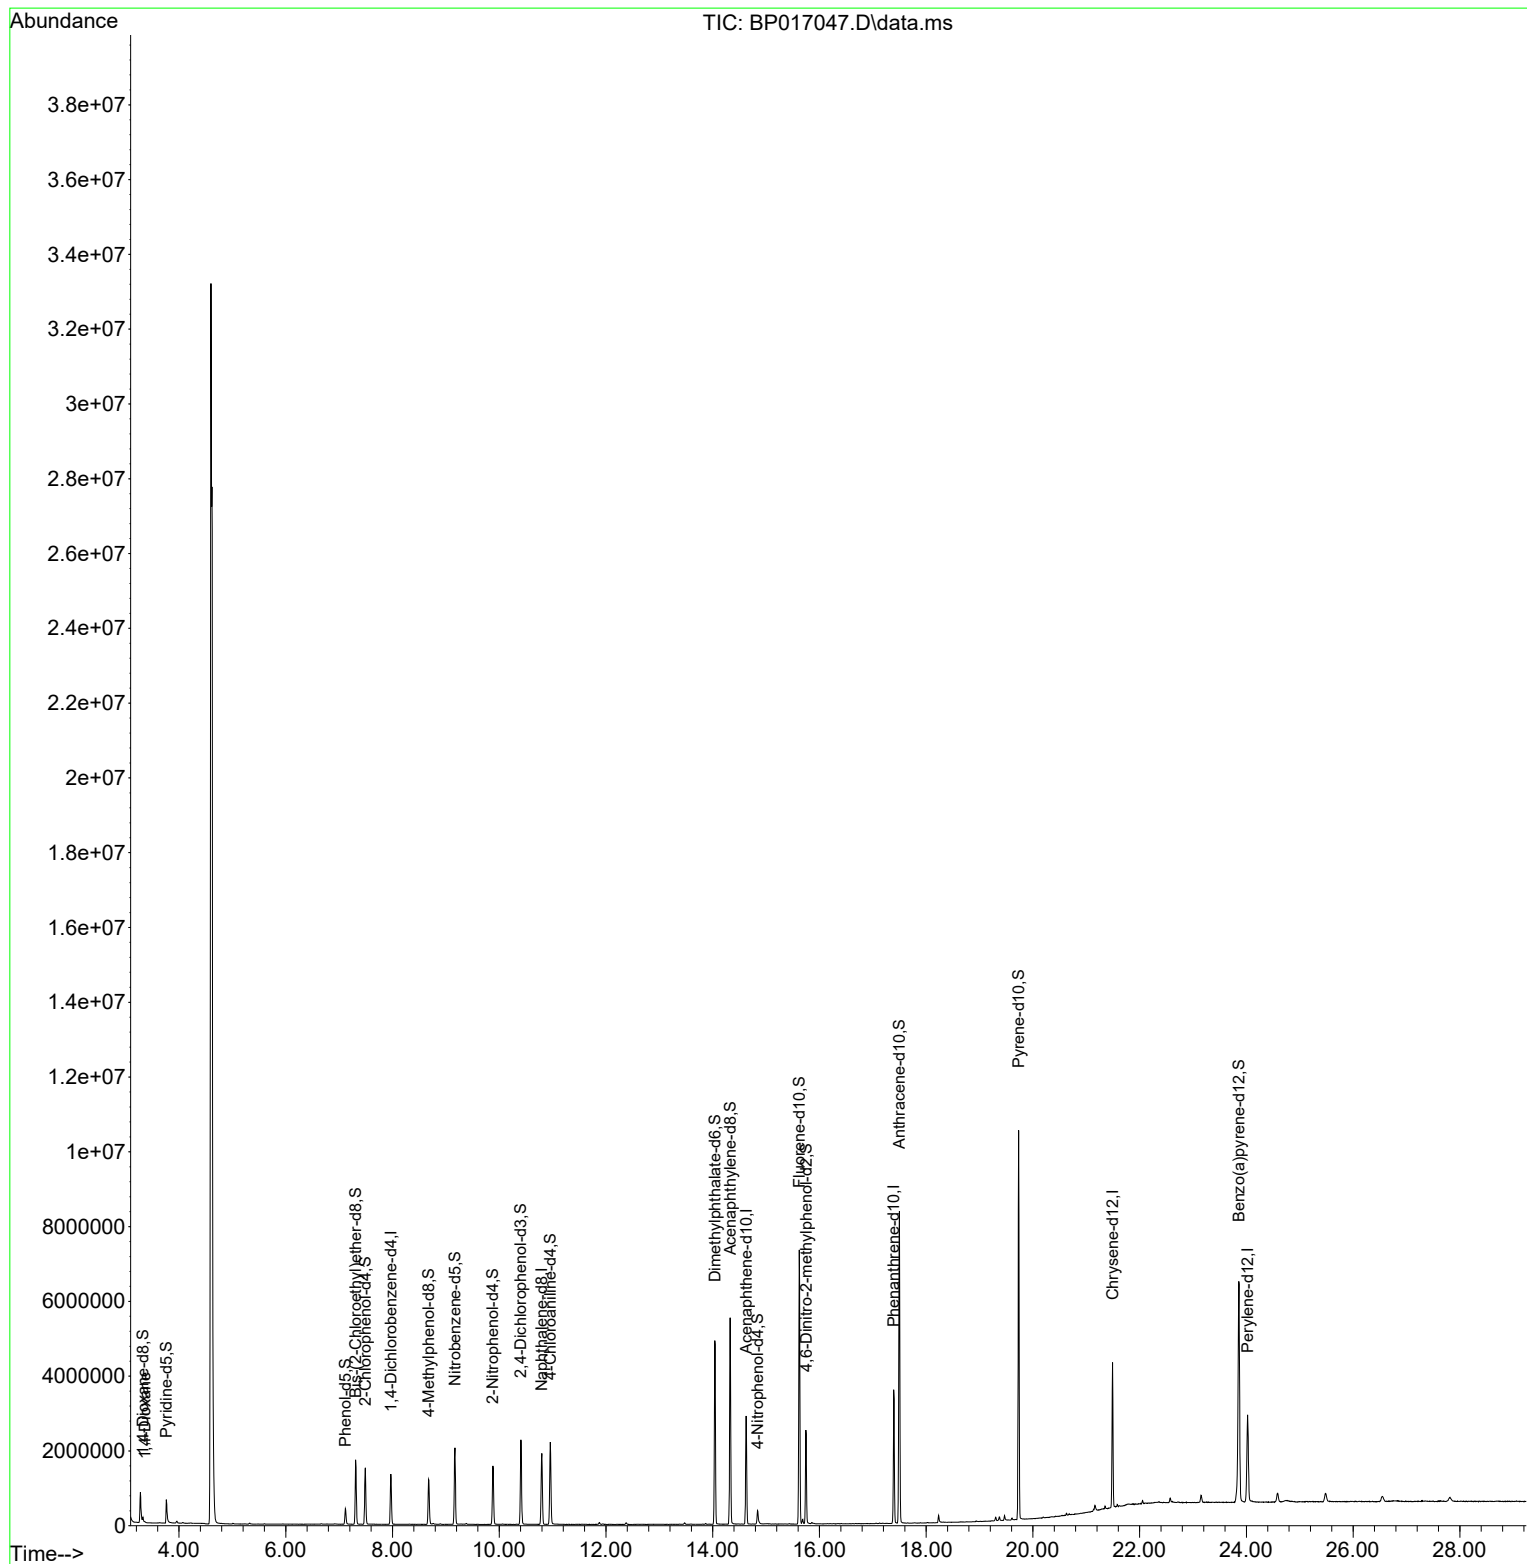

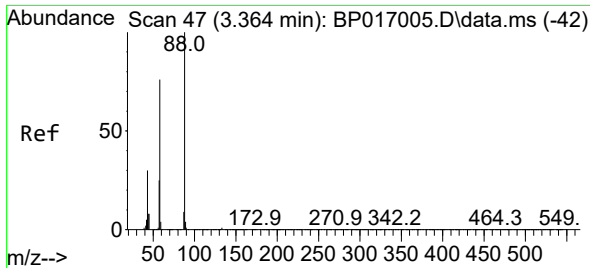

#2
 1,4-Dioxane
 Concen: 1.009 ng/uL
 RT: 3.364 min Scan# 41
 Delta R.T. -0.000 min
 Lab File: BP017047.D
 Acq: 09 Sep 2023 12:17

Instrument :
 BNA_P
 ClientSampleId :
 BH9X8

Tgt Ion: 88 Resp: 9658
 Ion Ratio Lower Upper
 88 100
 43 36.4 25.0 37.6
 58 70.4 60.6 90.8

