




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
 Data File : BP017027.D
 Acq On : 09 Sep 2023 00:17
 Operator : MA/JU
 Sample : 04153-06
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH464

Manual IntegrationsAPPROVED

Quant Time: Sep 09 04:21:06 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 09 01:41:21 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/09/2023
 Supervised By :mohammad ahmed 09/10/2023

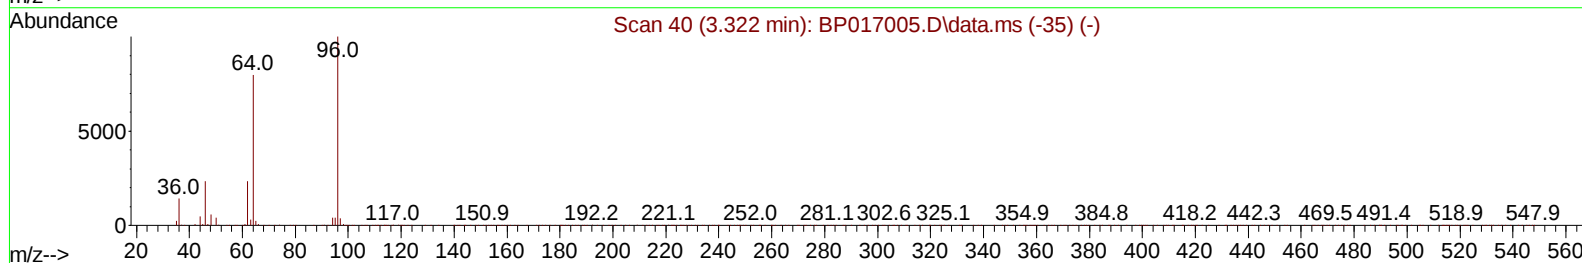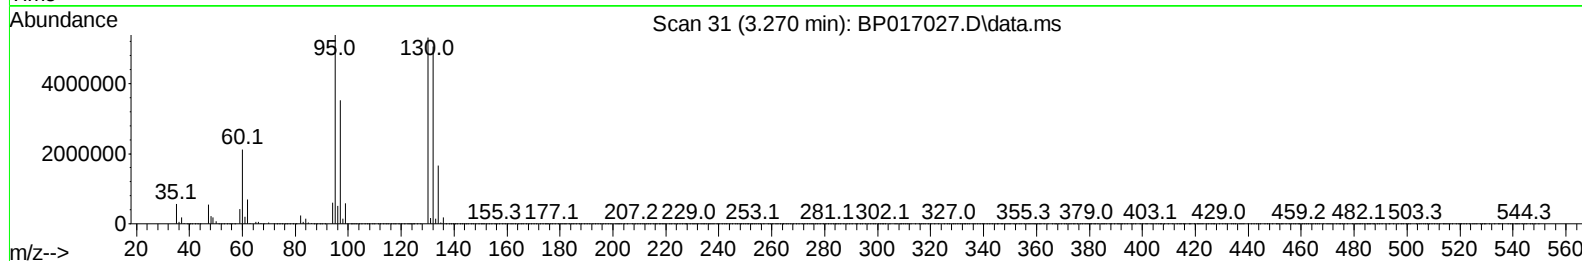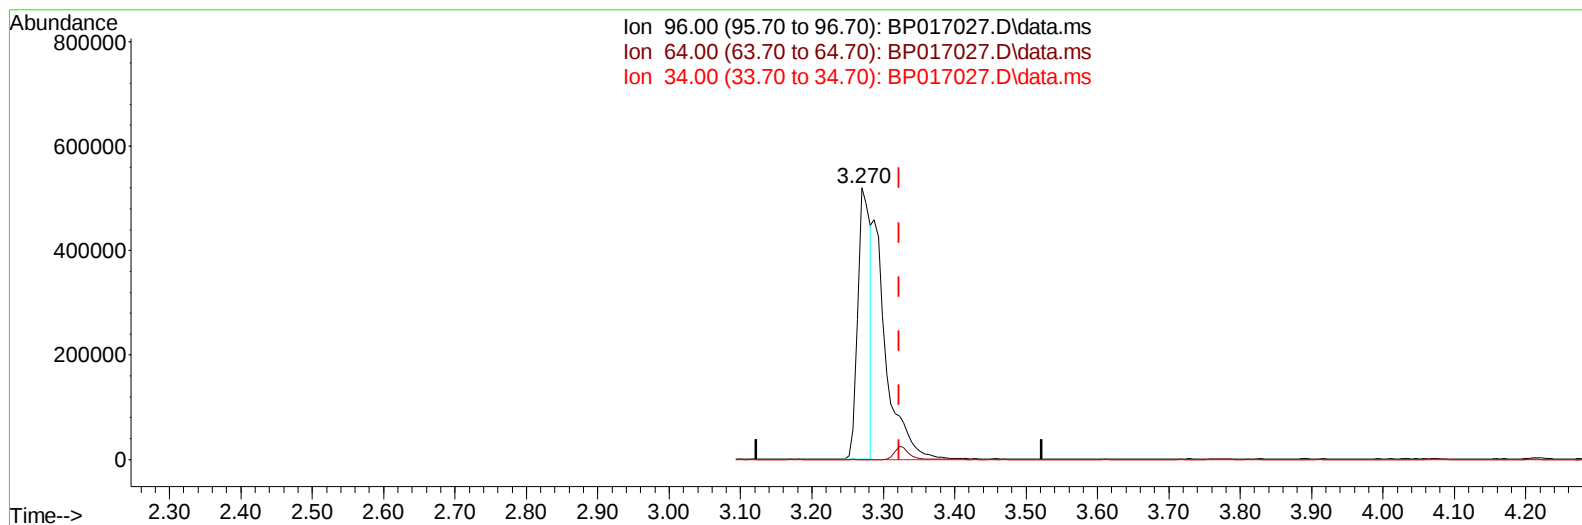

TIC: BP017027.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.270min (-0.053) 68.31 ng/uL

response 630615

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	74.60	0.00#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
 Data File : BP017027.D
 Acq On : 09 Sep 2023 00:17
 Operator : MA/JU
 Sample : 04153-06
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH464

Manual IntegrationsAPPROVED

Quant Time: Sep 09 04:21:06 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 09 01:41:21 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/09/2023
 Supervised By :mohammad ahmed 09/10/2023

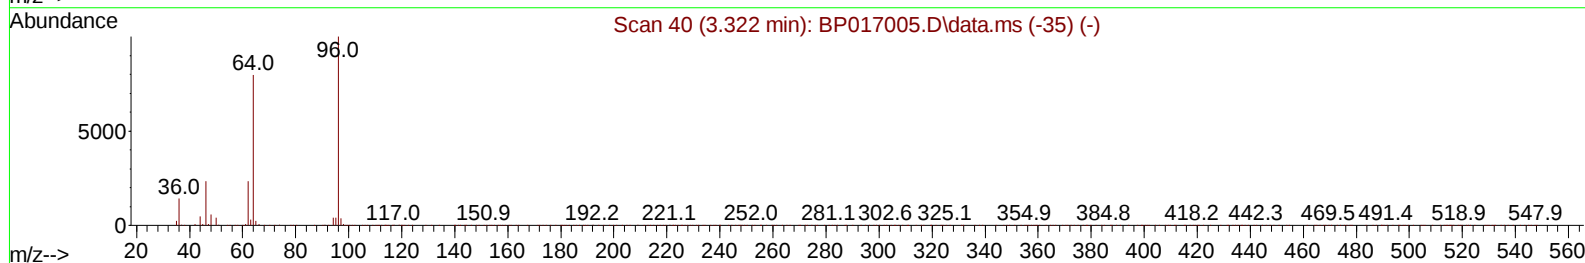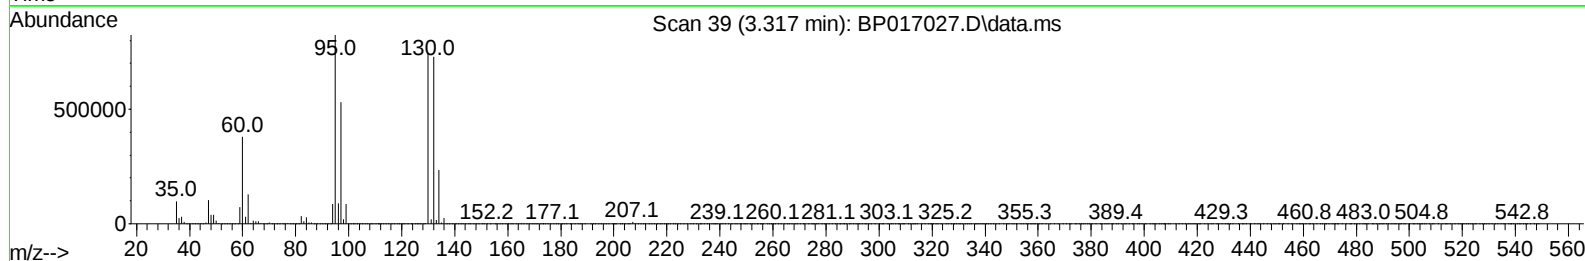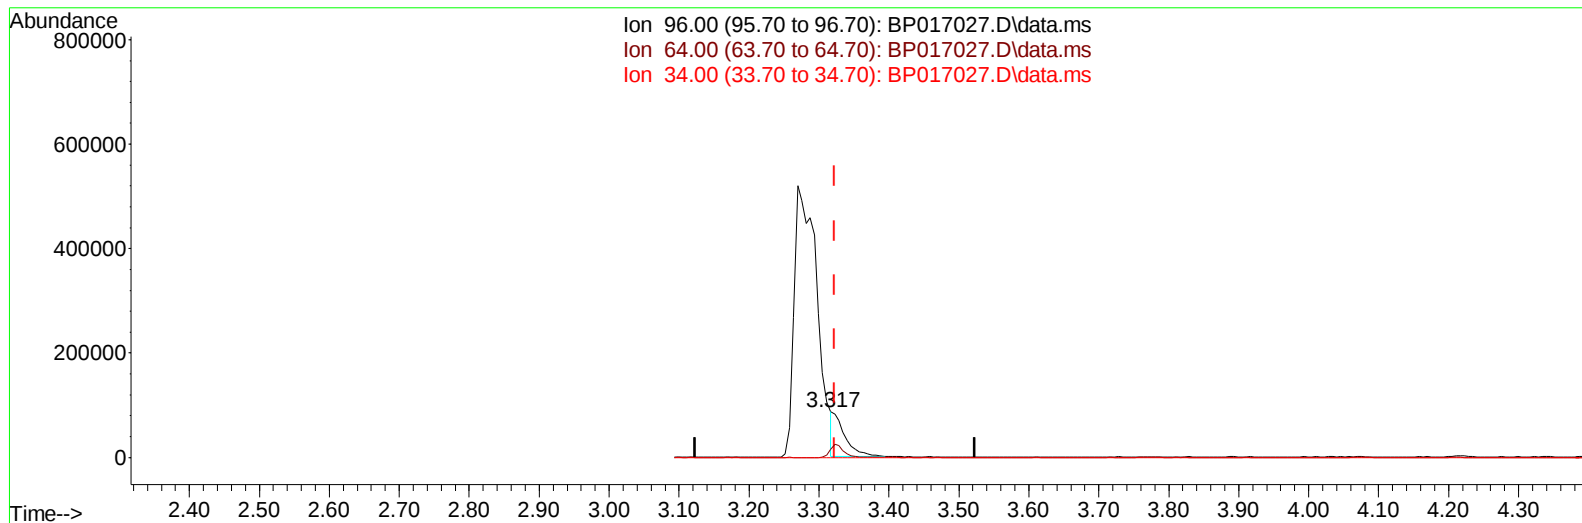

TIC: BP017027.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.317min (-0.006) 10.97 ng/uL m

response 101301

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	74.60	17.07#
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
 Data File : BP017027.D
 Acq On : 09 Sep 2023 00:17
 Operator : MA/JU
 Sample : 04153-06
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH464

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 09/09/2023
 Supervised By :mohammad ahmed 09/10/2023

Quant Time: Sep 09 04:36:36 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 09 01:41:21 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.975	152	349199	20.000	ng/ul	0.00
20) Naphthalene-d8	10.799	136	1532858	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.634	164	916645	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.398	188	1872070	20.000	ng/ul	0.00
79) Chrysene-d12	21.492	240	1333048	20.000	ng/ul	# 0.00
88) Perylene-d12	24.027	264	1245580	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.317	96	101301m	10.973	ng/uL	0.00
4) Pyridine-d5	3.764	84	354134	13.425	ng/ul	0.00
7) Phenol-d5	7.122	99	258737	8.110	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.311	67	693084	34.732	ng/ul	0.00
11) 2-Chlorophenol-d4	7.493	132	618124	26.771	ng/ul	0.00
15) 4-Methylphenol-d8	8.681	113	445313	18.322	ng/ul	0.00
21) Nitrobenzene-d5	9.169	128	385611	32.426	ng/ul	0.00
24) 2-Nitrophenol-d4	9.887	143	403447	31.296	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.410	165	679352	28.545	ng/ul	0.00
31) 4-Chloroaniline-d4	10.963	131	1107189	32.245	ng/ul	0.00
46) Dimethylphthalate-d6	14.046	166	2387763	34.994	ng/ul	0.00
49) Acenaphthylene-d8	14.328	160	2573819	32.686	ng/ul	0.00
54) 4-Nitrophenol-d4	14.845	143	73969	5.550	ng/ul	0.00
60) Fluorene-d10	15.628	176	1974736	33.802	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.751	200	293571	26.058	ng/ul	0.00
73) Anthracene-d10	17.498	188	3079276	35.817	ng/ul	0.00
81) Pyrene-d10	19.733	212	3340600	41.143	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.863	264	2385817	37.756	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017027.D
Acq On : 09 Sep 2023 00:17
Operator : MA/JU
Sample : 04153-06
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH464

Manual IntegrationsAPPROVED

Quant Time: Sep 09 04:36:36 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 09 01:41:21 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/09/2023
Supervised By :mohammad ahmed 09/10/2023

