

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
 Data File : BP017015.D
 Acq On : 08 Sep 2023 16:47
 Operator : MA/JU
 Sample : 04123-17
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH9F9

Quant Time: Sep 09 00:44:50 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 06 01:52:05 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.975	152	441717	20.000	ng/ul	0.00
20) Naphthalene-d8	10.804	136	1923291	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.634	164	1161996	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.398	188	2457929	20.000	ng/ul	-0.01
79) Chrysene-d12	21.498	240	1948734	20.000	ng/ul	-0.01
88) Perylene-d12	24.033	264	1903250	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.322	96	73234	6.271	ng/uL	0.00
4) Pyridine-d5	3.764	84	315446	9.454	ng/ul	0.00
7) Phenol-d5	7.122	99	349035	8.649	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.316	67	1009335	39.986	ng/ul	0.00
11) 2-Chlorophenol-d4	7.493	132	912128	31.230	ng/ul	-0.01
15) 4-Methylphenol-d8	8.681	113	626285	20.371	ng/ul	-0.01
21) Nitrobenzene-d5	9.175	128	582594	39.045	ng/ul	0.00
24) 2-Nitrophenol-d4	9.887	143	617549	38.180	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.410	165	1013816	33.951	ng/ul	-0.01
31) 4-Chloroaniline-d4	10.963	131	1362642	31.629	ng/ul	0.00
46) Dimethylphthalate-d6	14.051	166	3418649	39.524	ng/ul	0.00
49) Acenaphthylene-d8	14.334	160	3906399	39.134	ng/ul	0.00
54) 4-Nitrophenol-d4	14.845	143	109426	6.476	ng/ul	-0.01
60) Fluorene-d10	15.628	176	2960564	39.977	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.757	200	458437	30.993	ng/ul	0.00
73) Anthracene-d10	17.504	188	4581205	40.585	ng/ul	0.00
81) Pyrene-d10	19.739	212	4980579	41.960	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.868	264	4061399	42.063	ng/ul	-0.01
Target Compounds						
					Qvalue	
34) Caprolactam	11.798	113	23194	2.301	ng/ul	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017015.D
Acq On : 08 Sep 2023 16:47
Operator : MA/JU
Sample : 04123-17
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH9F9

Quant Time: Sep 09 00:44:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 06 01:52:05 2023
Response via : Initial Calibration

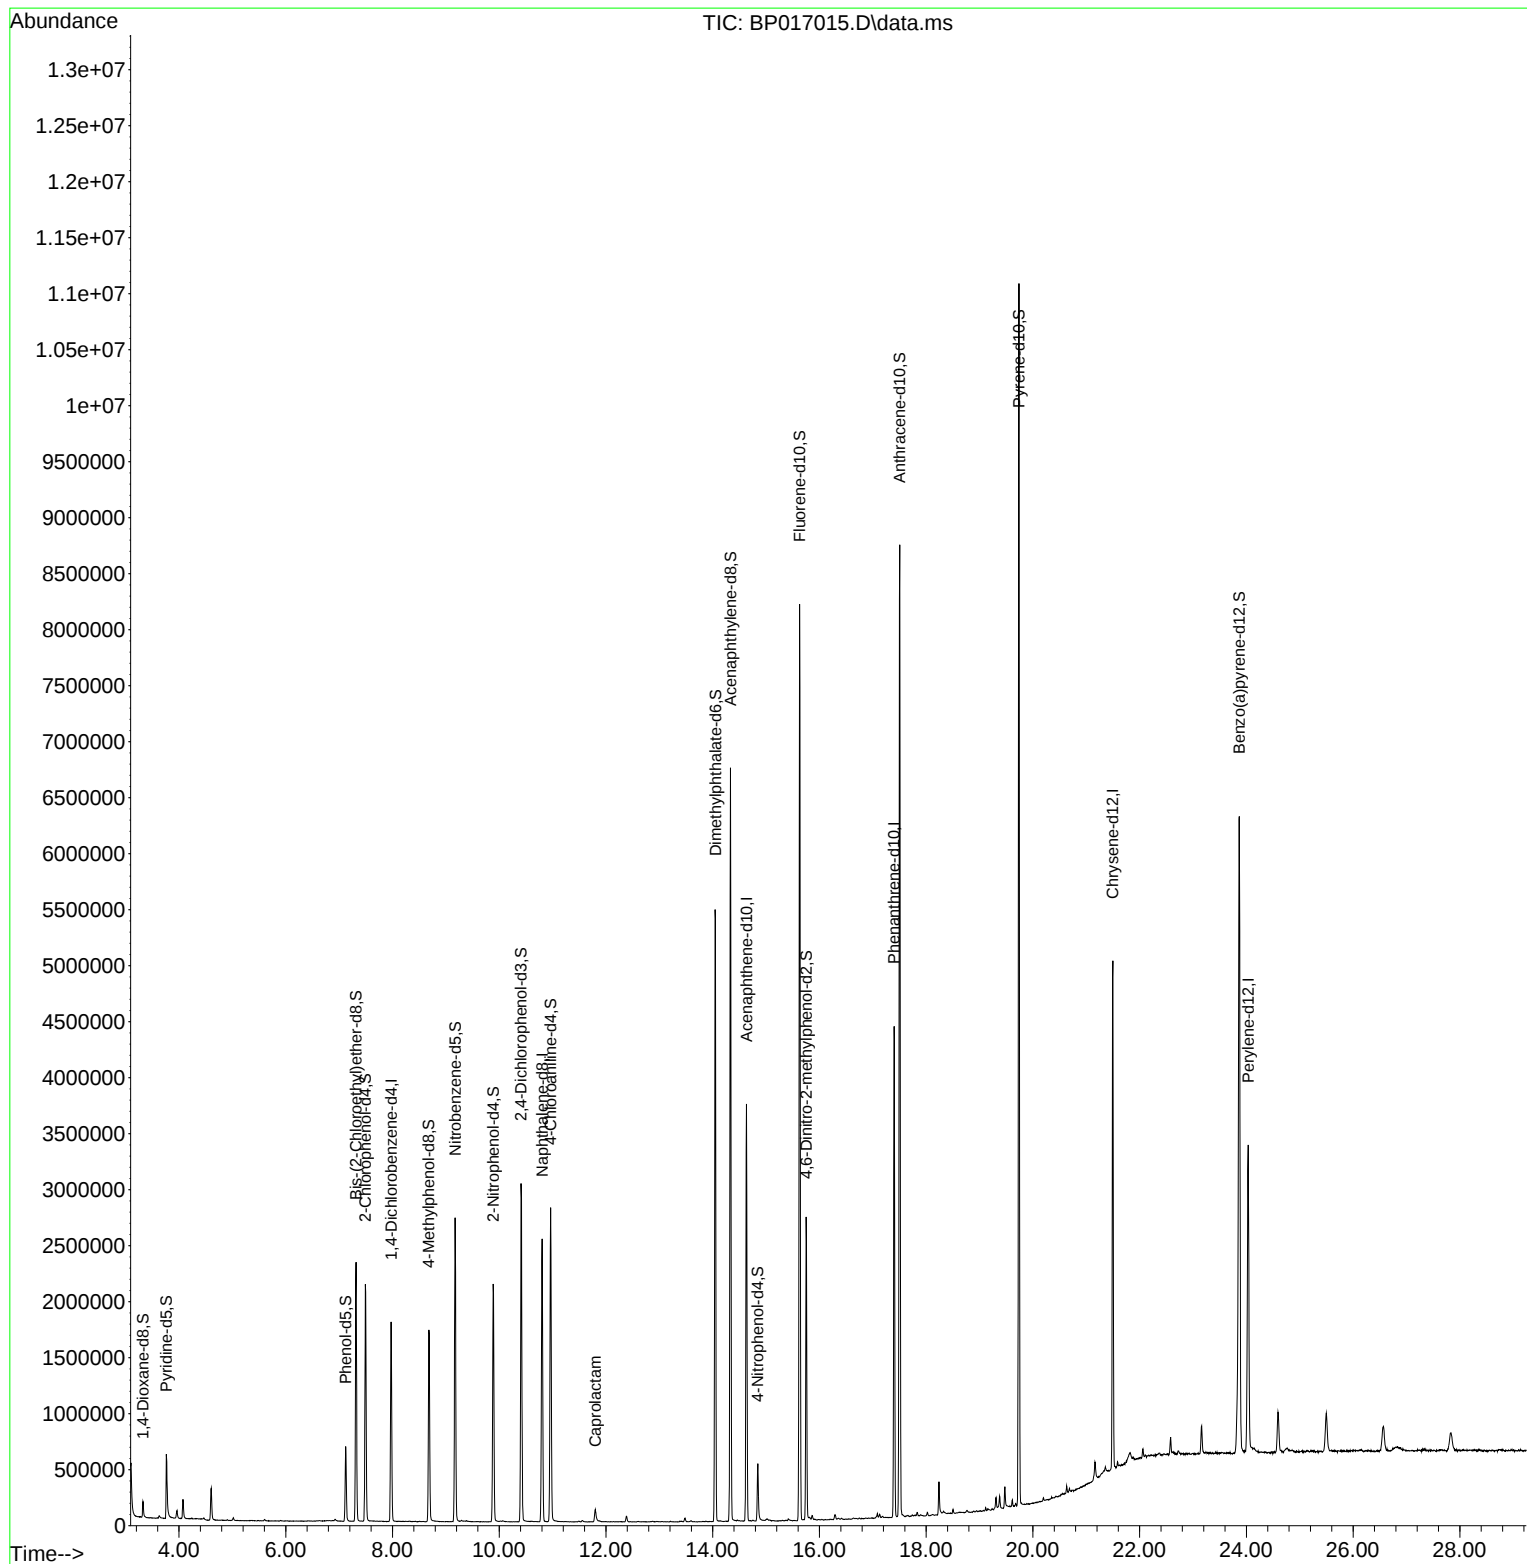

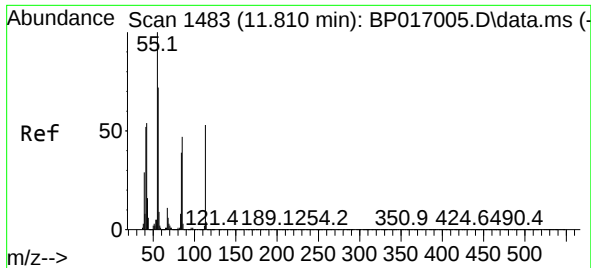

#34
 Caprolactam
 Concen: 2.301 ng/ul
 RT: 11.798 min Scan# 14
 Delta R.T. -0.012 min
 Lab File: BP017015.D
 Acq: 08 Sep 2023 16:47

Instrument :
 BNA_P
 ClientSampleId :
 BH9F9

Tgt Ion:	113	Resp:	23194
Ion	Ratio	Lower	Upper
113	100		
55	194.1	142.3	213.5
56	147.1	102.2	153.2

