

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
 Data File : BP017032.D
 Acq On : 09 Sep 2023 03:09
 Operator : MA/JU
 Sample : 04166-08
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBJP2

Quant Time: Sep 09 04:51:35 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 09 01:41:21 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.975	152	517839	20.000	ng/u1	0.00
20) Naphthalene-d8	10.798	136	2234174	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.628	164	1312992	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.398	188	2579651	20.000	ng/u1	0.00
79) Chrysene-d12	21.492	240	1691312	20.000	ng/u1	0.00
88) Perylene-d12	24.027	264	1677095	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.328	96	65485	4.783	ng/uL	0.00
4) Pyridine-d5	3.769	84	261477	6.684	ng/u1	0.01
7) Phenol-d5	7.122	99	353262	7.467	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.310	67	1006510	34.012	ng/u1	0.00
11) 2-Chlorophenol-d4	7.493	132	914278	26.702	ng/u1	0.00
15) 4-Methylphenol-d8	8.681	113	631598	17.524	ng/u1	0.00
21) Nitrobenzene-d5	9.169	128	589316	34.000	ng/u1	0.00
24) 2-Nitrophenol-d4	9.887	143	625374	33.284	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.410	165	1015610	29.278	ng/u1	0.00
31) 4-Chloroaniline-d4	10.957	131	468356	9.358	ng/u1	0.00
46) Dimethylphthalate-d6	14.045	166	3530558	36.123	ng/u1	0.00
49) Acenaphthylene-d8	14.328	160	3878865	34.389	ng/u1	0.00
54) 4-Nitrophenol-d4	14.845	143	109242	5.722	ng/u1	0.00
60) Fluorene-d10	15.628	176	2924783	34.952	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.751	200	477864	30.782	ng/u1	0.00
73) Anthracene-d10	17.498	188	4486761	37.873	ng/u1	0.00
81) Pyrene-d10	19.733	212	4454672	43.242	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.862	264	3315788	38.972	ng/u1	0.00


Target Compounds					Qvalue	
2) 1,4-Dioxane	3.364	88	57878	3.916	ng/uL	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017032.D
Acq On : 09 Sep 2023 03:09
Operator : MA/JU
Sample : 04166-08
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJP2


Quant Time: Sep 09 04:51:35 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 09 01:41:21 2023
Response via : Initial Calibration

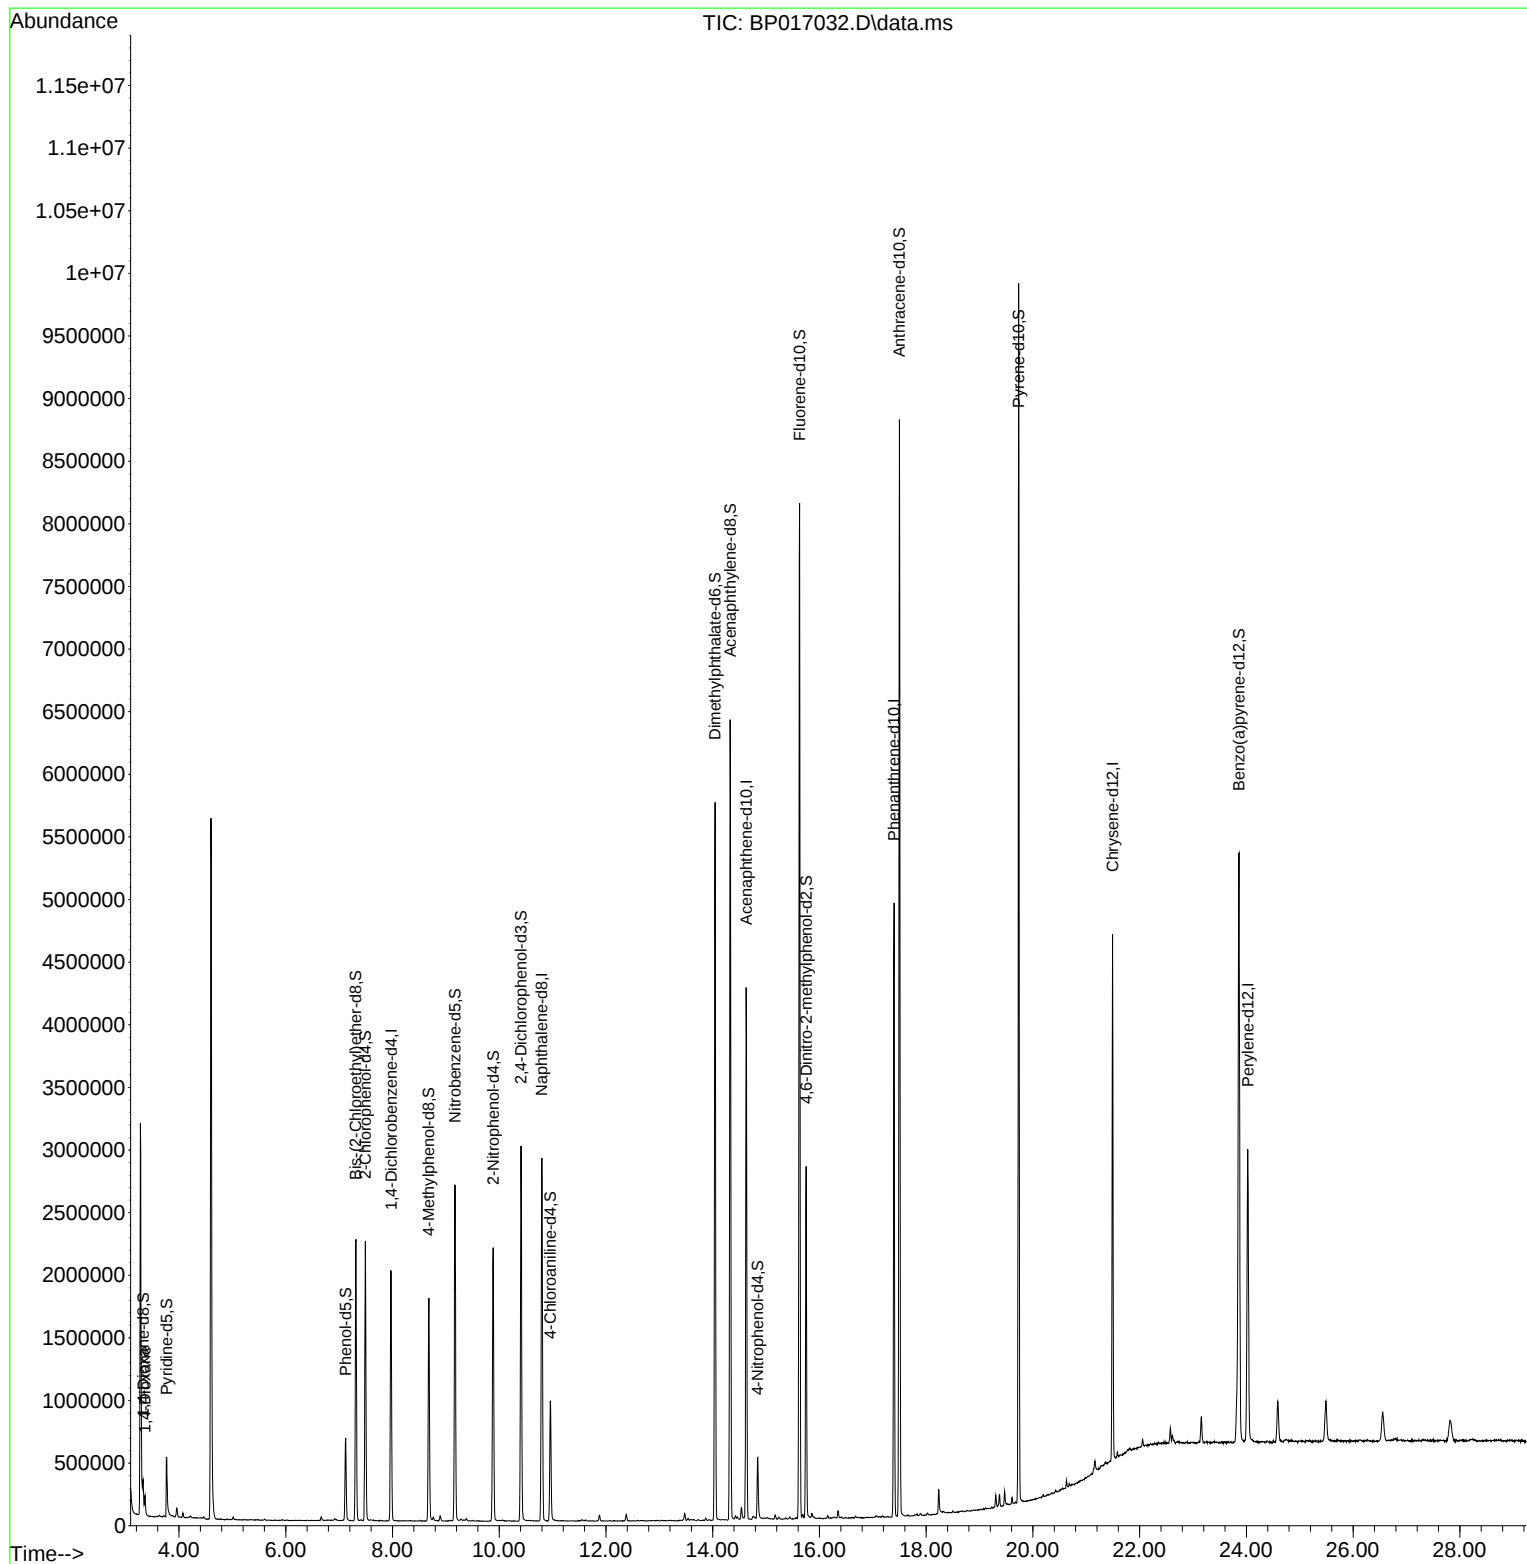

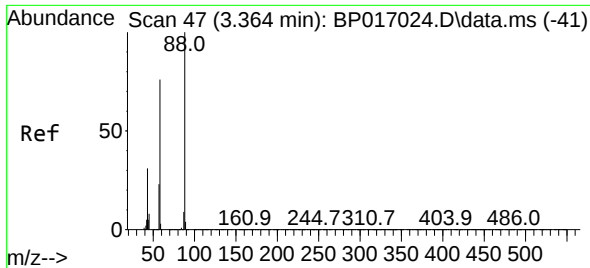

#2
 1,4-Dioxane
 Concen: 3.916 ng/uL
 RT: 3.364 min Scan# 41
 Delta R.T. -0.000 min
 Lab File: BP017032.D
 Acq: 09 Sep 2023 03:09

Instrument :
 BNA_P
 ClientSampleId :
 BBJP2

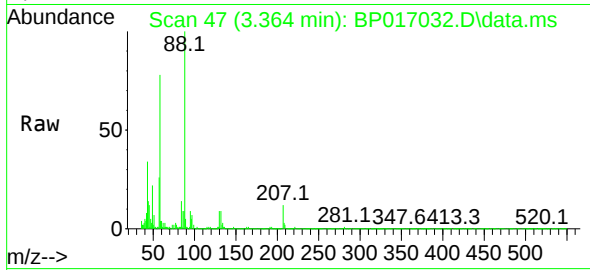

Tgt Ion:	88	Resp:	57878
Ion	Ratio	Lower	Upper
88	100		
43	33.8	25.0	37.6
58	77.8	60.6	90.8

