

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
 Data File : BP017033.D
 Acq On : 09 Sep 2023 03:43
 Operator : MA/JU
 Sample : 04166-09
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBKJ9

Quant Time: Sep 09 04:55:55 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 09 01:41:21 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.975	152	587414	20.000	ng/u1	0.00
20) Naphthalene-d8	10.799	136	2598001	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.628	164	1554905	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.398	188	3191315	20.000	ng/u1	0.00
79) Chrysene-d12	21.492	240	2200836	20.000	ng/u1	0.00
88) Perylene-d12	24.027	264	1970562	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.323	96	73532	4.735	ng/uL	0.00
4) Pyridine-d5	3.764	84	456640	10.291	ng/u1	0.00
7) Phenol-d5	7.122	99	448010	8.348	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.311	67	1358350	40.465	ng/u1	0.00
11) 2-Chlorophenol-d4	7.493	132	1210008	31.153	ng/u1	0.00
15) 4-Methylphenol-d8	8.681	113	842804	20.614	ng/u1	0.00
21) Nitrobenzene-d5	9.175	128	793015	39.345	ng/u1	0.00
24) 2-Nitrophenol-d4	9.887	143	832598	38.107	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.410	165	1399707	34.700	ng/u1	0.00
31) 4-Chloroaniline-d4	10.957	131	1347536	23.155	ng/u1	0.00
46) Dimethylphthalate-d6	14.046	166	4835055	41.774	ng/u1	0.00
49) Acenaphthylene-d8	14.328	160	5391194	40.361	ng/u1	0.00
54) 4-Nitrophenol-d4	14.845	143	156845	6.937	ng/u1	0.00
60) Fluorene-d10	15.628	176	3997803	40.342	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.751	200	688511	35.850	ng/u1	0.00
73) Anthracene-d10	17.498	188	6116740	41.736	ng/u1	0.00
81) Pyrene-d10	19.733	212	6307104	47.049	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.863	264	4356646	43.579	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.364	88	30492	1.819	ng/uL	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017033.D
Acq On : 09 Sep 2023 03:43
Operator : MA/JU
Sample : 04166-09
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBKJ9


Quant Time: Sep 09 04:55:55 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 09 01:41:21 2023
Response via : Initial Calibration

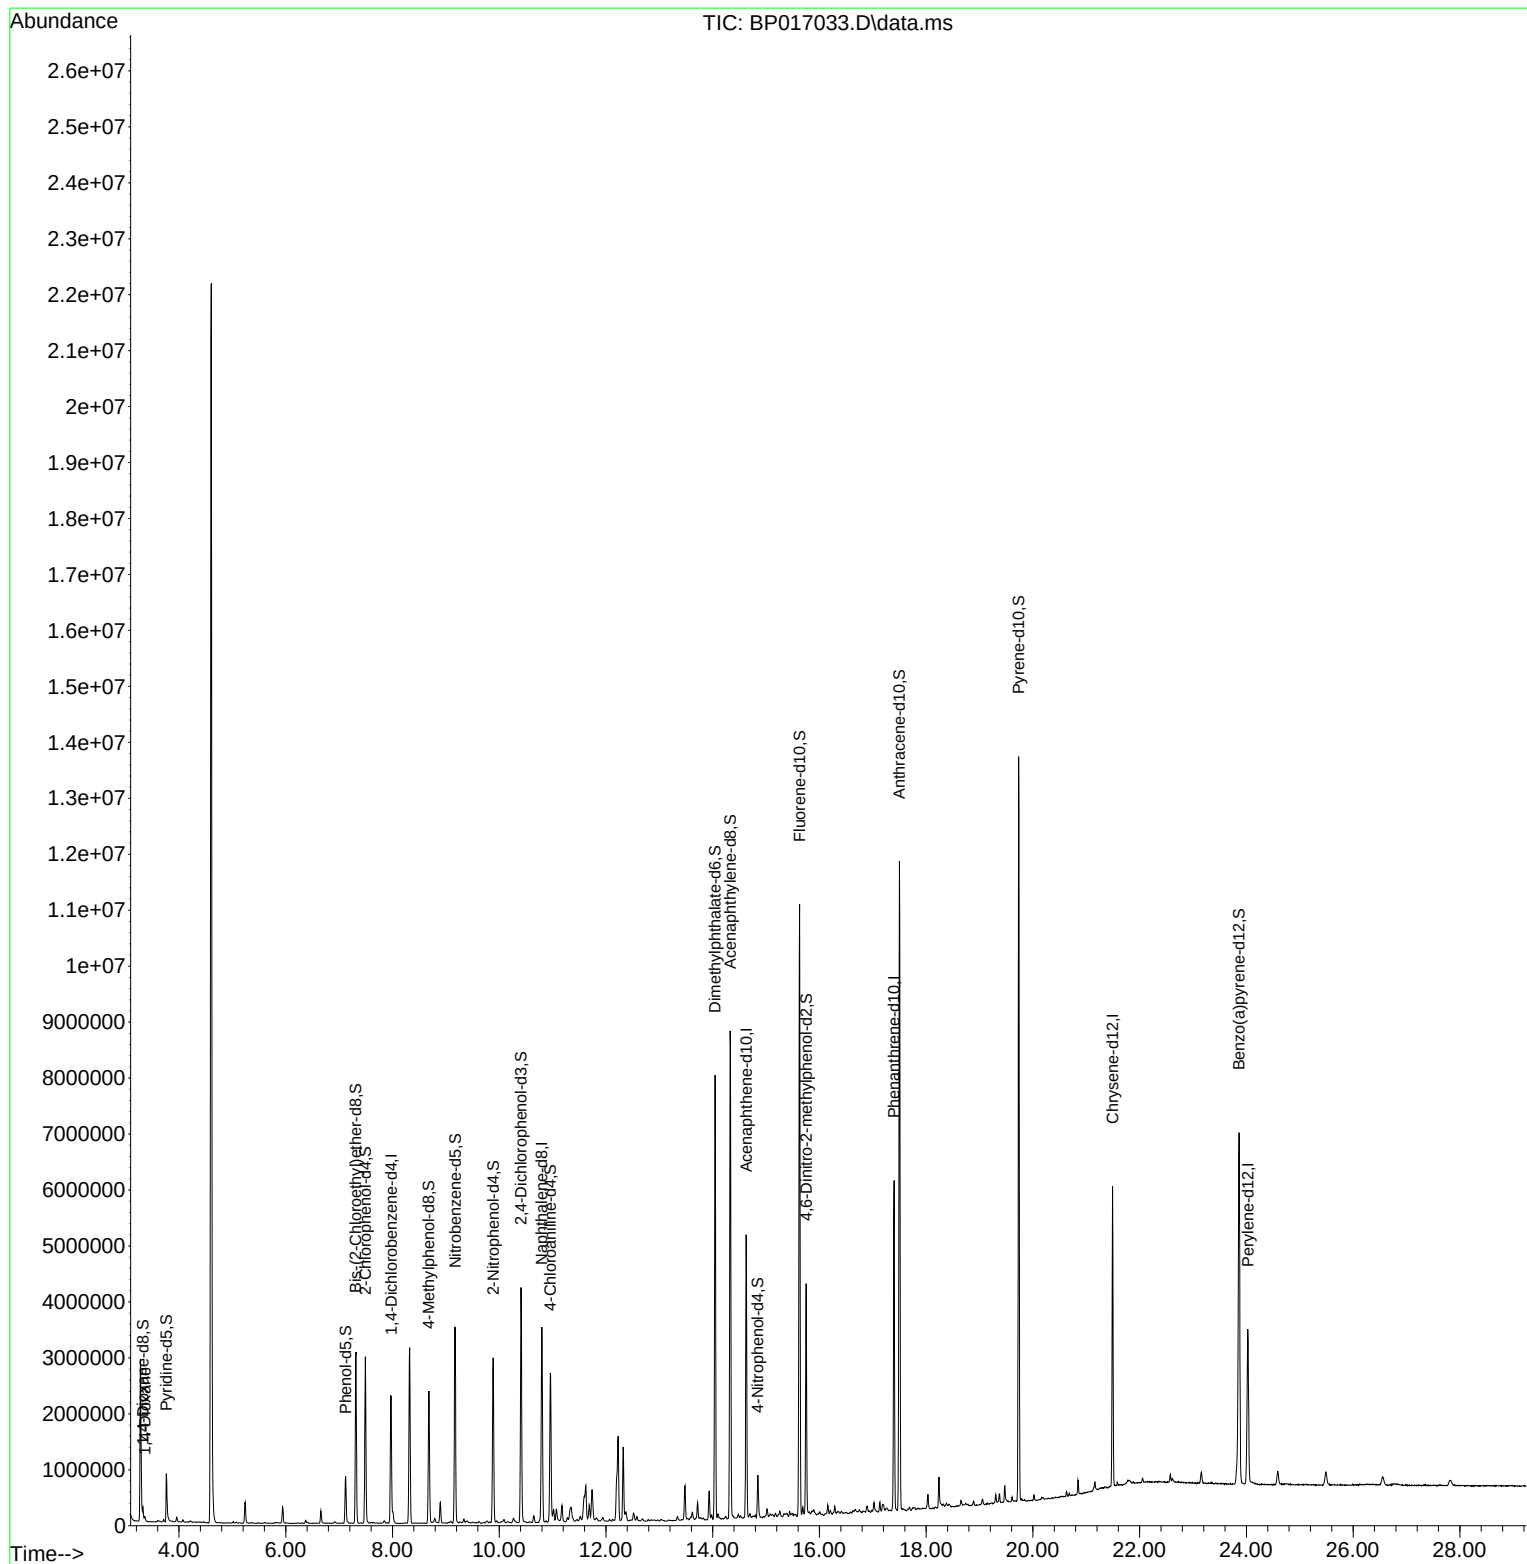

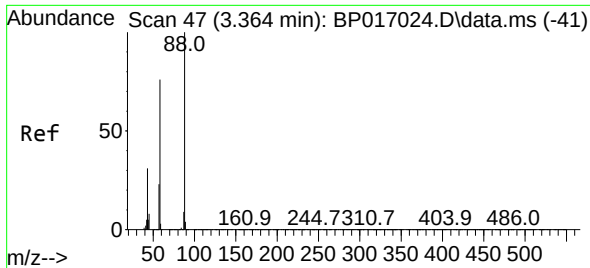

#2
 1,4-Dioxane
 Concen: 1.819 ng/uL
 RT: 3.364 min Scan# 41
 Delta R.T. -0.000 min
 Lab File: BP017033.D
 Acq: 09 Sep 2023 03:43

Instrument :
 BNA_P
 ClientSampleId :
 BBKJ9

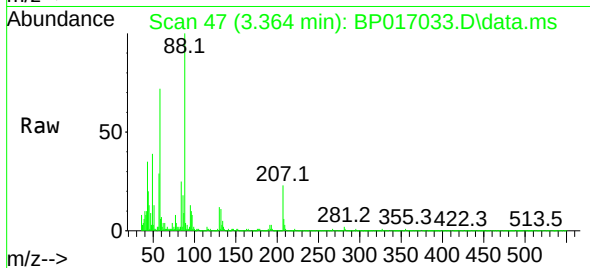

Tgt Ion:	88	Resp:	30492
Ion	Ratio	Lower	Upper
88	100		
43	35.0	25.0	37.6
58	72.1	60.6	90.8

