

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
 Data File : BP017034.D
 Acq On : 09 Sep 2023 04:18
 Operator : MA/JU
 Sample : 04166-10
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBKJ5

Quant Time: Sep 09 04:57:50 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 09 01:41:21 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.975	152	415863	20.000	ng/u1	0.00
20) Naphthalene-d8	10.798	136	1714581	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.627	164	941351	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.398	188	1725313	20.000	ng/u1	0.00
79) Chrysene-d12	21.492	240	1080919	20.000	ng/u1	0.00
88) Perylene-d12	24.027	264	1163313	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.328	96	63970	5.819	ng/uL	0.00
4) Pyridine-d5	3.763	84	489995	15.598	ng/u1	0.00
7) Phenol-d5	7.122	99	431826	11.366	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.316	67	1050129	44.188	ng/u1	0.00
11) 2-Chlorophenol-d4	7.493	132	1020536	37.114	ng/u1	0.00
15) 4-Methylphenol-d8	8.681	113	717097	24.775	ng/u1	0.00
21) Nitrobenzene-d5	9.175	128	605102	45.490	ng/u1	0.00
24) 2-Nitrophenol-d4	9.887	143	630043	43.694	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.410	165	1041208	39.112	ng/u1	0.00
31) 4-Chloroaniline-d4	10.957	131	923132	24.035	ng/u1	0.00
46) Dimethylphthalate-d6	14.045	166	3138593	44.791	ng/u1	0.00
49) Acenaphthylene-d8	14.328	160	3586234	44.347	ng/u1	0.00
54) 4-Nitrophenol-d4	14.845	143	104357	7.624	ng/u1	0.00
60) Fluorene-d10	15.627	176	2577512	42.962	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.751	200	340764	32.820	ng/u1	0.00
73) Anthracene-d10	17.498	188	3663594	46.238	ng/u1	0.00
81) Pyrene-d10	19.733	212	3510140	53.314	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.856	264	2779260	47.092	ng/u1	0.00
Target Compounds						
					Qvalue	
30) Naphthalene	10.851	128	98983	1.058	ng/u1	97
37) 1-Methylnaphthalene	12.675	142	207761	3.338	ng/u1	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017034.D
Acq On : 09 Sep 2023 04:18
Operator : MA/JU
Sample : 04166-10
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBKJ5

Quant Time: Sep 09 04:57:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 09 01:41:21 2023
Response via : Initial Calibration




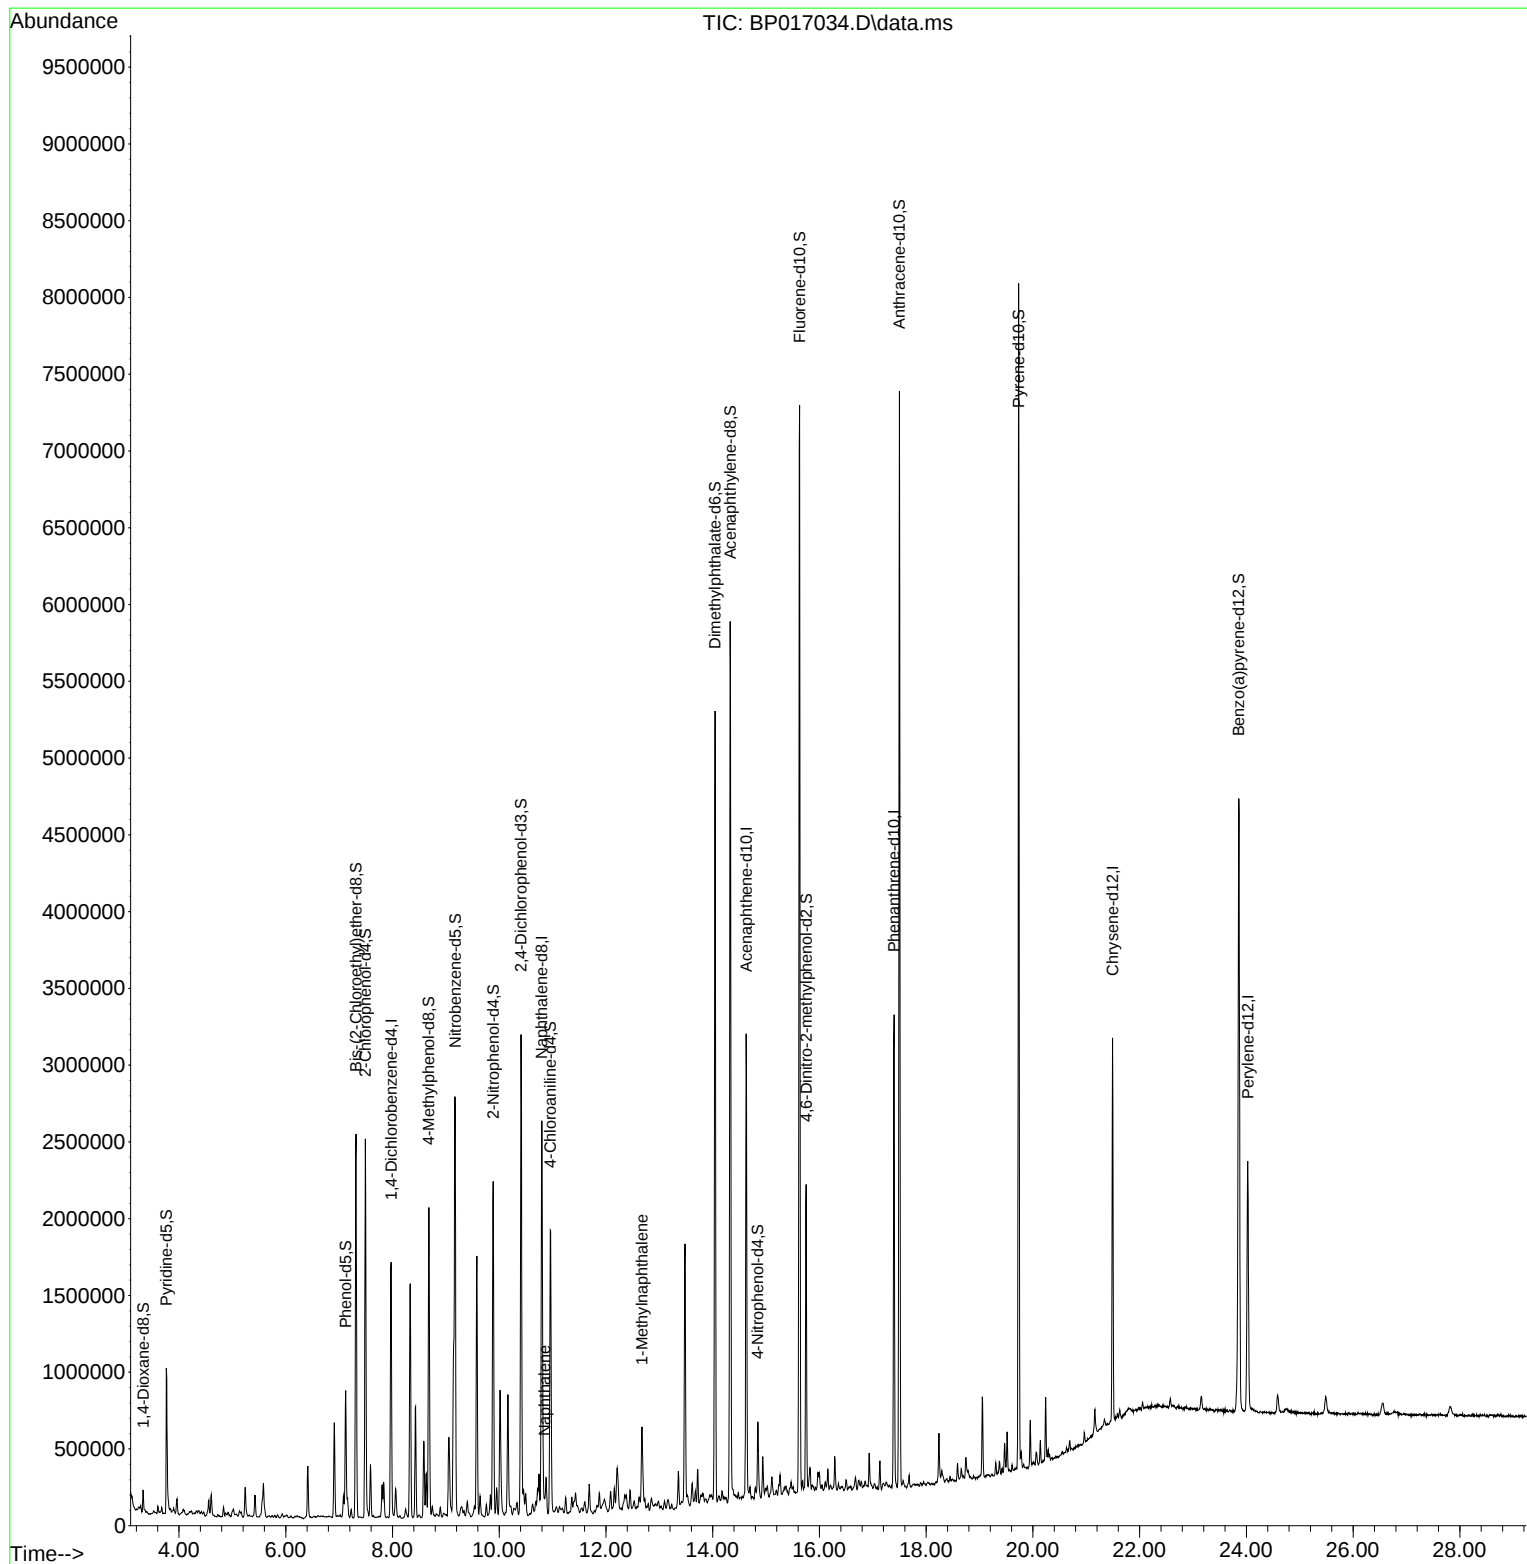


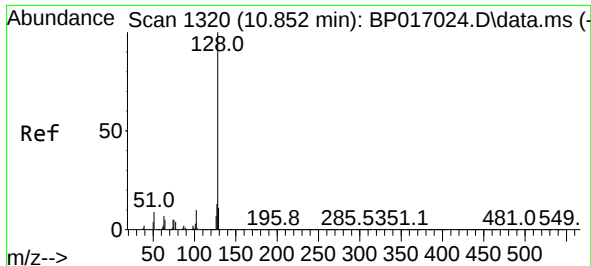

#30
Naphthalene
Concen: 1.058 ng/ul
RT: 10.851 min Scan# 11
Delta R.T. -0.000 min
Lab File: BP017034.D
Acq: 09 Sep 2023 04:18

Instrument :
BNA_P
ClientSampleId :
BBKJ5

Tgt Ion:128 Resp: 98983
Ion Ratio Lower Upper
128 100
129 11.9 8.8 13.2
127 14.3 10.3 15.5

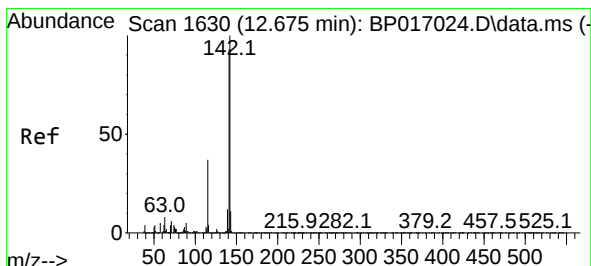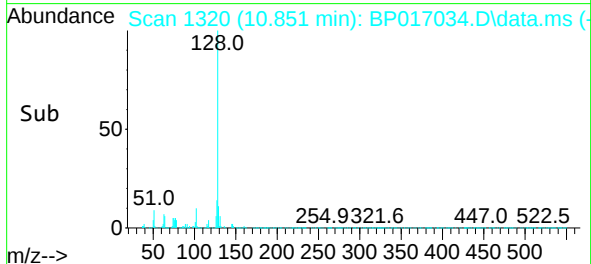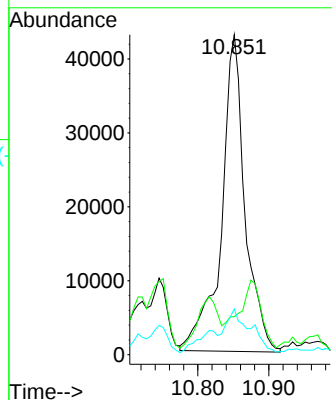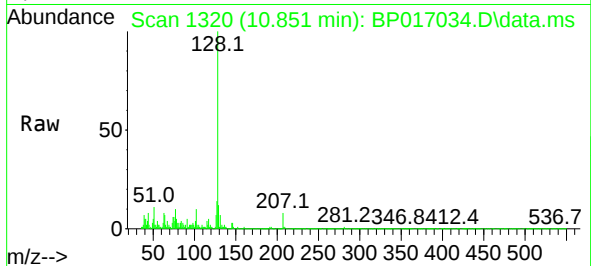

#37
1-Methylnaphthalene
Concen: 3.338 ng/ul
RT: 12.675 min Scan# 1630
Delta R.T. -0.000 min
Lab File: BP017034.D
Acq: 09 Sep 2023 04:18

Tgt Ion:142 Resp: 207761
Ion Ratio Lower Upper
142 100
141 93.4 74.5 111.7
116 4.3 3.1 4.7

