

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
 Data File : BP017052.D
 Acq On : 09 Sep 2023 15:09
 Operator : MA/JU
 Sample : 04227-16
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBKJ7

Quant Time: Sep 10 00:21:12 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 09 01:41:21 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.969	152	363073	20.000	ng/u1	0.00
20) Naphthalene-d8	10.799	136	1574260	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.628	164	915015	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.392	188	1909344	20.000	ng/u1	0.00
79) Chrysene-d12	21.492	240	1427294	20.000	ng/u1	0.00
88) Perylene-d12	24.021	264	1350384	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.322	96	48049	5.006	ng/uL	0.00
4) Pyridine-d5	3.764	84	444192	16.196	ng/u1	0.00
7) Phenol-d5	7.122	99	283439	8.545	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.310	67	949588	45.767	ng/u1	0.00
11) 2-Chlorophenol-d4	7.493	132	828345	34.505	ng/u1	0.00
15) 4-Methylphenol-d8	8.681	113	551165	21.811	ng/u1	0.00
21) Nitrobenzene-d5	9.169	128	538996	44.132	ng/u1	0.00
24) 2-Nitrophenol-d4	9.881	143	558210	42.163	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.410	165	953113	38.994	ng/u1	0.00
31) 4-Chloroaniline-d4	10.957	131	967704	27.442	ng/u1	0.00
46) Dimethylphthalate-d6	14.045	166	3278837	48.139	ng/u1	0.00
49) Acenaphthylene-d8	14.328	160	3742686	47.614	ng/u1	0.00
54) 4-Nitrophenol-d4	14.851	143	91589	6.884	ng/u1	0.00
60) Fluorene-d10	15.622	176	2797359	47.969	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.751	200	447985	38.988	ng/u1	0.00
73) Anthracene-d10	17.498	188	4332623	49.411	ng/u1	0.00
81) Pyrene-d10	19.733	212	4667456	53.688	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.857	264	3462325	50.539	ng/u1	0.00


Target Compounds					Qvalue
2) 1,4-Dioxane	3.358	88	37417	3.610 ng/uL#	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017052.D
Acq On : 09 Sep 2023 15:09
Operator : MA/JU
Sample : 04227-16
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBKJ7


Quant Time: Sep 10 00:21:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 09 01:41:21 2023
Response via : Initial Calibration

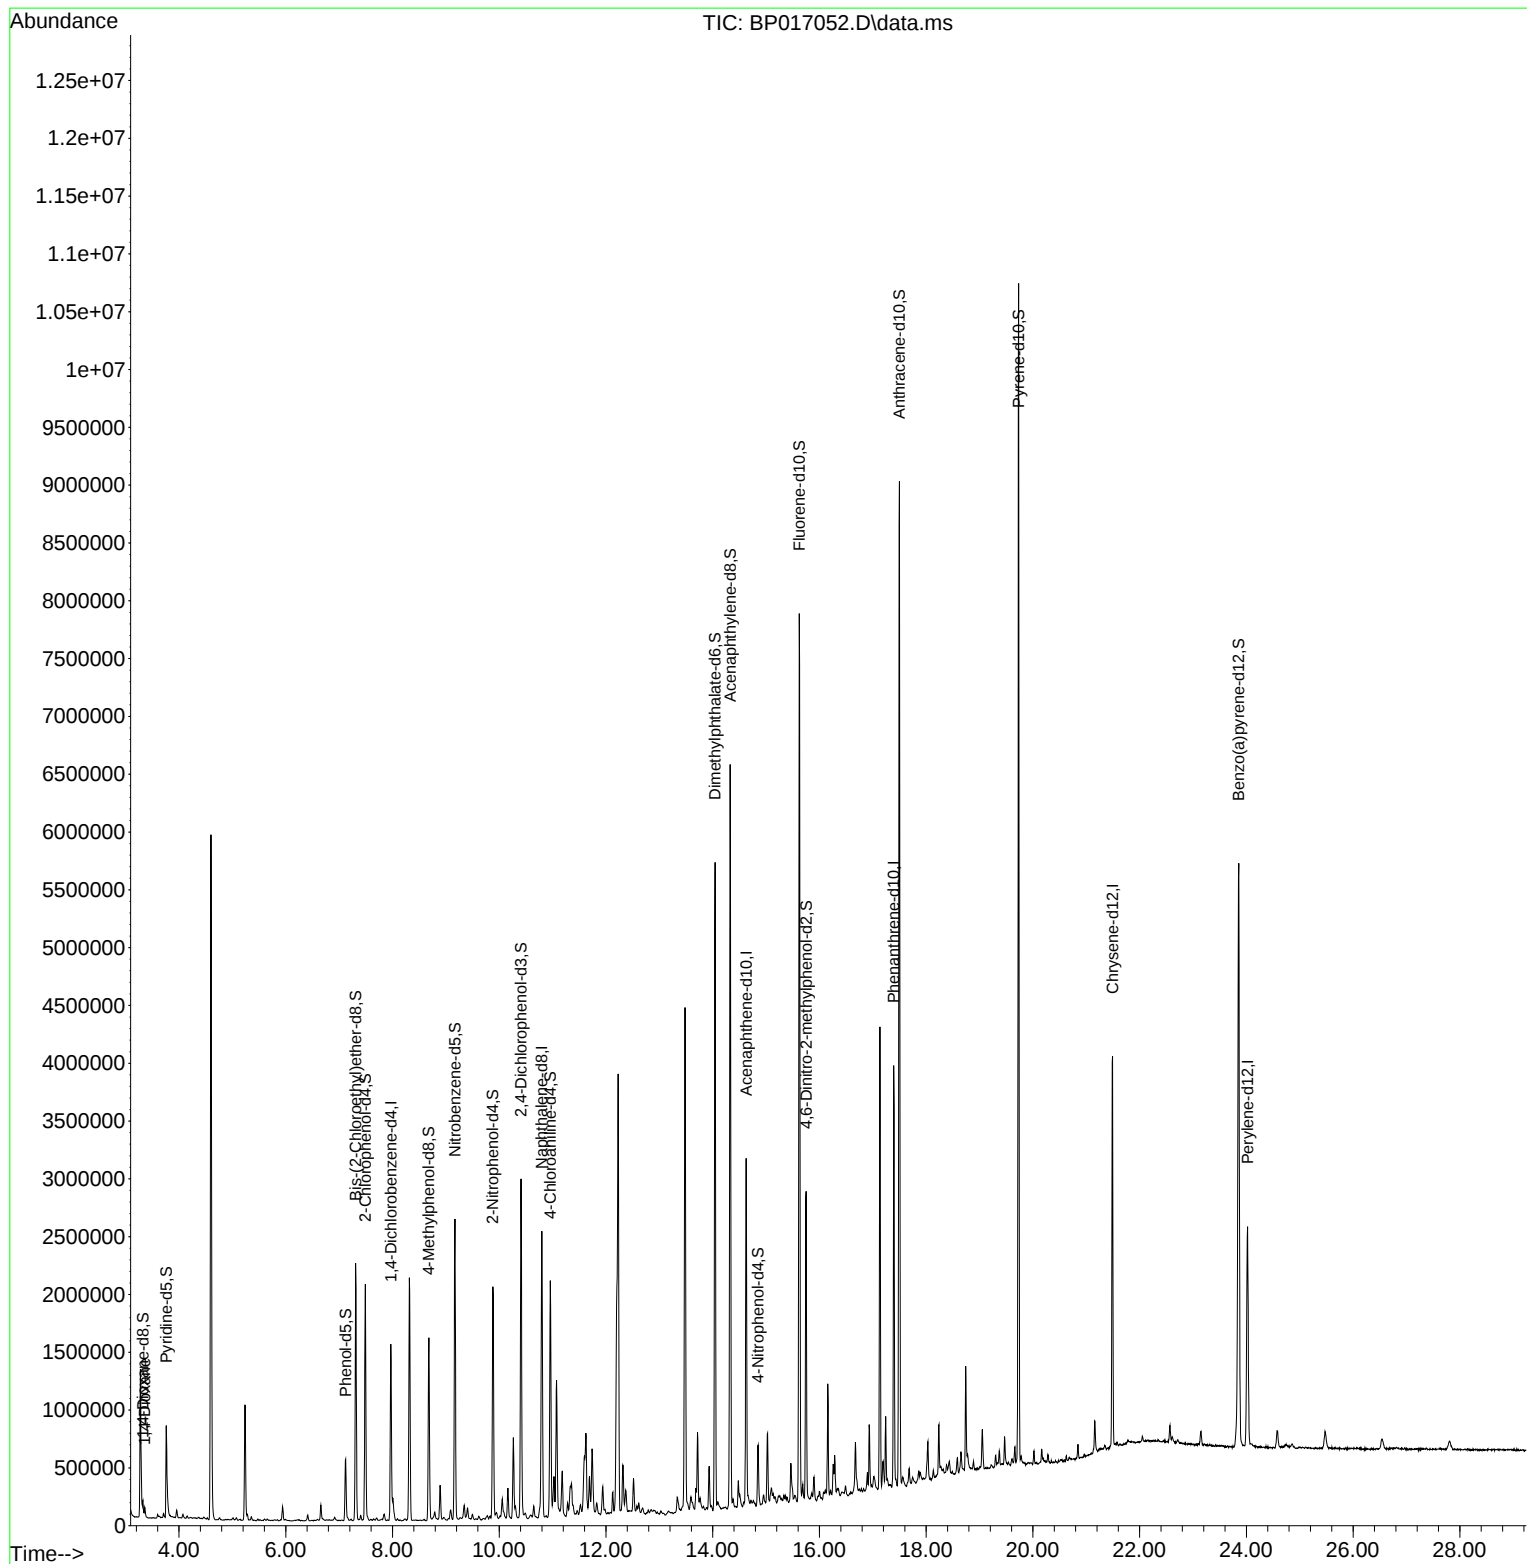

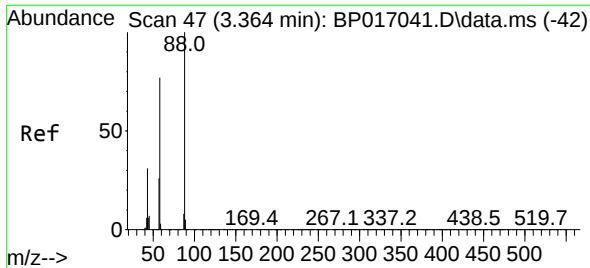

#2
 1,4-Dioxane
 Concen: 3.610 ng/uL
 RT: 3.358 min Scan# 41
 Delta R.T. -0.006 min
 Lab File: BP017052.D
 Acq: 09 Sep 2023 15:09

Instrument :
 BNA_P
 ClientSampleId :
 BBKJ7

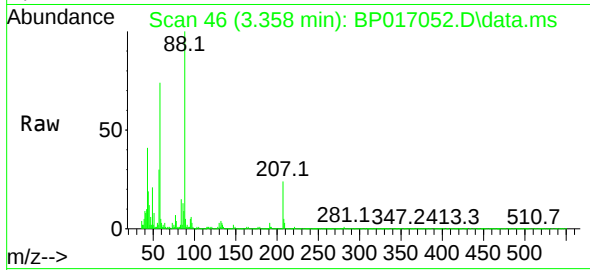

Tgt Ion: 88 Resp: 37417
 Ion Ratio Lower Upper
 88 100
 43 41.0 25.0 37.6#
 58 74.2 60.6 90.8

