

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
 Data File : BP017067.D
 Acq On : 10 Sep 2023 00:23
 Operator : MA/JU
 Sample : 04227-01
 Misc :
 ALS Vial : 79 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBKE3

Quant Time: Sep 10 01:19:18 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 09 01:41:21 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.969	152	456302	20.000	ng/u1	0.00
20) Naphthalene-d8	10.793	136	2040280	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.628	164	1230461	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.392	188	2633774	20.000	ng/u1	0.00
79) Chrysene-d12	21.486	240	2112065	20.000	ng/u1	0.00
88) Perylene-d12	24.021	264	2073039	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.323	96	70745	5.864	ng/uL	0.00
4) Pyridine-d5	3.764	84	430276	12.483	ng/u1	0.00
7) Phenol-d5	7.116	99	284576	6.826	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.311	67	1094466	41.973	ng/u1	0.00
11) 2-Chlorophenol-d4	7.487	132	888282	29.441	ng/u1	0.00
15) 4-Methylphenol-d8	8.675	113	572982	18.042	ng/u1	-0.01
21) Nitrobenzene-d5	9.169	128	625136	39.494	ng/u1	0.00
24) 2-Nitrophenol-d4	9.881	143	610679	35.590	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.410	165	1091066	34.443	ng/u1	0.00
31) 4-Chloroaniline-d4	10.957	131	1403797	30.716	ng/u1	0.00
46) Dimethylphthalate-d6	14.045	166	4189109	45.736	ng/u1	0.00
49) Acenaphthylene-d8	14.328	160	4599791	43.516	ng/u1	0.00
54) 4-Nitrophenol-d4	14.845	143	96712	5.406	ng/u1	0.00
60) Fluorene-d10	15.622	176	3558756	45.381	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.751	200	548220	34.588	ng/u1	0.00
73) Anthracene-d10	17.498	188	5701376	47.137	ng/u1	0.00
81) Pyrene-d10	19.733	212	6378194	49.580	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.857	264	5044245	47.963	ng/u1	0.00
Target Compounds						
					Qvalue	
30) Naphthalene	10.846	128	314407	2.824	ng/u1	99
37) 1-Methylnaphthalene	12.669	142	152068	2.053	ng/u1	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017067.D
Acq On : 10 Sep 2023 00:23
Operator : MA/JU
Sample : 04227-01
Misc :
ALS Vial : 79 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBKE3

Quant Time: Sep 10 01:19:18 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 09 01:41:21 2023
Response via : Initial Calibration




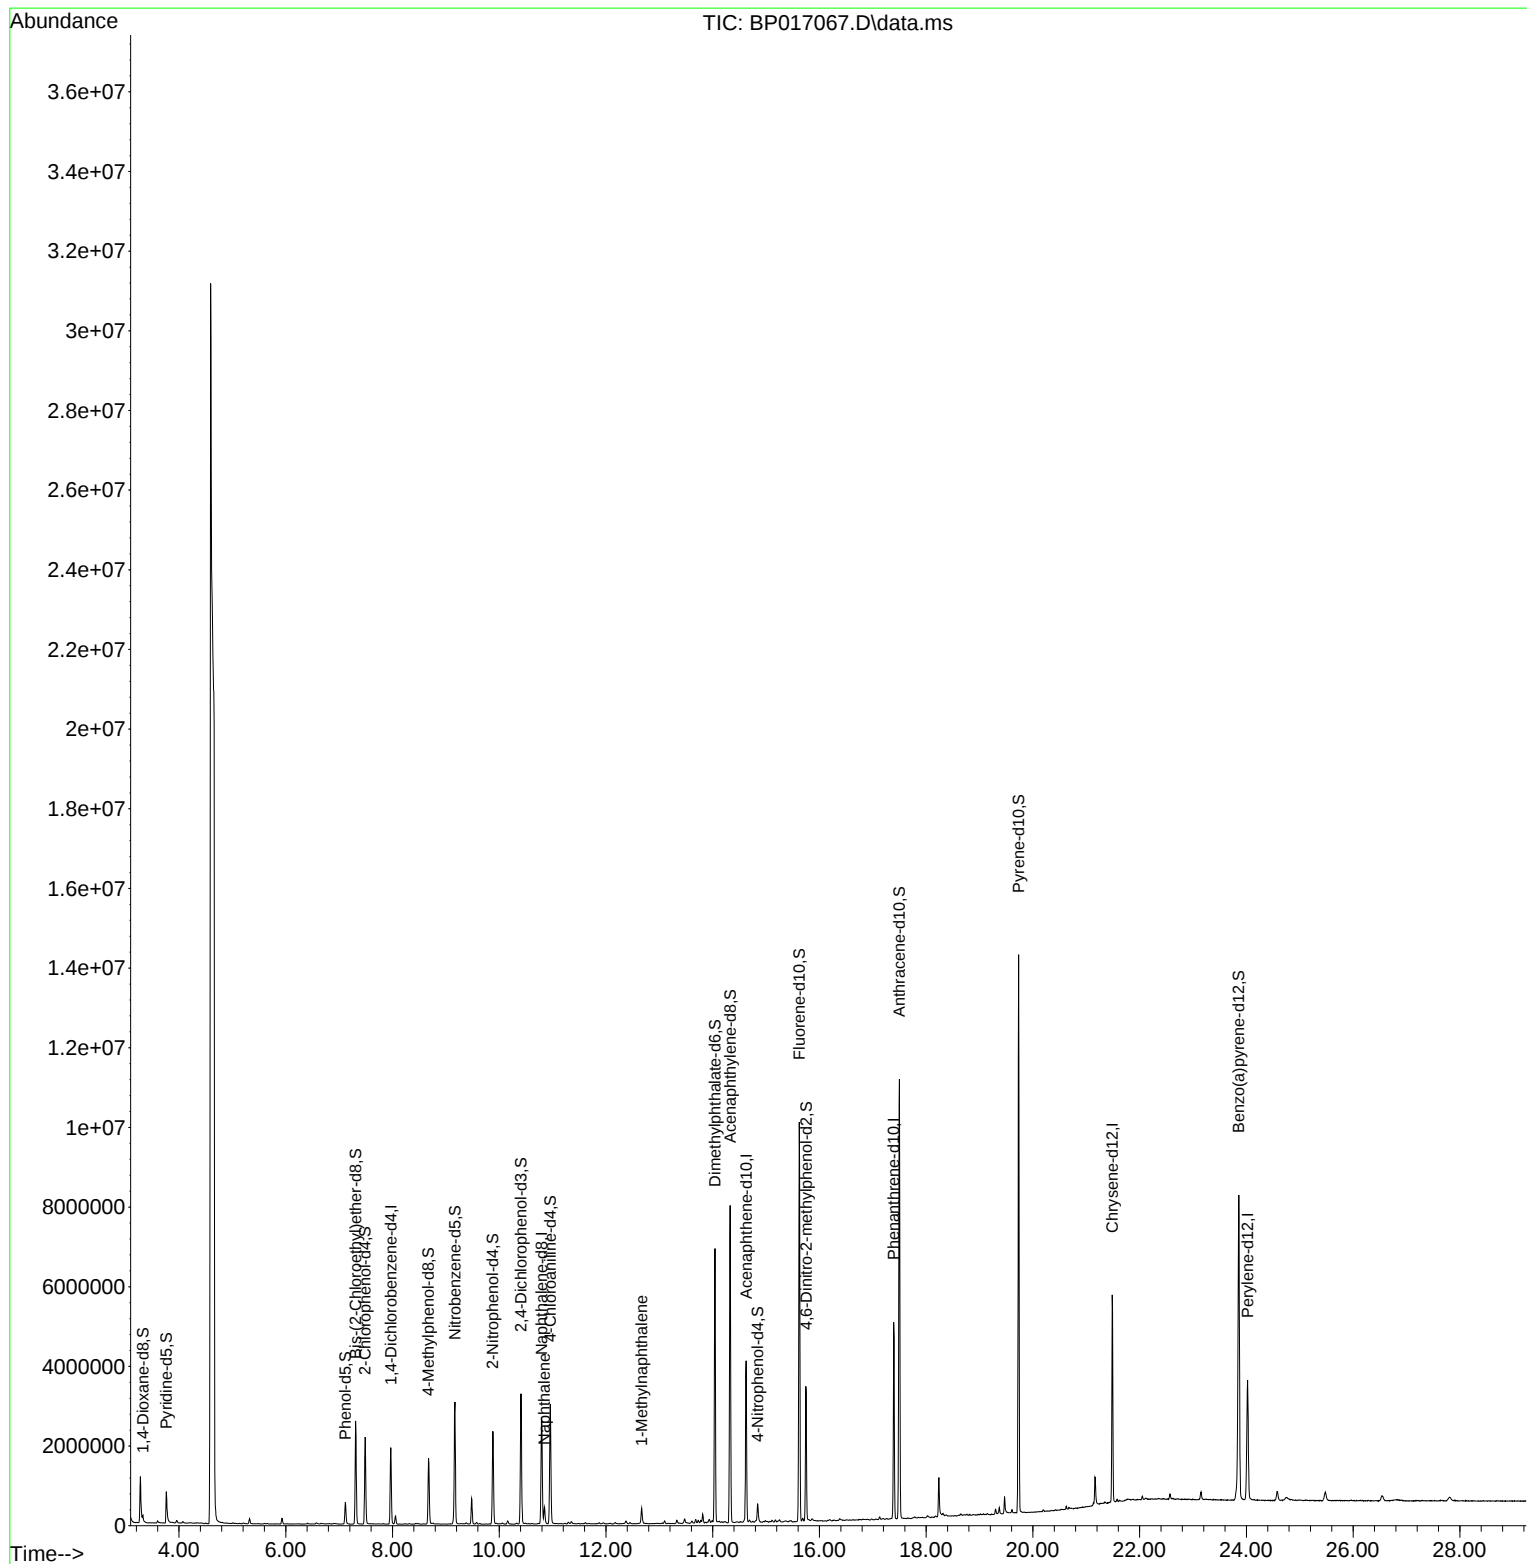


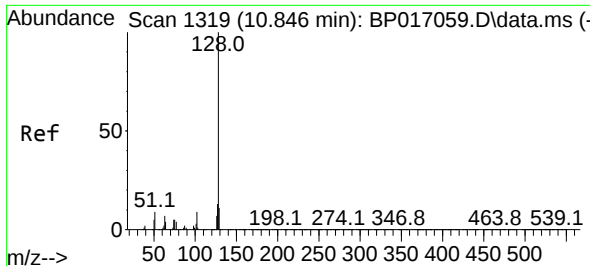

#30
Naphthalene
Concen: 2.824 ng/ul
RT: 10.846 min Scan# 1319
Delta R.T. -0.006 min
Lab File: BP017067.D
Acq: 10 Sep 2023 00:23

Instrument :
BNA_P
ClientSampleId :
BBKE3

Tgt Ion:128 Resp: 314407
Ion Ratio Lower Upper
128 100
129 11.4 8.8 13.2
127 13.2 10.3 15.5

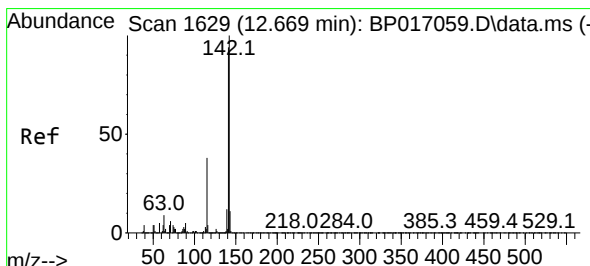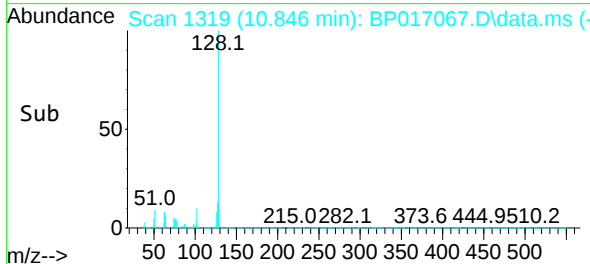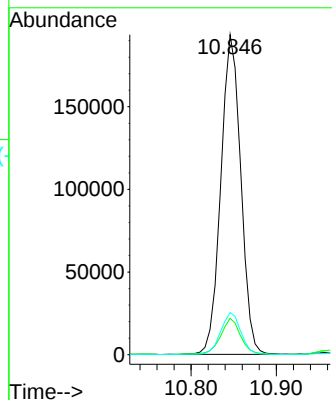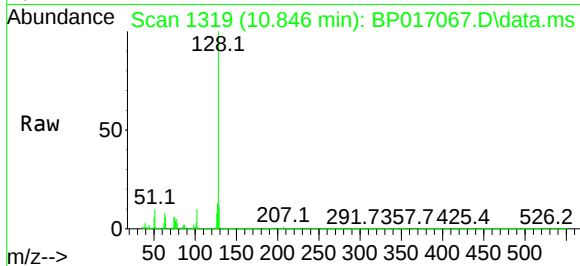

#37
1-Methylnaphthalene
Concen: 2.053 ng/ul
RT: 12.669 min Scan# 1629
Delta R.T. -0.006 min
Lab File: BP017067.D
Acq: 10 Sep 2023 00:23

Tgt Ion:142 Resp: 152068
Ion Ratio Lower Upper
142 100
141 93.6 74.5 111.7
116 4.3 3.1 4.7

