

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
 Data File : BP017068.D
 Acq On : 10 Sep 2023 00:58
 Operator : MA/JU
 Sample : 04227-02
 Misc :
 ALS Vial : 80 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBKE2

Quant Time: Sep 10 01:34:17 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 09 01:41:21 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.969	152	458300	20.000	ng/u1	0.00
20) Naphthalene-d8	10.793	136	1976383	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.628	164	1162976	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.392	188	2353642	20.000	ng/u1	0.00
79) Chrysene-d12	21.486	240	1655465	20.000	ng/u1	0.00
88) Perylene-d12	24.015	264	1500759	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.322	96	68630	5.664	ng/uL	0.00
4) Pyridine-d5	3.758	84	583009	16.840	ng/u1	0.00
7) Phenol-d5	7.116	99	409535	9.781	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.310	67	1081554	41.297	ng/u1	0.00
11) 2-Chlorophenol-d4	7.487	132	986481	32.554	ng/u1	0.00
15) 4-Methylphenol-d8	8.675	113	701461	21.991	ng/u1	-0.01
21) Nitrobenzene-d5	9.169	128	605965	39.520	ng/u1	0.00
24) 2-Nitrophenol-d4	9.881	143	619428	37.267	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.404	165	1046261	34.096	ng/u1	0.00
31) 4-Chloroaniline-d4	10.957	131	1307579	29.535	ng/u1	0.00
46) Dimethylphthalate-d6	14.039	166	3660620	42.286	ng/u1	0.00
49) Acenaphthylene-d8	14.328	160	4059188	40.630	ng/u1	0.00
54) 4-Nitrophenol-d4	14.839	143	126107	7.457	ng/u1	0.00
60) Fluorene-d10	15.622	176	3070476	41.426	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.745	200	456289	32.214	ng/u1	-0.01
73) Anthracene-d10	17.492	188	4660353	43.116	ng/u1	0.00
81) Pyrene-d10	19.733	212	4923037	48.823	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.851	264	3372586	44.297	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.358	88	125545	9.597	ng/uL	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017068.D
Acq On : 10 Sep 2023 00:58
Operator : MA/JU
Sample : 04227-02
Misc :
ALS Vial : 80 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBKE2


Quant Time: Sep 10 01:34:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 09 01:41:21 2023
Response via : Initial Calibration

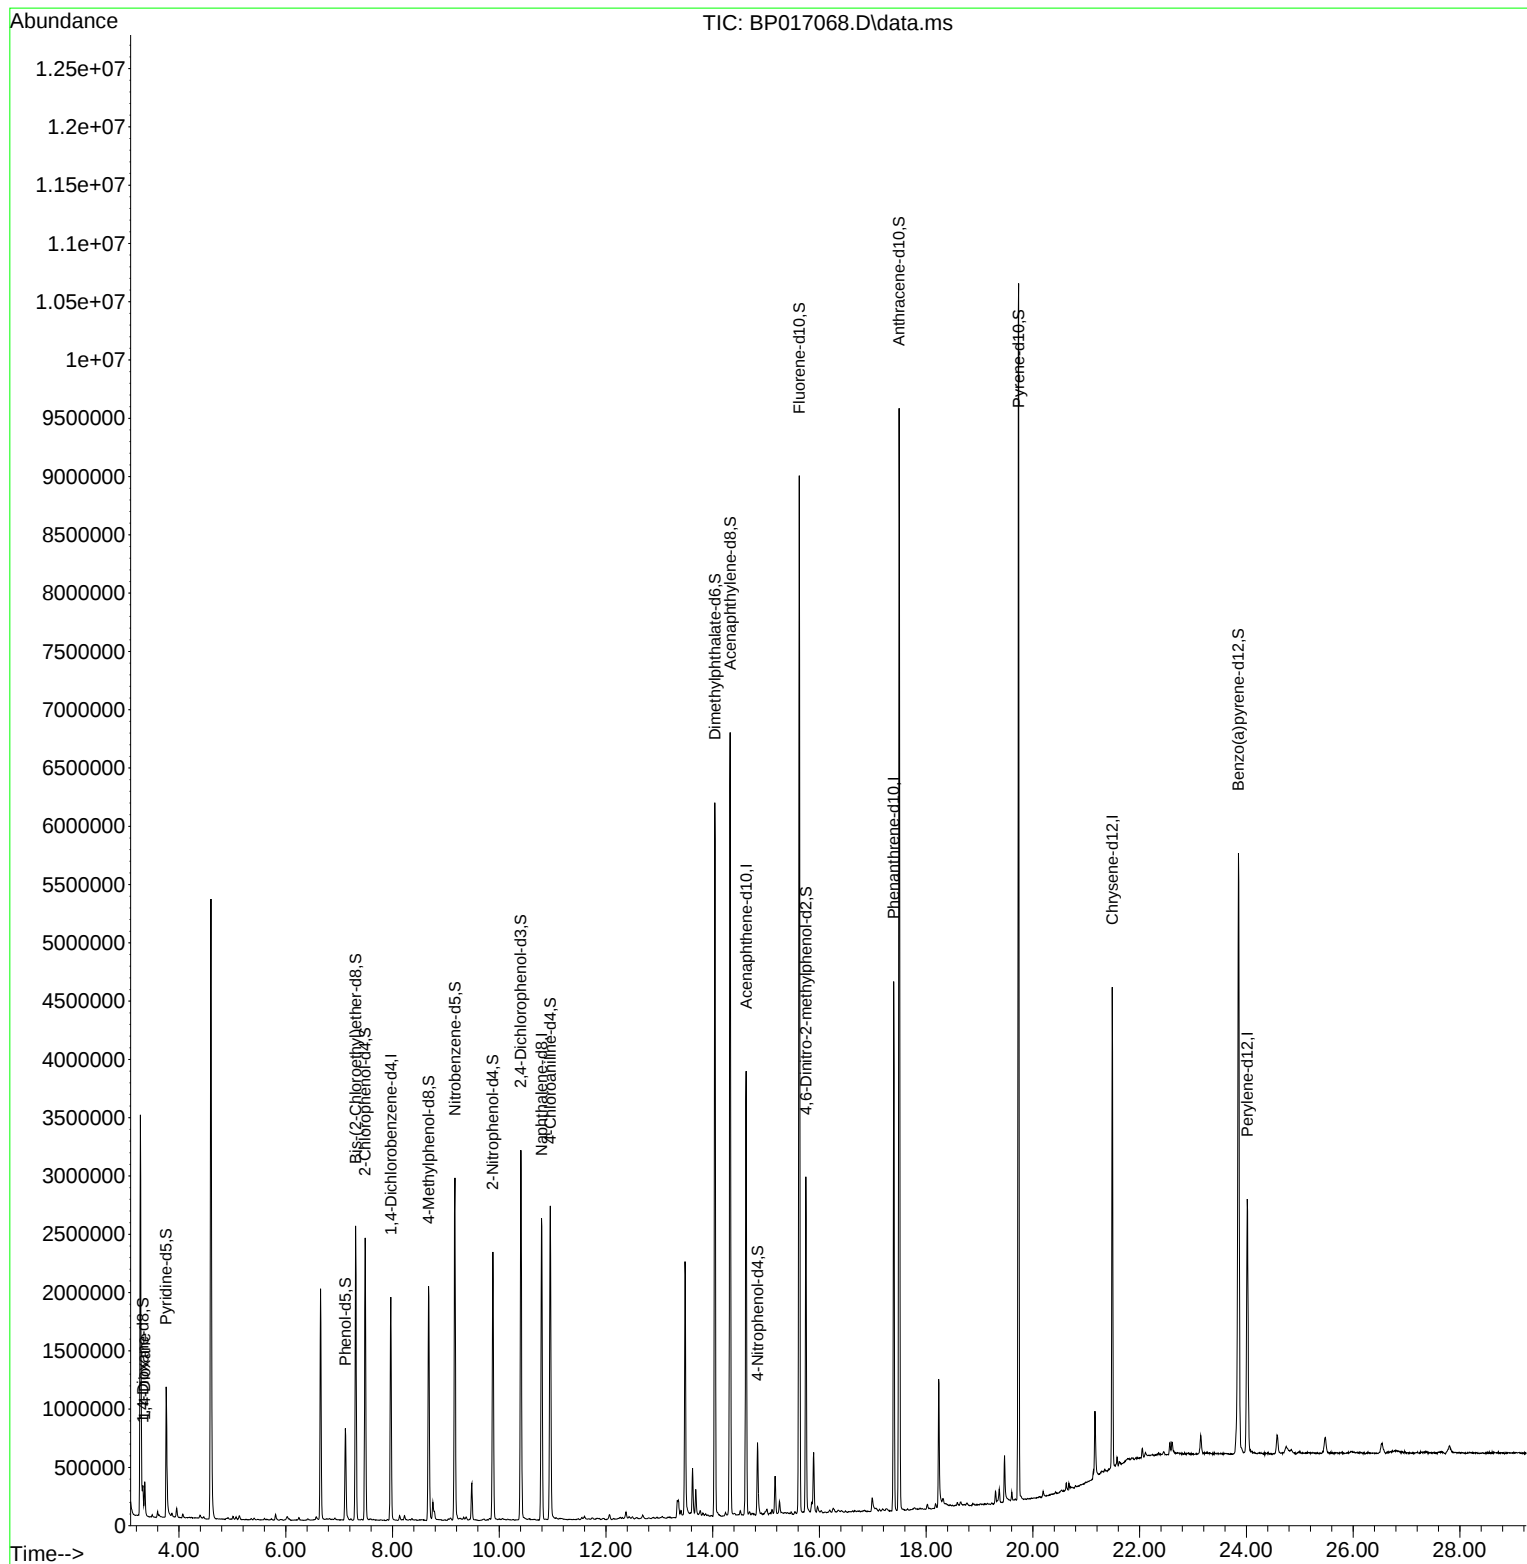

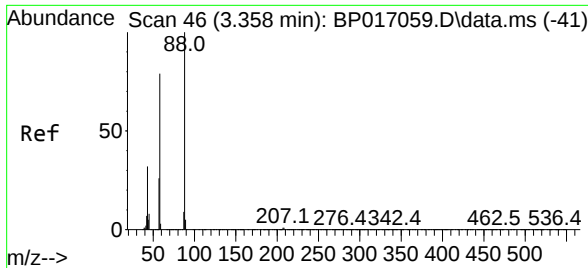

#2
 1,4-Dioxane
 Concen: 9.597 ng/uL
 RT: 3.358 min Scan# 41
 Delta R.T. -0.006 min
 Lab File: BP017068.D
 Acq: 10 Sep 2023 00:58

Instrument :
 BNA_P
 ClientSampleId :
 BBKE2

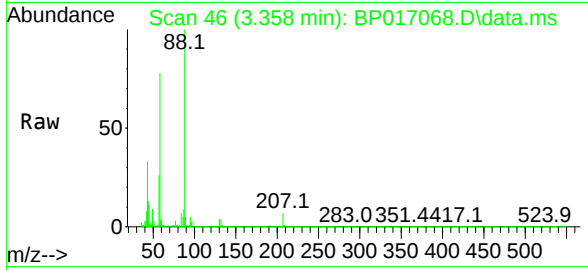

Tgt Ion: 88 Resp: 125545
 Ion Ratio Lower Upper
 88 100
 43 32.9 25.0 37.6
 58 77.7 60.6 90.8

