

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
 Data File : BP017072.D
 Acq On : 10 Sep 2023 03:15
 Operator : MA/JU
 Sample : 04227-06
 Misc :
 ALS Vial : 84 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBKE5

Quant Time: Sep 10 03:54:41 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 09 01:41:21 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.969	152	454880	20.000	ng/u1	0.00
20) Naphthalene-d8	10.793	136	1978121	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.628	164	1194164	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.392	188	2523894	20.000	ng/u1	0.00
79) Chrysene-d12	21.486	240	1872696	20.000	ng/u1	0.00
88) Perylene-d12	24.022	264	1816417	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.323	96	59588	4.955	ng/uL	0.00
4) Pyridine-d5	3.764	84	410767	11.954	ng/u1	0.00
7) Phenol-d5	7.122	99	303357	7.300	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.311	67	990237	38.094	ng/u1	0.00
11) 2-Chlorophenol-d4	7.493	132	873299	29.035	ng/u1	0.00
15) 4-Methylphenol-d8	8.699	113	581031	18.352	ng/u1	0.01
21) Nitrobenzene-d5	9.169	128	580312	37.814	ng/u1	0.00
24) 2-Nitrophenol-d4	9.881	143	602330	36.207	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.416	165	1004608	32.710	ng/u1	0.00
31) 4-Chloroaniline-d4	10.958	131	1367633	30.865	ng/u1	0.00
46) Dimethylphthalate-d6	14.040	166	3408706	38.347	ng/u1	0.00
49) Acenaphthylene-d8	14.328	160	3860311	37.630	ng/u1	0.00
54) 4-Nitrophenol-d4	14.846	143	89175	5.136	ng/u1	0.00
60) Fluorene-d10	15.622	176	2921582	38.388	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.746	200	371273	24.444	ng/u1	-0.01
73) Anthracene-d10	17.492	188	4501850	38.840	ng/u1	0.00
81) Pyrene-d10	19.728	212	4881737	42.798	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.851	264	3629863	39.391	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.358	88	281918	21.713	ng/uL	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017072.D
Acq On : 10 Sep 2023 03:15
Operator : MA/JU
Sample : 04227-06
Misc :
ALS Vial : 84 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBKE5


Quant Time: Sep 10 03:54:41 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 09 01:41:21 2023
Response via : Initial Calibration

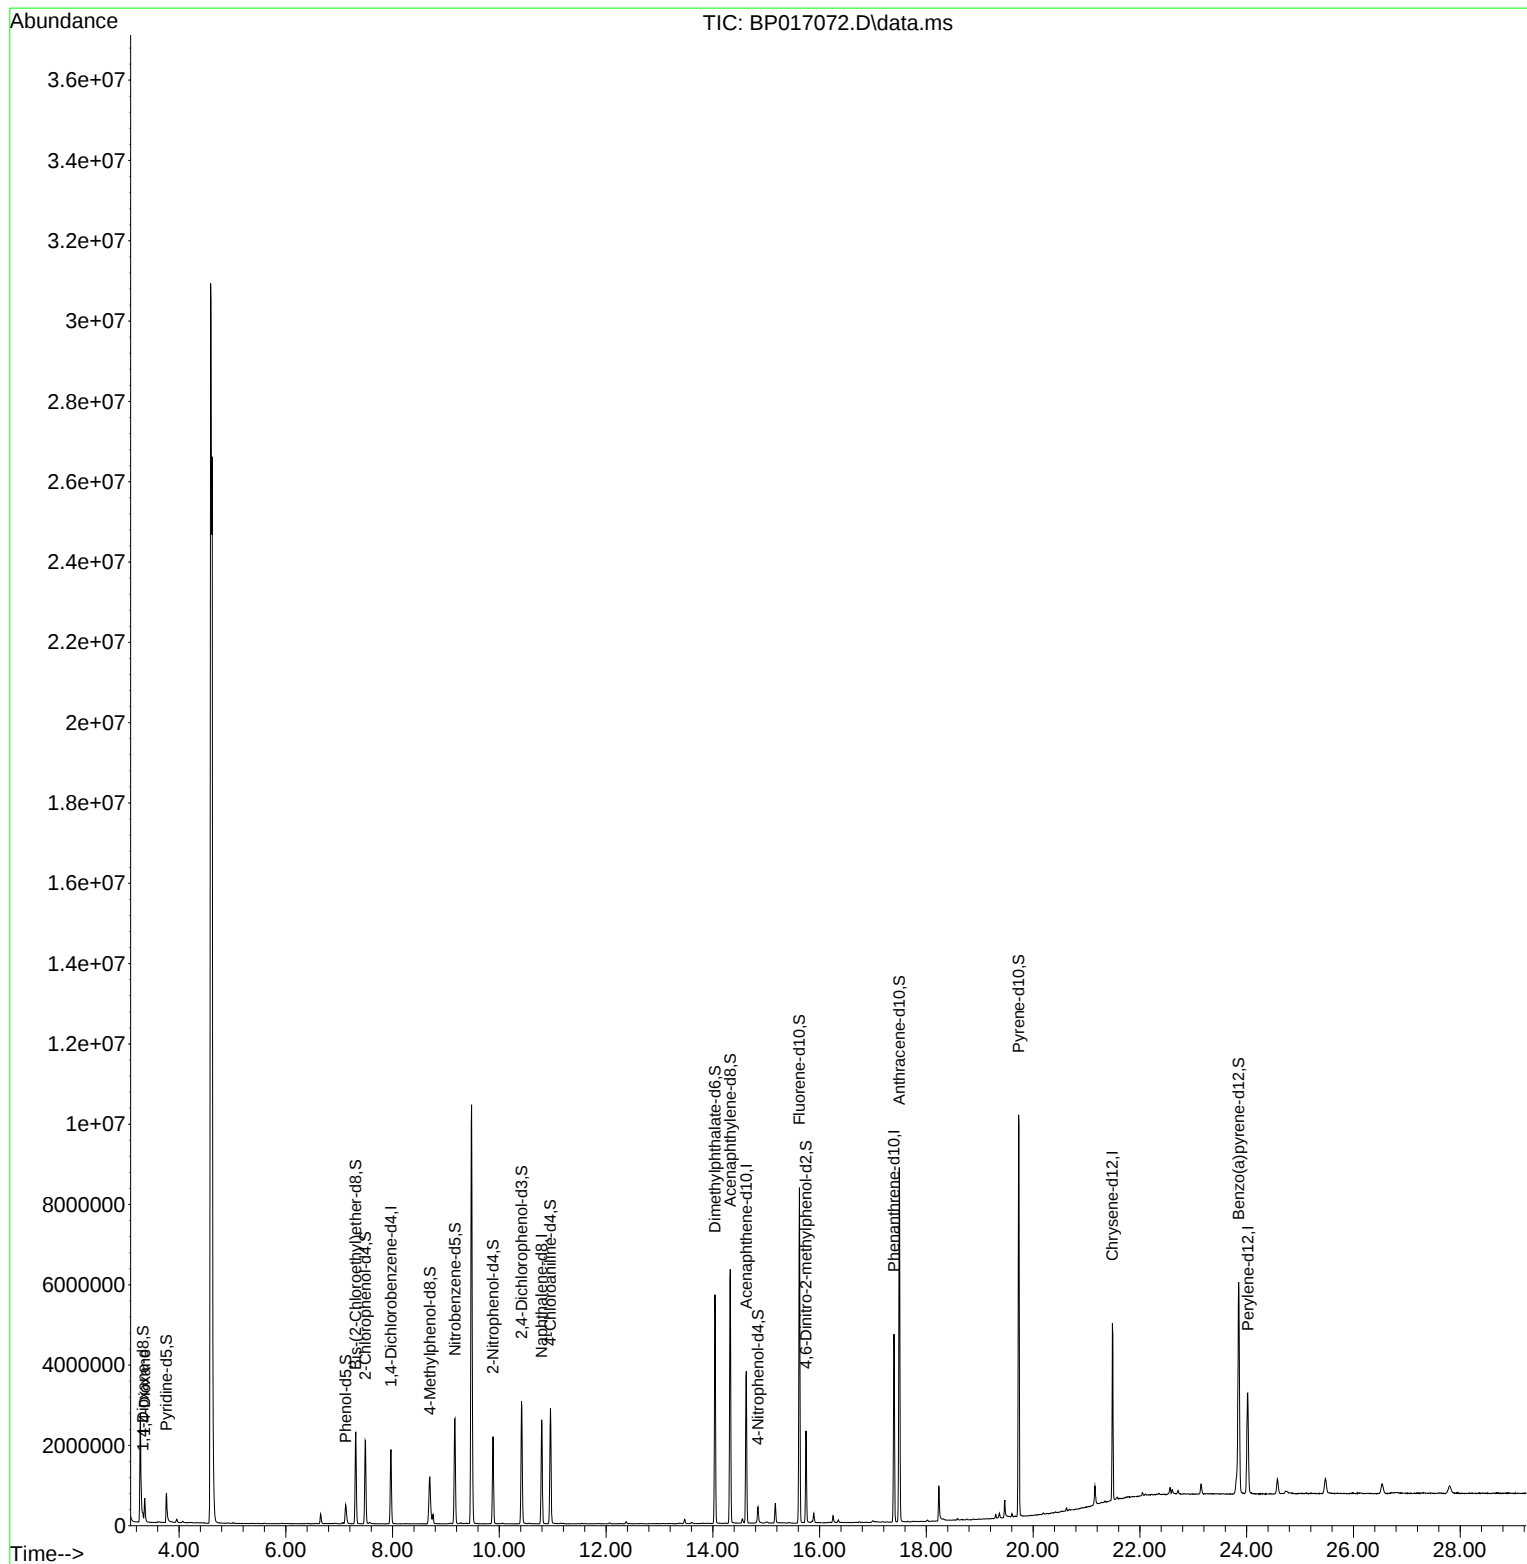

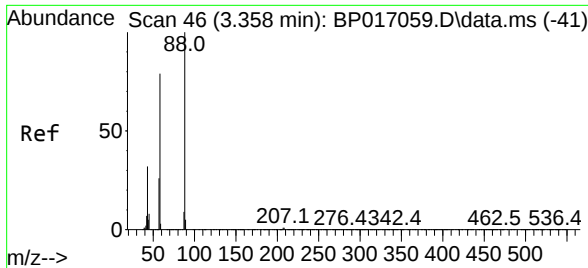

#2
 1,4-Dioxane
 Concen: 21.713 ng/uL
 RT: 3.358 min Scan# 41
 Delta R.T. -0.006 min
 Lab File: BP017072.D
 Acq: 10 Sep 2023 03:15

Instrument :
 BNA_P
 ClientSampleId :
 BBKE5

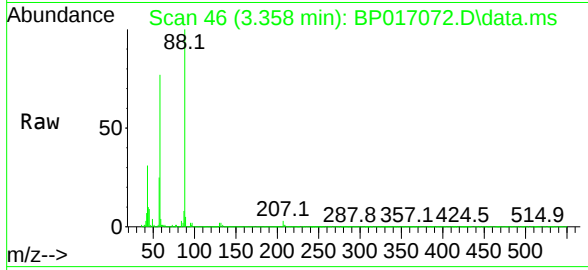

Tgt Ion: 88 Resp: 281918

Ion	Ratio	Lower	Upper
88	100		
43	31.4	25.0	37.6
58	76.8	60.6	90.8

