

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
 Data File : BP017075.D
 Acq On : 10 Sep 2023 04:58
 Operator : MA/JU
 Sample : 04227-12
 Misc :
 ALS Vial : 87 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHAT1

Quant Time: Sep 10 05:46:14 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 09 01:41:21 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.969	152	490028	20.000	ng/u1	0.00
20) Naphthalene-d8	10.793	136	2074172	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.628	164	1146723	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.392	188	2135187	20.000	ng/u1	0.00
79) Chrysene-d12	21.486	240	1334519	20.000	ng/u1	0.00
88) Perylene-d12	24.015	264	1334215	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.328	96	69013	5.327	ng/uL	0.00
4) Pyridine-d5	3.764	84	612556	16.548	ng/u1	0.00
7) Phenol-d5	7.122	99	374264	8.360	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.310	67	1228213	43.860	ng/u1	0.00
11) 2-Chlorophenol-d4	7.487	132	1091187	33.677	ng/u1	0.00
15) 4-Methylphenol-d8	8.681	113	716116	20.996	ng/u1	0.00
21) Nitrobenzene-d5	9.169	128	702476	43.655	ng/u1	0.00
24) 2-Nitrophenol-d4	9.881	143	728332	41.754	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.404	165	1224239	38.015	ng/u1	0.00
31) 4-Chloroaniline-d4	10.957	131	1490286	32.075	ng/u1	0.00
46) Dimethylphthalate-d6	14.040	166	3951090	46.288	ng/u1	0.00
49) Acenaphthylene-d8	14.328	160	4588276	46.577	ng/u1	0.00
54) 4-Nitrophenol-d4	14.845	143	83504	5.008	ng/u1	0.00
60) Fluorene-d10	15.622	176	3296599	45.107	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.745	200	461558	35.920	ng/u1	-0.01
73) Anthracene-d10	17.492	188	4653413	47.456	ng/u1	0.00
81) Pyrene-d10	19.727	212	4467737	54.964	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.851	264	3261961	48.192	ng/u1	0.00


Target Compounds					Qvalue
2) 1,4-Dioxane	3.364	88	18302	1.308 ng/uL	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017075.D
Acq On : 10 Sep 2023 04:58
Operator : MA/JU
Sample : 04227-12
Misc :
ALS Vial : 87 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHAT1


Quant Time: Sep 10 05:46:14 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 09 01:41:21 2023
Response via : Initial Calibration

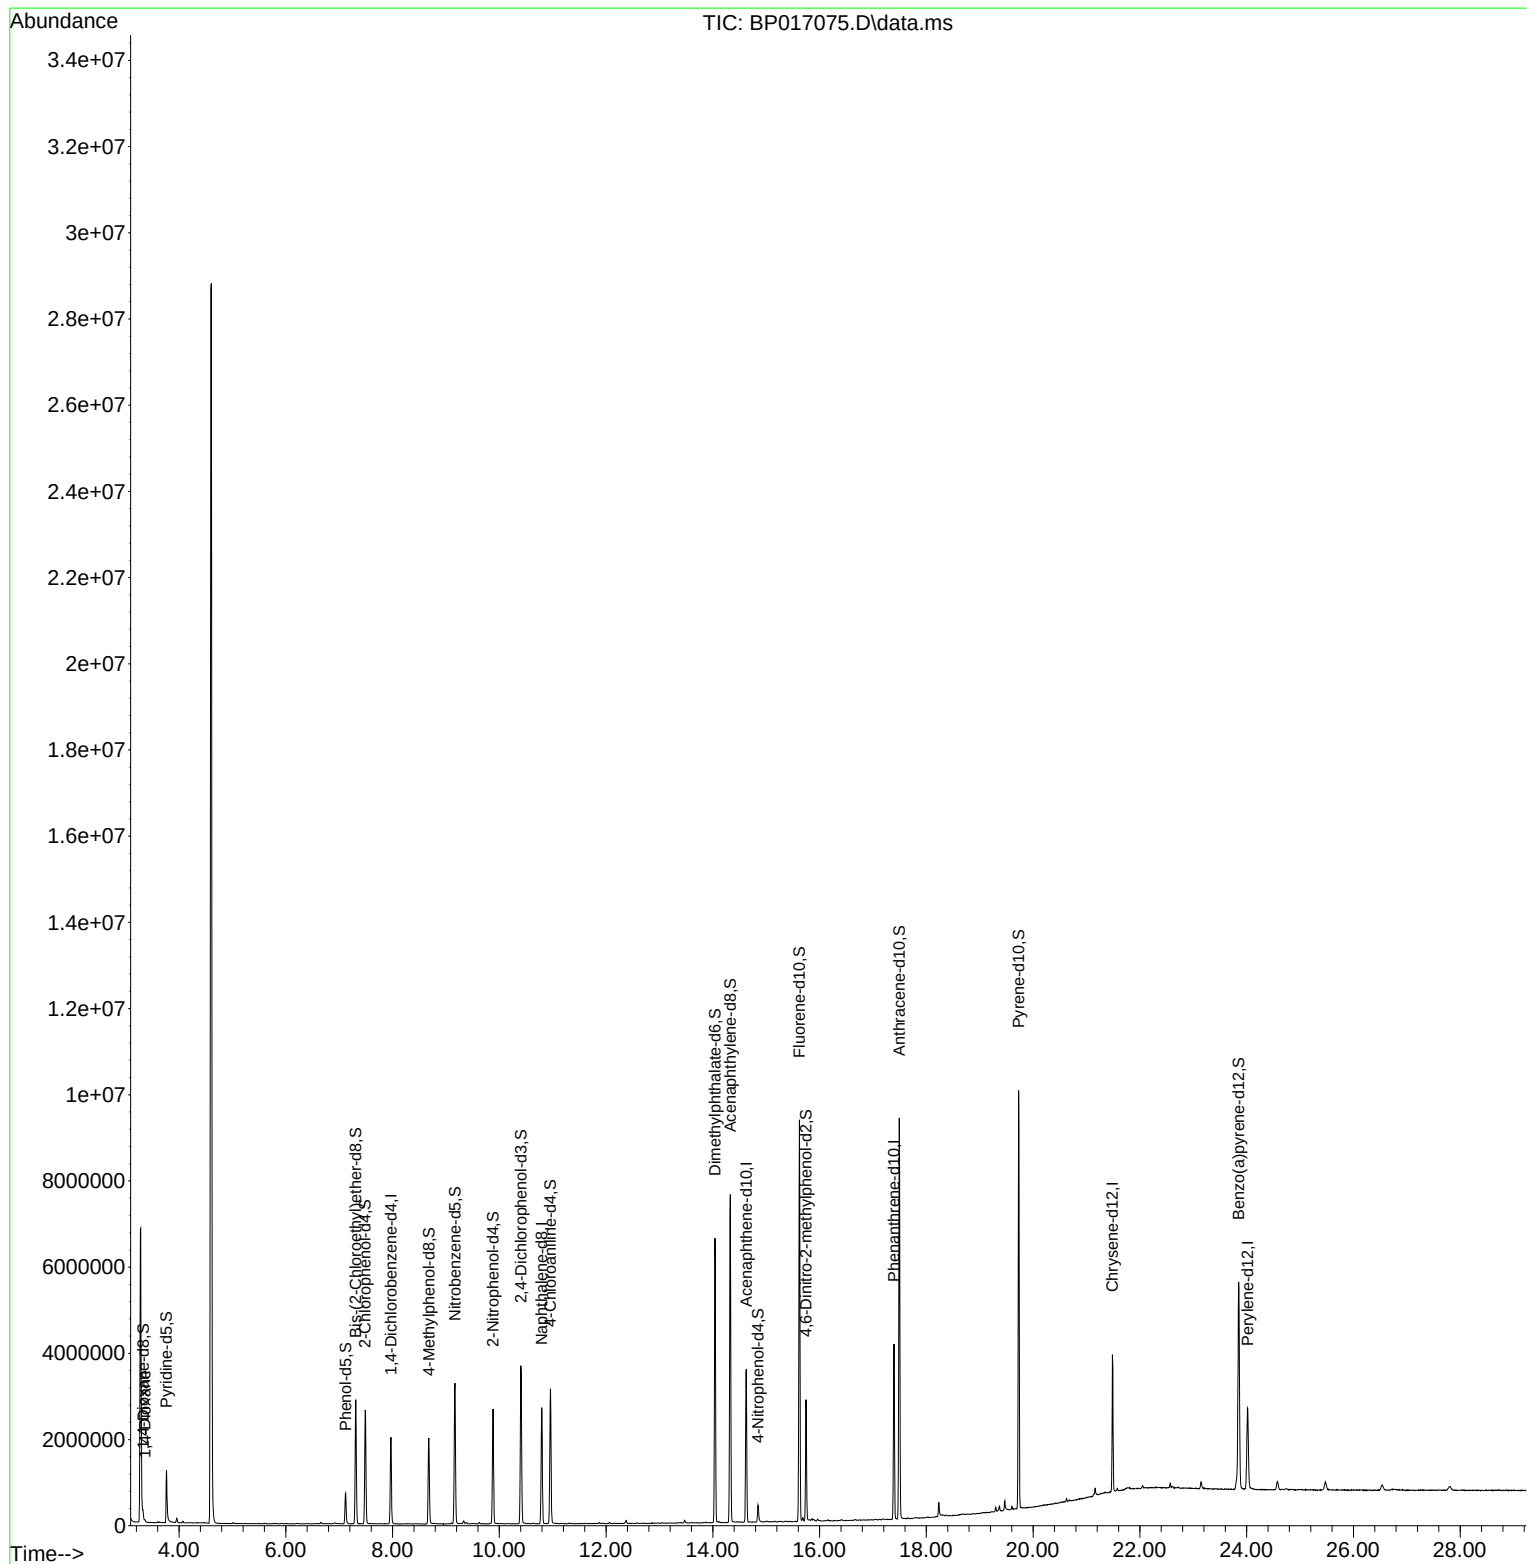

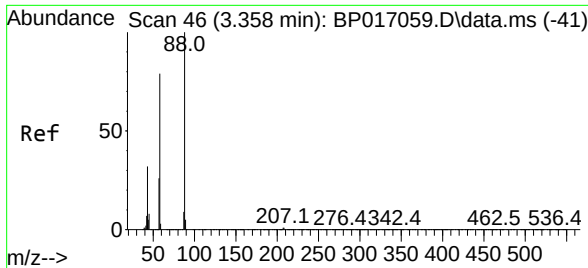

#2
 1,4-Dioxane
 Concen: 1.308 ng/uL
 RT: 3.364 min Scan# 41
 Delta R.T. -0.000 min
 Lab File: BP017075.D
 Acq: 10 Sep 2023 04:58

Instrument :
 BNA_P
 ClientSampleId :
 BHAT1

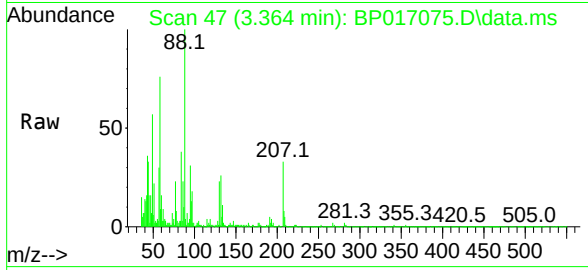

Tgt Ion: 88 Resp: 18302

Ion	Ratio	Lower	Upper
88	100		
43	35.9	25.0	37.6
58	76.4	60.6	90.8

