

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
 Data File : BP017006.D
 Acq On : 08 Sep 2023 11:37
 Operator : MA/JU
 Sample : PB155065BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK065

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017006.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.328	37	41	52	rVB	187840	256666	2.85%	0.242%
2	3.764	111	115	134	rBV	1971648	3021585	33.59%	2.851%
3	4.075	163	168	173	rBV	90807	125326	1.39%	0.118%
4	6.928	648	653	655	rBV6	5638	8995	0.10%	0.008%
5	7.122	679	686	704	rBV	2256132	3480086	38.69%	3.284%
6	7.316	712	719	731	rVB	1842635	2764210	30.73%	2.608%
7	7.493	742	749	763	rBV	2168790	3380856	37.59%	3.190%
8	7.975	823	831	846	rVB	1576279	2413009	26.83%	2.277%
9	8.681	944	951	969	rBV	2521387	4107292	45.66%	3.875%
10	9.175	1025	1035	1051	rBV	2083491	3303873	36.73%	3.117%
11	9.293	1051	1055	1059	rBV7	12722	20156	0.22%	0.019%
12	9.887	1148	1156	1172	rBV	1686981	2720144	30.24%	2.567%
13	10.410	1238	1245	1266	rBV	2423815	4012895	44.61%	3.786%
14	10.805	1303	1312	1320	rBV	2102581	3442268	38.27%	3.248%
15	10.963	1329	1339	1351	rBV	2524879	4149822	46.14%	3.915%
16	11.557	1433	1440	1443	rBV9	5633	9998	0.11%	0.009%
17	12.387	1574	1581	1588	rBV	37240	65232	0.73%	0.062%
18	12.604	1613	1618	1627	rBV	5156	13622	0.15%	0.013%
19	13.481	1761	1767	1775	rBV2	21870	36394	0.40%	0.034%
20	13.599	1780	1787	1790	rBV6	6229	10303	0.11%	0.010%
21	14.046	1856	1863	1874	rBV	4197762	5586167	62.10%	5.271%
22	14.334	1905	1912	1927	rBV	4887091	6799456	75.59%	6.415%
23	14.634	1955	1963	1973	rBV	3069131	4335843	48.20%	4.091%
24	14.846	1993	1999	2019	rBV	1974546	2871107	31.92%	2.709%
25	15.069	2035	2037	2043	rVB7	9283	11194	0.12%	0.011%
26	15.628	2125	2132	2142	rBV	6086278	8321343	92.51%	7.851%
27	15.751	2147	2153	2168	rVV	1726453	2360591	26.24%	2.227%
28	15.869	2168	2173	2180	rVB3	25746	43725	0.49%	0.041%
29	17.069	2374	2377	2381	rBV6	7836	10233	0.11%	0.010%
30	17.187	2393	2397	2401	rBV3	8563	14008	0.16%	0.013%
31	17.404	2427	2434	2444	rBV	3391119	4803175	53.40%	4.532%
32	17.504	2444	2451	2464	rBV	6174512	8497347	94.47%	8.017%
33	18.239	2572	2576	2582	rBV5	24131	40021	0.44%	0.038%
34	19.310	2754	2758	2764	rBV3	64991	88058	0.98%	0.083%
35	19.381	2766	2770	2775	rVB	58471	81550	0.91%	0.077%
36	19.475	2784	2786	2789	rBV4	18142	16675	0.19%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017006.D
Acq On : 08 Sep 2023 11:37
Operator : MA/JU
Sample : PB155065BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK065

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Title : SVOA CALIBRATION

37	19.739	2825	2831	2837	rBV	7190719	8994847	100.00%	8.487%
38	21.498	3125	3130	3136	rBV	3218889	3990051	44.36%	3.765%
39	23.869	3524	3533	3544	rVB2	3781959	8014402	89.10%	7.562%
40	24.039	3555	3562	3572	rVB	1806005	3763830	41.84%	3.551%




Sum of corrected areas: 105986355

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017006.D
Acq On : 08 Sep 2023 11:37
Operator : MA/JU
Sample : PB155065BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK065

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

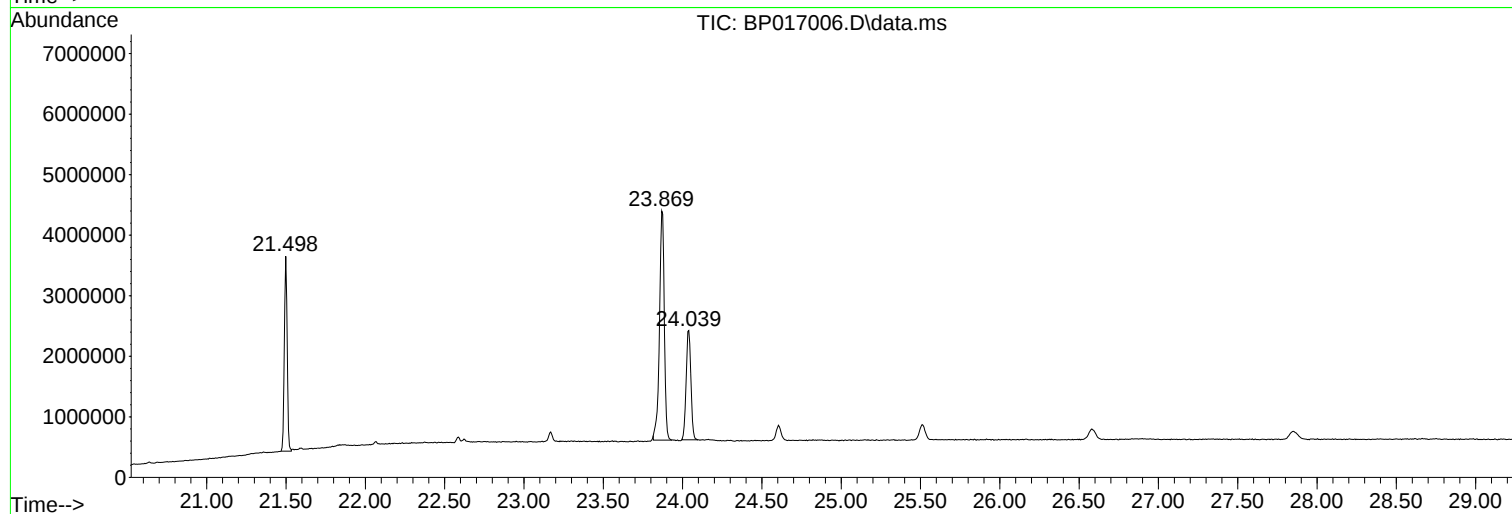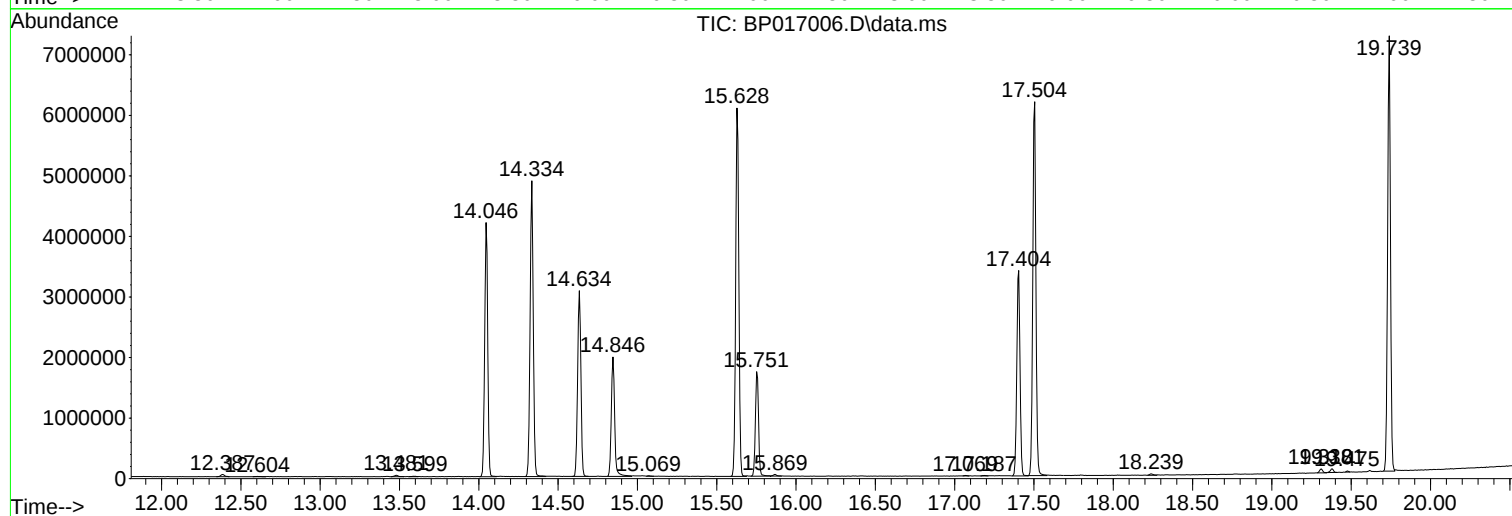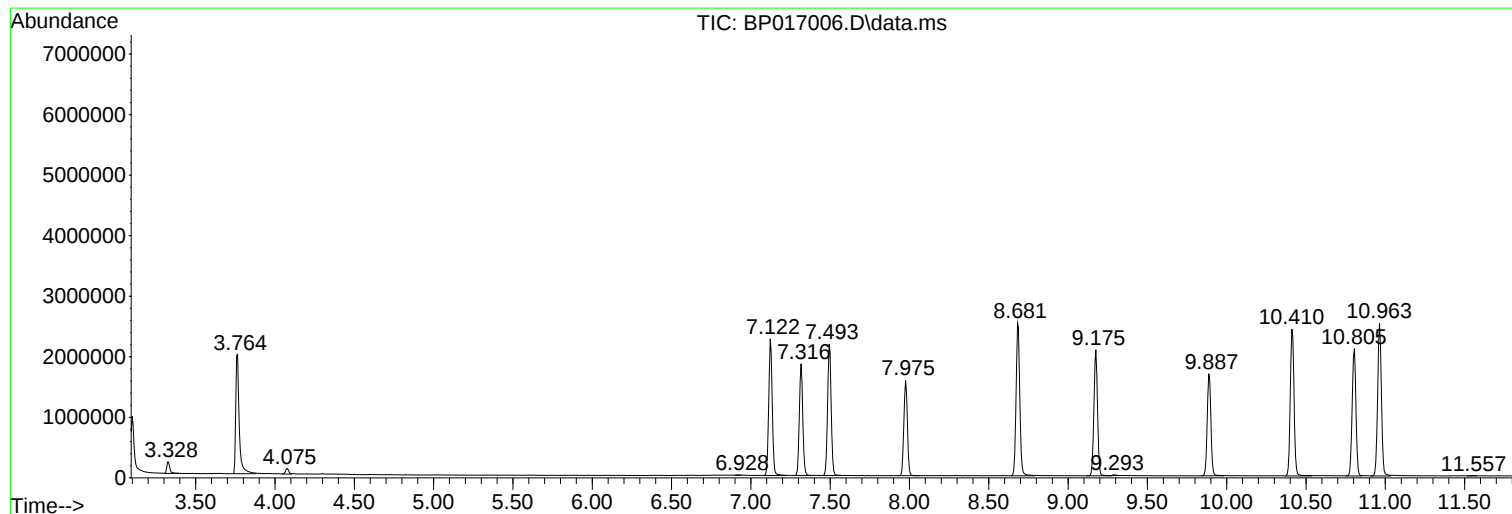

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017006.D
Acq On : 08 Sep 2023 11:37
Operator : MA/JU
Sample : PB155065BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK065

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017006.D
Acq On : 08 Sep 2023 11:37
Operator : MA/JU
Sample : PB155065BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK065

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------