

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
 Data File : BP017009.D
 Acq On : 08 Sep 2023 13:20
 Operator : MA/JU
 Sample : 04123-11
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH9H3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017009.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.322	37	40	51	rVB	177129	246306	1.57%	0.164%
2	3.628	89	92	98	rVB	19210	29958	0.19%	0.020%
3	3.764	111	115	130	rBV	860846	1311720	8.36%	0.875%
4	3.964	144	149	157	rVB	82183	132390	0.84%	0.088%
5	4.075	164	168	179	rVB	30015	50922	0.32%	0.034%
6	4.463	231	234	245	rVB4	24327	46750	0.30%	0.031%
7	4.605	253	258	264	rBV	100767	147135	0.94%	0.098%
8	5.016	323	328	333	rBV	30829	43634	0.28%	0.029%
9	5.605	423	428	436	rVB3	15056	25287	0.16%	0.017%
10	6.922	648	652	662	rVB3	18968	41235	0.26%	0.028%
11	7.122	679	686	701	rBV	820943	1267343	8.08%	0.846%
12	7.316	710	719	728	rBV	2619517	3919897	25.00%	2.616%
13	7.493	742	749	760	rBV	2399947	3865685	24.65%	2.580%
14	7.581	760	764	771	rVB2	14420	26450	0.17%	0.018%
15	7.975	824	831	842	rBV	1917324	2954942	18.84%	1.972%
16	8.681	944	951	963	rBV	2079949	3396248	21.66%	2.266%
17	9.051	1008	1014	1018	rBV6	14755	27489	0.18%	0.018%
18	9.175	1025	1035	1048	rBV	3068560	4854841	30.96%	3.240%
19	9.340	1058	1063	1068	rBV2	48740	79456	0.51%	0.053%
20	9.393	1068	1072	1077	rVB6	19841	33641	0.21%	0.022%
21	9.634	1108	1113	1119	rVB	17130	25434	0.16%	0.017%
22	9.763	1130	1135	1140	rVB	29205	48241	0.31%	0.032%
23	9.834	1142	1147	1150	rBV5	11303	22306	0.14%	0.015%
24	9.887	1150	1156	1173	rVB	2400772	3926559	25.04%	2.620%
25	10.046	1177	1183	1193	rVB2	18698	43692	0.28%	0.029%
26	10.146	1196	1200	1206	rBV2	17213	28590	0.18%	0.019%
27	10.410	1237	1245	1262	rBV	3352749	5702846	36.37%	3.806%
28	10.563	1266	1271	1279	rVV	7266	22747	0.15%	0.015%
29	10.651	1283	1286	1292	rVB5	16751	27242	0.17%	0.018%
30	10.804	1299	1312	1320	rBV	2676209	4461907	28.45%	2.977%
31	10.963	1331	1339	1354	rBV	2862013	4734013	30.19%	3.159%
32	11.451	1418	1422	1425	rBV4	13761	20545	0.13%	0.014%
33	11.493	1425	1429	1434	rVB6	12248	22856	0.15%	0.015%
34	11.545	1434	1438	1445	rBV9	12346	28226	0.18%	0.019%
35	11.622	1447	1451	1457	rVB4	18014	29106	0.19%	0.019%
36	11.816	1477	1484	1485	rBV6	10786	18506	0.12%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
 Data File : BP017009.D
 Acq On : 08 Sep 2023 13:20
 Operator : MA/JU
 Sample : 04123-11
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH9H3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
 Title : SVOA CALIBRATION

37	11.916	1496	1501	1504	rBV	26414	38122	0.24%	0.025%
38	11.957	1504	1508	1512	rVB7	19948	32590	0.21%	0.022%
39	12.075	1520	1528	1537	rBV2	68251	147683	0.94%	0.099%
40	12.263	1555	1560	1563	rBV3	12581	22010	0.14%	0.015%
41	12.381	1575	1580	1587	rVB2	65012	110196	0.70%	0.074%
42	12.504	1599	1601	1607	rVB6	14218	17434	0.11%	0.012%
43	12.598	1613	1617	1623	rVB9	8146	16283	0.10%	0.011%
44	12.722	1634	1638	1642	rBV6	11935	19245	0.12%	0.013%
45	12.869	1657	1663	1667	rBV8	17530	37874	0.24%	0.025%
46	12.910	1667	1670	1675	rVB5	17569	27758	0.18%	0.019%
47	13.092	1689	1701	1707	rBV4	47502	95632	0.61%	0.064%
48	13.169	1707	1714	1718	rBV5	18528	46635	0.30%	0.031%
49	13.310	1734	1738	1741	rVB4	16464	21345	0.14%	0.014%
50	13.481	1762	1767	1777	rVB2	40272	78496	0.50%	0.052%
51	13.628	1788	1792	1801	rVB6	30618	59952	0.38%	0.040%
52	13.751	1808	1813	1819	rVB9	12386	27277	0.17%	0.018%
53	13.851	1828	1830	1838	rVB7	12846	19745	0.13%	0.013%
54	14.051	1857	1864	1871	rBV	6579868	8884003	56.65%	5.928%
55	14.257	1894	1899	1904	rBV	42571	76633	0.49%	0.051%
56	14.334	1905	1912	1923	rVV	7465346	10701791	68.25%	7.141%
57	14.634	1955	1963	1971	rBV	4061835	5818327	37.10%	3.883%
58	14.757	1981	1984	1986	rBV3	13449	18419	0.12%	0.012%
59	14.845	1993	1999	2015	rBV	702420	1074759	6.85%	0.717%
60	15.122	2043	2046	2051	rVB6	13234	21846	0.14%	0.015%
61	15.257	2062	2069	2075	rBV6	15499	41949	0.27%	0.028%
62	15.586	2119	2125	2126	rBV4	25858	37217	0.24%	0.025%
63	15.633	2126	2133	2139	rVV	9450855	13190540	84.12%	8.802%
64	15.692	2139	2143	2148	rVB	171742	226795	1.45%	0.151%
65	15.757	2148	2154	2161	rBV	3379748	4319800	27.55%	2.883%
66	15.869	2170	2173	2178	rVB	38317	49170	0.31%	0.033%
67	15.922	2179	2182	2189	rVB9	22264	42652	0.27%	0.028%
68	16.416	2263	2266	2271	rVB3	26501	35893	0.23%	0.024%
69	17.404	2428	2434	2444	rVB	4789913	6690626	42.67%	4.465%
70	17.504	2444	2451	2460	rBV2	10239940	14164424	90.33%	9.452%
71	18.245	2572	2577	2583	rBV	270189	399466	2.55%	0.267%
72	19.310	2755	2758	2762	rBV	113342	133749	0.85%	0.089%
73	19.380	2766	2770	2773	rVB	118304	144168	0.92%	0.096%
74	19.474	2783	2786	2800	rBV2	177134	267864	1.71%	0.179%
75	19.616	2807	2810	2816	rBV2	75123	85869	0.55%	0.057%
76	19.739	2825	2831	2837	rBV	12273913	15681387	100.00%	10.464%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017009.D
Acq On : 08 Sep 2023 13:20
Operator : MA/JU
Sample : 04123-11
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH9H3

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Title : SVOA CALIBRATION

77	21.498	3125	3130	3138	rBV	4632755	5992094	38.21%	3.999%
78	23.168	3411	3414	3420	rVB	255510	391756	2.50%	0.261%
79	23.874	3523	3534	3546	rVB2	6087340	12986666	82.82%	8.666%
80	24.039	3555	3562	3572	rVB	2537962	5166916	32.95%	3.448%
81	24.604	3654	3658	3670	rVB2	360548	729017	4.65%	0.486%




Sum of corrected areas: 149856218

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017009.D
Acq On : 08 Sep 2023 13:20
Operator : MA/JU
Sample : 04123-11
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH9H3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

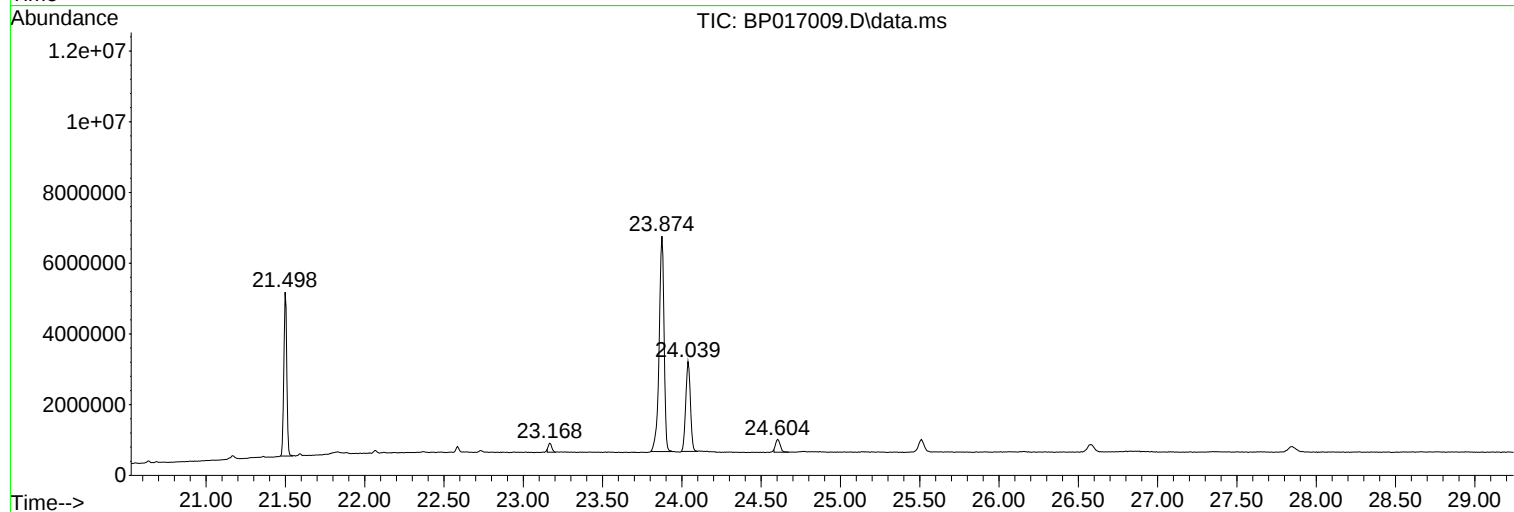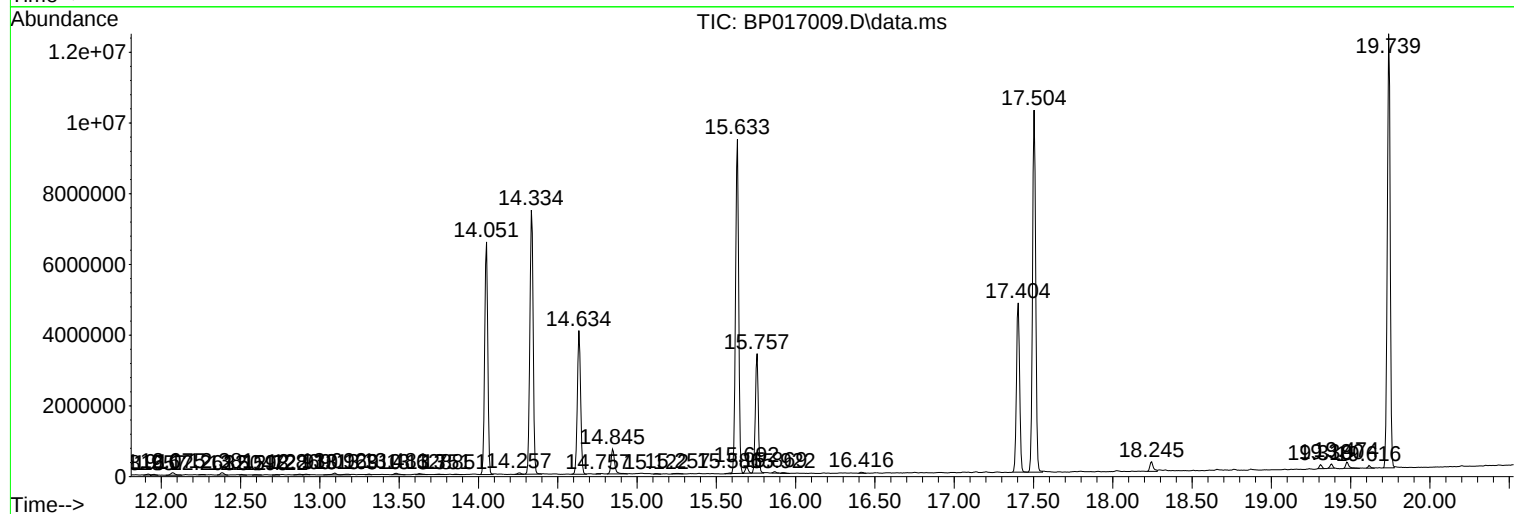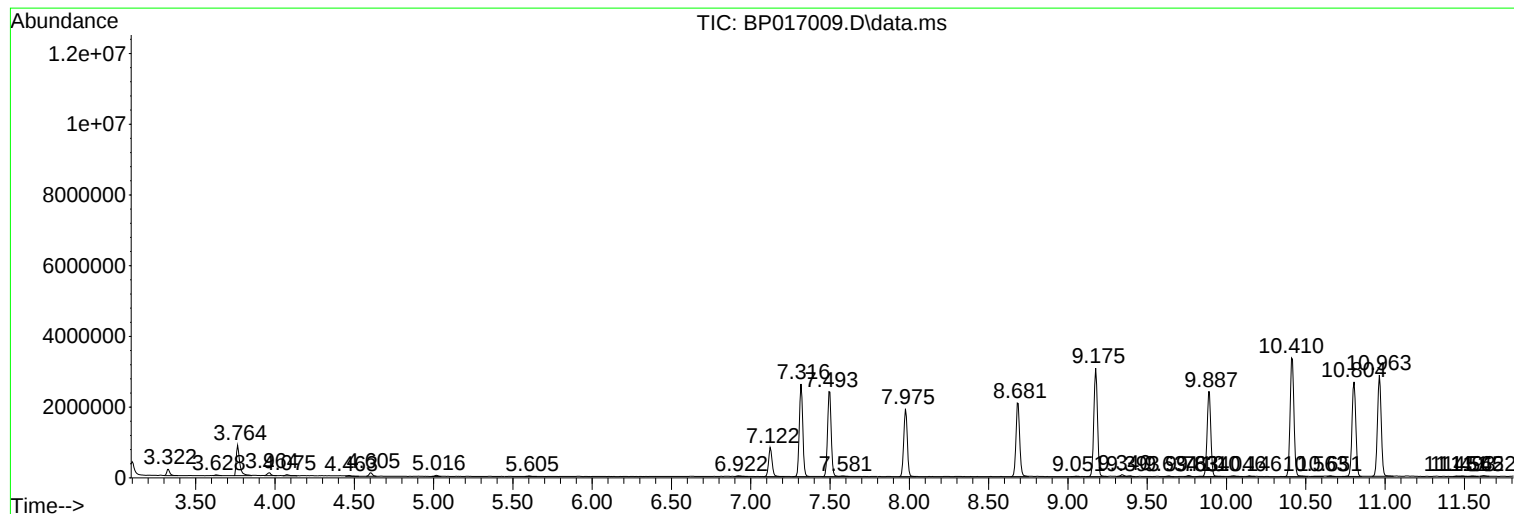

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017009.D
Acq On : 08 Sep 2023 13:20
Operator : MA/JU
Sample : 04123-11
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH9H3










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
24.604	2.82 ng/ul	729017	Perylene-d12	24.039

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Heneicosane, 11-(1-ethylpropyl)-	366	C26H54	055282-11-6	80
2			Hexacosane	366	C26H54	000630-01-3	76
3			Di-n-decylsulfone	346	C20H42O2S	111530-37-1	72
4			Tetradecane, 1-iodo-	324	C14H29I	019218-94-1	72
5			Hexacosane	366	C26H54	000630-01-3	70

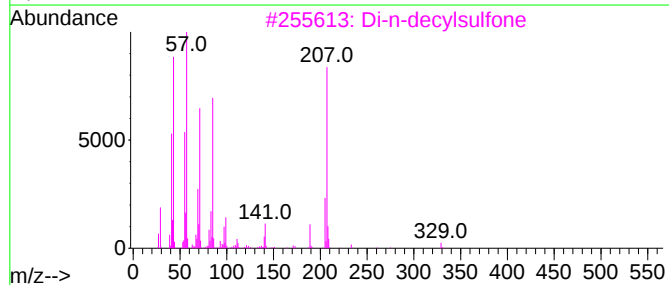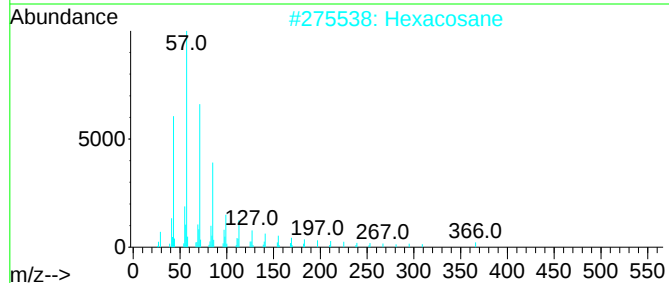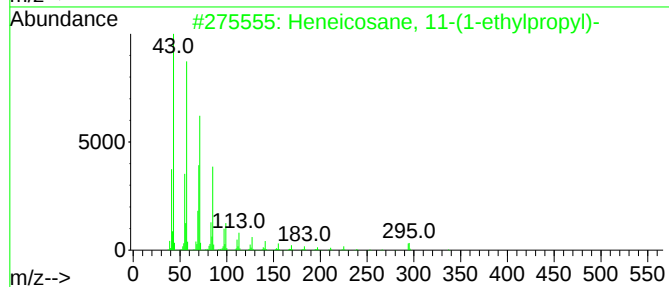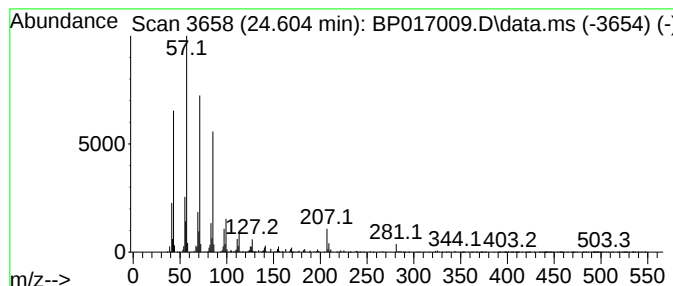

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017009.D
Acq On : 08 Sep 2023 13:20
Operator : MA/JU
Sample : 04123-11
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH9H3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	24.604	2.8	ng/u1	729017	6	24.039	5166920	20.0