

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
 Data File : BP017015.D
 Acq On : 08 Sep 2023 16:47
 Operator : MA/JU
 Sample : 04123-17
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH9F9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017015.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.322	36	40	53	rVB	145369	218652	1.59%	0.162%
2	3.628	89	92	99	rBV3	22098	40249	0.29%	0.030%
3	3.764	111	115	129	rBV	572994	918064	6.69%	0.682%
4	3.964	143	149	155	rVB	69188	106910	0.78%	0.079%
5	4.075	163	168	176	rBV	170352	245317	1.79%	0.182%
6	4.463	231	234	244	rVB5	20650	38402	0.28%	0.029%
7	4.605	252	258	266	rBV	286452	444161	3.24%	0.330%
8	5.016	323	328	337	rVB	26547	44069	0.32%	0.033%
9	5.605	424	428	432	rBV2	11699	15431	0.11%	0.011%
10	6.928	648	653	659	rVB3	14314	23546	0.17%	0.017%
11	7.122	680	686	700	rBV	667431	1018392	7.42%	0.757%
12	7.316	712	719	731	rBV	2311878	3512329	25.61%	2.610%
13	7.493	741	749	760	rBV	2115836	3414577	24.89%	2.537%
14	7.975	824	831	842	rBV	1782037	2747305	20.03%	2.042%
15	8.681	941	951	965	rBV	1713875	2825838	20.60%	2.100%
16	9.175	1028	1035	1047	rBV	2712087	4314608	31.46%	3.206%
17	9.887	1147	1156	1166	rBV	2122821	3480024	25.37%	2.586%
18	10.410	1237	1245	1258	rBV	3021410	4935292	35.98%	3.668%
19	10.804	1304	1312	1319	rBV	2525087	4100565	29.90%	3.047%
20	10.963	1330	1339	1356	rBV	2803073	4627755	33.74%	3.439%
21	11.551	1436	1439	1447	rBV6	11624	22938	0.17%	0.017%
22	11.798	1474	1481	1491	rBV	109098	253615	1.85%	0.188%
23	12.387	1574	1581	1588	rBV2	50272	86661	0.63%	0.064%
24	12.881	1653	1665	1666	rBV2	5549	14379	0.10%	0.011%
25	13.481	1761	1767	1772	rBV	34863	56495	0.41%	0.042%
26	14.045	1856	1863	1875	rBV	5463918	7619917	55.55%	5.663%
27	14.334	1905	1912	1928	rBV	6728494	9306514	67.85%	6.916%
28	14.634	1953	1963	1971	rBV	3724901	5366213	39.12%	3.988%
29	14.751	1979	1983	1990	rBV10	8295	15133	0.11%	0.011%
30	14.845	1992	1999	2016	rBV	512914	824194	6.01%	0.612%
31	15.416	2093	2096	2109	rVB4	17662	37639	0.27%	0.028%
32	15.628	2124	2132	2141	rBV	8184963	11530518	84.07%	8.569%
33	15.751	2147	2153	2161	rBV	2704152	3573921	26.06%	2.656%
34	15.863	2169	2172	2179	rVB	35573	52786	0.38%	0.039%
35	16.292	2240	2245	2251	rBV2	44113	85346	0.62%	0.063%
36	17.086	2372	2380	2384	rBV2	40855	69870	0.51%	0.052%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
 Data File : BP017015.D
 Acq On : 08 Sep 2023 16:47
 Operator : MA/JU
 Sample : 04123-17
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH9F9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
 Title : SVOA CALIBRATION

37	17.128	2384	2387	2391	rVB3	30849	41702	0.30%	0.031%
38	17.398	2427	2433	2442	rBV	4382145	6305398	45.97%	4.686%
39	17.504	2444	2451	2459	rBV	8675373	12292077	89.62%	9.135%
40	17.833	2503	2507	2512	rVB2	30585	38193	0.28%	0.028%
41	18.022	2536	2539	2544	rVB3	30058	38323	0.28%	0.028%
42	18.239	2571	2576	2585	rBV	298721	434408	3.17%	0.323%
43	18.504	2618	2621	2626	rBV3	37607	43766	0.32%	0.033%
44	19.116	2723	2725	2728	rVB2	27200	24842	0.18%	0.018%
45	19.310	2754	2758	2762	rBV	94143	116518	0.85%	0.087%
46	19.374	2766	2769	2777	rVB	109690	152944	1.12%	0.114%
47	19.474	2782	2786	2792	rBV	189006	251659	1.83%	0.187%
48	19.616	2807	2810	2814	rVB	57984	60110	0.44%	0.045%
49	19.739	2825	2831	2837	rBV	10908991	13716006	100.00%	10.193%
50	20.633	2981	2983	2988	rVB3	57307	53753	0.39%	0.040%
51	21.163	3070	3073	3082	rVB3	140846	216327	1.58%	0.161%
52	21.498	3125	3130	3136	rBV	4516514	5863642	42.75%	4.357%
53	23.163	3409	3413	3421	rVB	243357	390094	2.84%	0.290%
54	23.868	3522	3533	3548	rVB2	5677054	12489090	91.05%	9.281%
55	24.033	3554	3561	3572	rVB	2702419	5374309	39.18%	3.994%
56	24.592	3652	3656	3664	rVB	341120	675588	4.93%	0.502%




Sum of corrected areas: 134566374

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017015.D
Acq On : 08 Sep 2023 16:47
Operator : MA/JU
Sample : 04123-17
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH9F9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

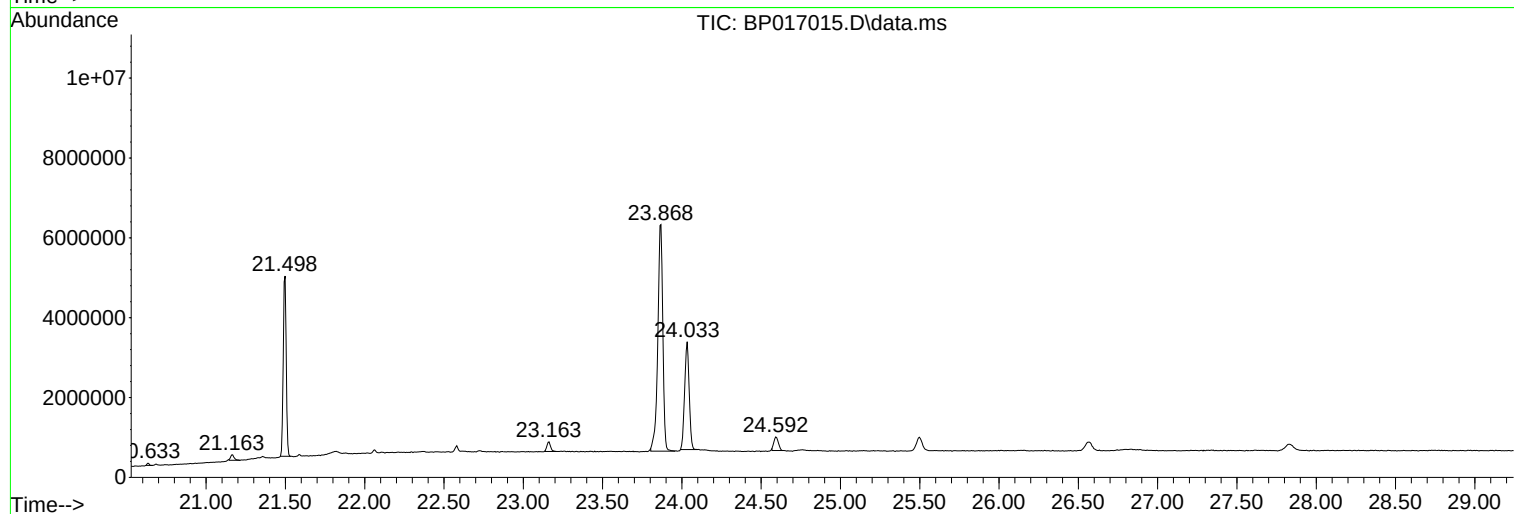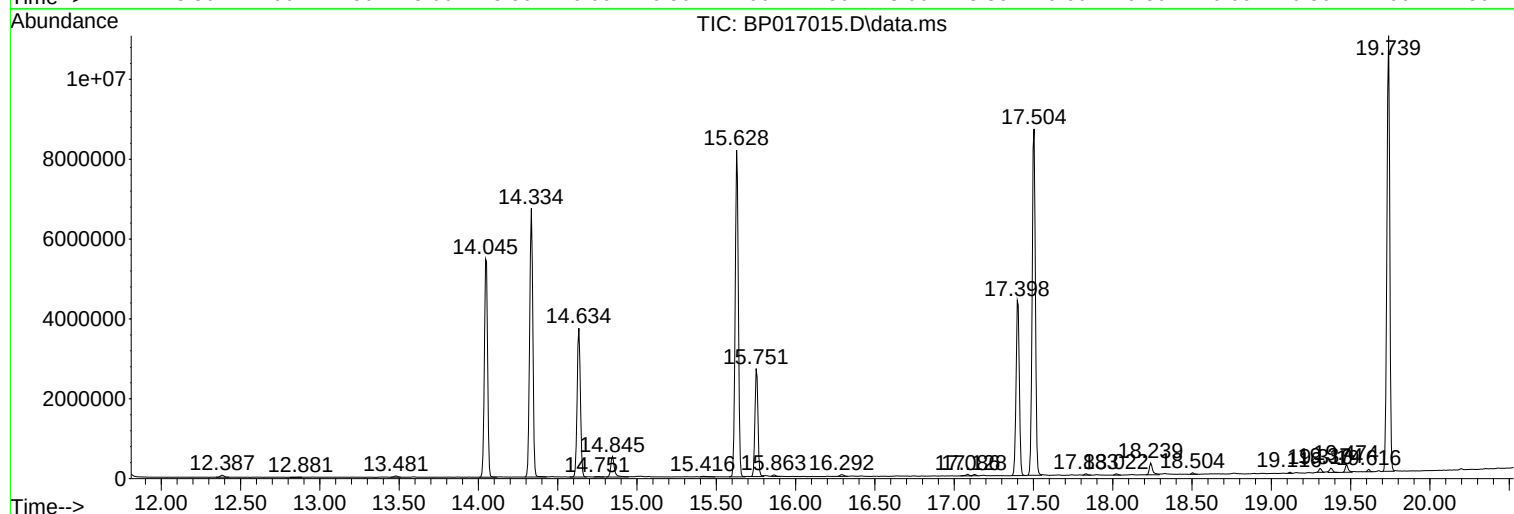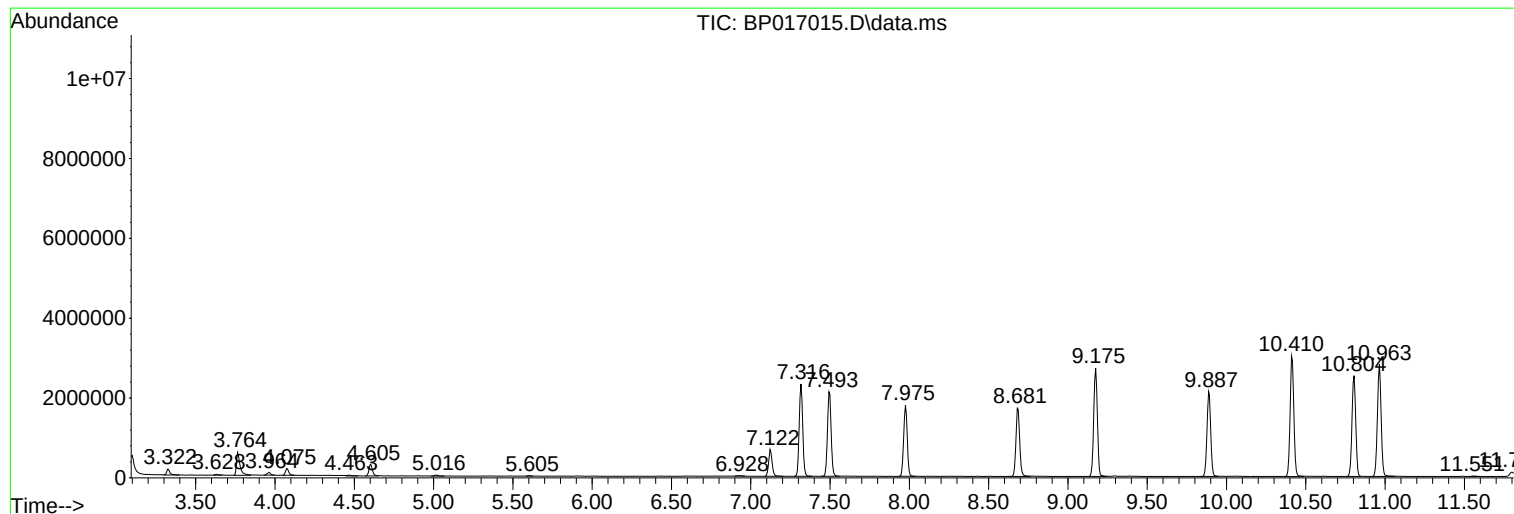

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017015.D
Acq On : 08 Sep 2023 16:47
Operator : MA/JU
Sample : 04123-17
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH9F9










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.605	3.23 ng/ul	444161	1,4-Dichlorobenzene-d4	7.975

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	99
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
5			Pyrimidine, 5-fluoro-2,4-dichloro-	166	C4HC12FN2	002927-71-1	38

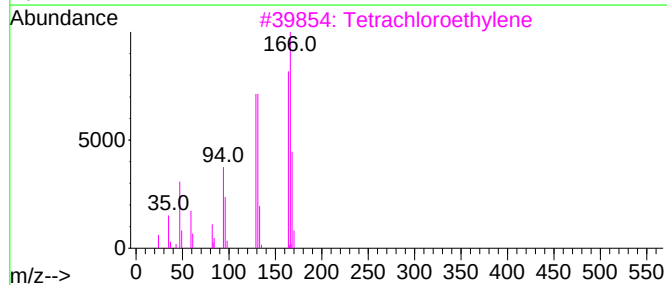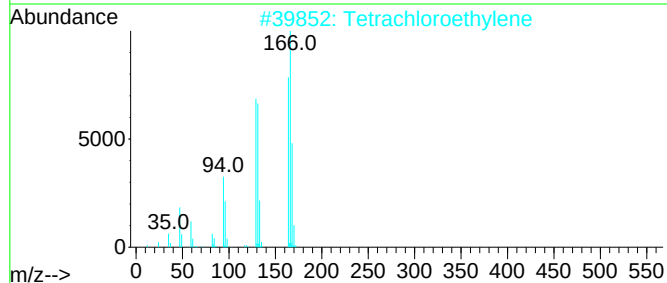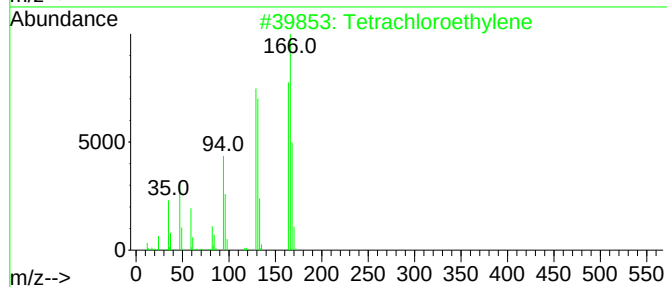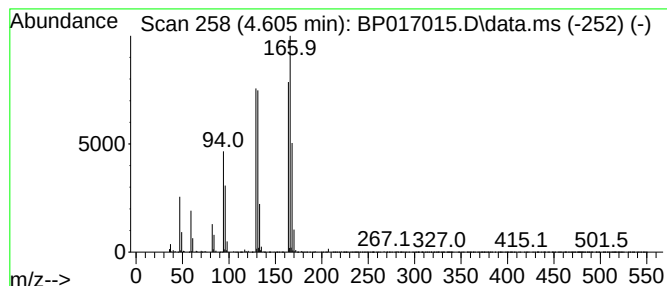

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017015.D
Acq On : 08 Sep 2023 16:47
Operator : MA/JU
Sample : 04123-17
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH9F9










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 (DEL) Alkane: Straight-Chai... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
24.592	2.51 ng/ul	675588	Perylene-d12	24.033

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		Octacosane, 2-methyl-	408	C29H60	001560-98-1	91
2		Heneicosane	296	C21H44	000629-94-7	91
3		Hexatriacontane	507	C36H74	000630-06-8	91
4		Hexacosane	366	C26H54	000630-01-3	91
5		Tetracosane	338	C24H50	000646-31-1	91

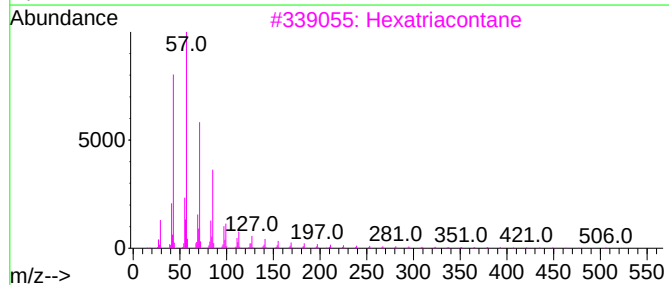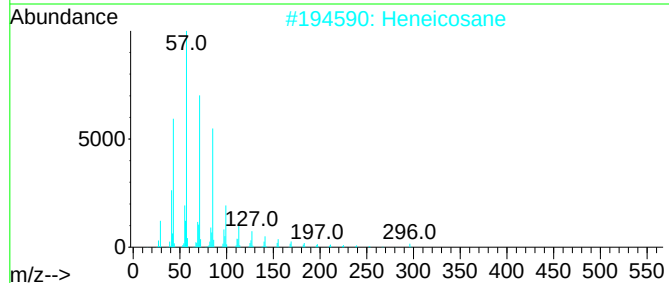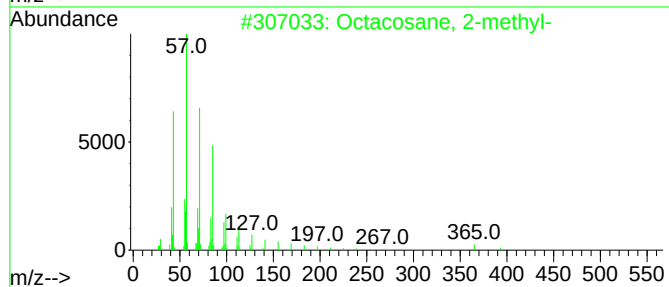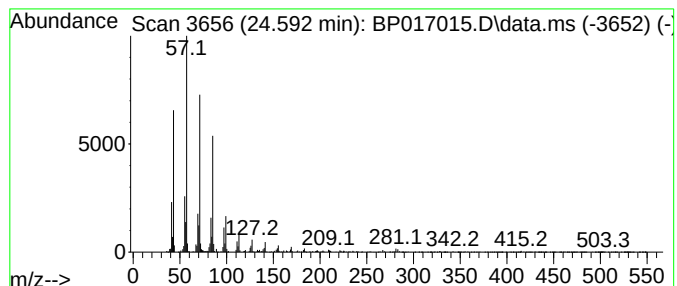

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017015.D
Acq On : 08 Sep 2023 16:47
Operator : MA/JU
Sample : 04123-17
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH9F9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.605	3.2	ng/u1	444161	1	7.975	2747310	20.0
(DEL) Alkane: S...	24.592	2.5	ng/u1	675588	6	24.033	5374310	20.0