

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
 Data File : BP017028.D
 Acq On : 09 Sep 2023 00:52
 Operator : MA/JU
 Sample : 04153-07
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH465

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017028.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	28	32	37	rBV2	50366	72093	0.65%	0.070%
2	3.322	37	40	51	rVB	86460	126281	1.14%	0.123%
3	3.640	89	94	98	rBV4	13167	26521	0.24%	0.026%
4	3.764	112	115	133	rBV	535604	856175	7.72%	0.833%
5	3.958	143	148	154	rVB	60902	94742	0.85%	0.092%
6	4.075	164	168	179	rVB	33034	61431	0.55%	0.060%
7	5.016	323	328	334	rVB	21513	32571	0.29%	0.032%
8	6.922	648	652	655	rBV5	8691	14167	0.13%	0.014%
9	7.122	680	686	697	rBV	518236	804154	7.25%	0.782%
10	7.316	712	719	727	rBV	1825285	2841937	25.64%	2.764%
11	7.493	741	749	760	rBV	1768102	2721039	24.55%	2.647%
12	7.975	823	831	839	rBV	1272487	2012401	18.15%	1.957%
13	8.681	944	951	962	rBV	1429361	2252240	20.32%	2.191%
14	9.169	1026	1034	1040	rBV	2142078	3489946	31.48%	3.394%
15	9.216	1040	1042	1050	rVV	79211	118850	1.07%	0.116%
16	9.287	1050	1054	1058	rVB7	8853	15695	0.14%	0.015%
17	9.887	1146	1156	1168	rBV	1727395	2707972	24.43%	2.634%
18	10.410	1236	1245	1257	rBV	2425190	3904263	35.22%	3.797%
19	10.798	1304	1311	1321	rBV	1836853	3034358	27.37%	2.951%
20	10.963	1330	1339	1353	rBV	2332957	4003873	36.12%	3.894%
21	11.551	1434	1439	1447	rBV	7898	16145	0.15%	0.016%
22	12.381	1574	1580	1585	rBV	41647	67194	0.61%	0.065%
23	13.475	1761	1766	1771	rBV2	31328	50347	0.45%	0.049%
24	14.045	1856	1863	1876	rBV	4725232	6197335	55.91%	6.028%
25	14.334	1904	1912	1922	rBV	5027920	7396476	66.72%	7.194%
26	14.628	1955	1962	1971	rVB	2805186	4018129	36.25%	3.908%
27	14.839	1992	1998	2010	rBV	328212	560618	5.06%	0.545%
28	15.063	2033	2036	2043	rVB7	17364	27249	0.25%	0.027%
29	15.628	2125	2132	2143	rBV	6433198	9218947	83.16%	8.966%
30	15.751	2146	2153	2167	rVV	1866032	2486698	22.43%	2.419%
31	15.863	2168	2172	2177	rVB3	31834	42239	0.38%	0.041%
32	17.175	2392	2395	2401	rBV5	7627	15708	0.14%	0.015%
33	17.398	2426	2433	2443	rBV	3412817	4673882	42.16%	4.546%
34	17.498	2443	2450	2462	rBV2	7593617	10119362	91.29%	9.842%
35	18.233	2571	2575	2583	rBV2	67989	99836	0.90%	0.097%
36	19.304	2753	2757	2762	rVB2	74535	97876	0.88%	0.095%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017028.D
Acq On : 09 Sep 2023 00:52
Operator : MA/JU
Sample : 04153-07
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH465

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Title : SVOA CALIBRATION

37	19.374	2765	2769	2773	rVV	68717	93881	0.85%	0.091%
38	19.469	2782	2785	2790	rBV3	59282	68825	0.62%	0.067%
39	19.610	2806	2809	2813	rBV	29345	37857	0.34%	0.037%
40	19.733	2824	2830	2843	rBV	8759249	11085309	100.00%	10.782%
41	21.492	3124	3129	3135	rBV	3271465	4160659	37.53%	4.047%
42	23.857	3524	3531	3548	rVB2	4560369	9170467	82.73%	8.919%
43	24.027	3553	3560	3579	rVB	1849405	3919875	35.36%	3.813%




Sum of corrected areas: 102815623

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017028.D
Acq On : 09 Sep 2023 00:52
Operator : MA/JU
Sample : 04153-07
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH465

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

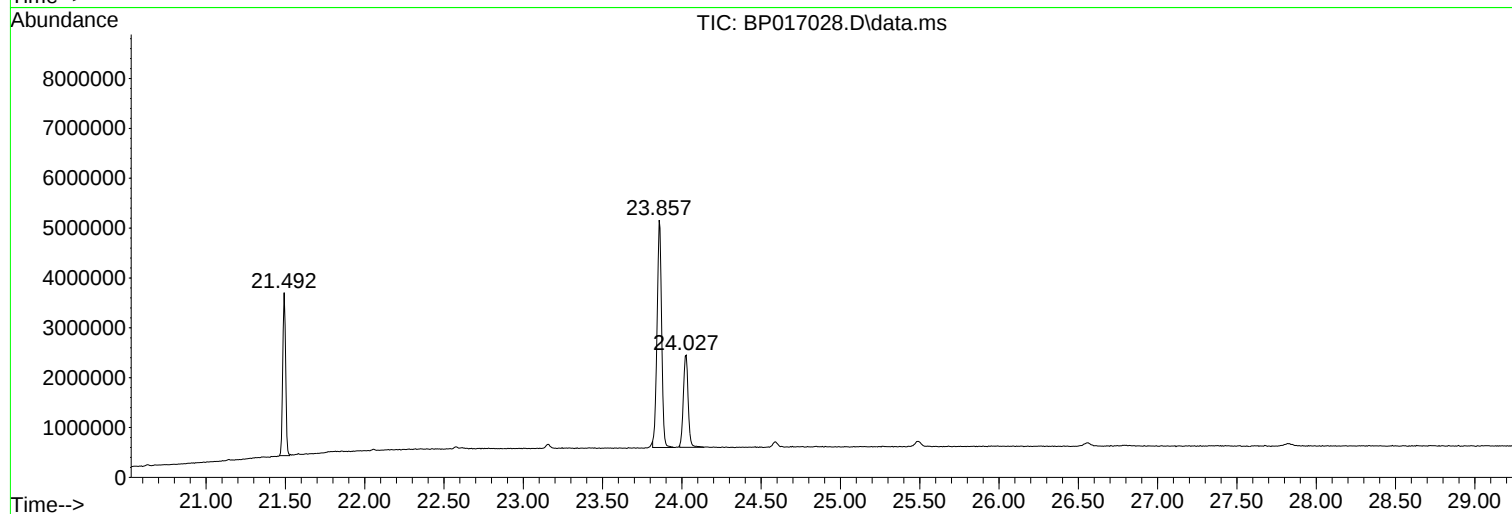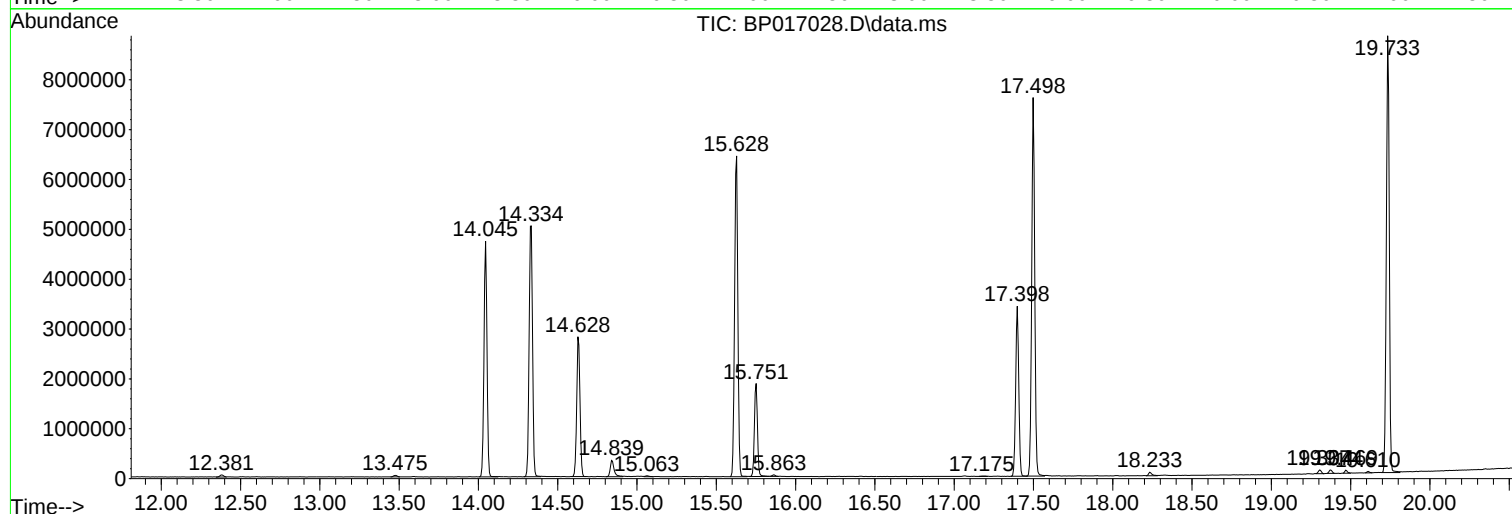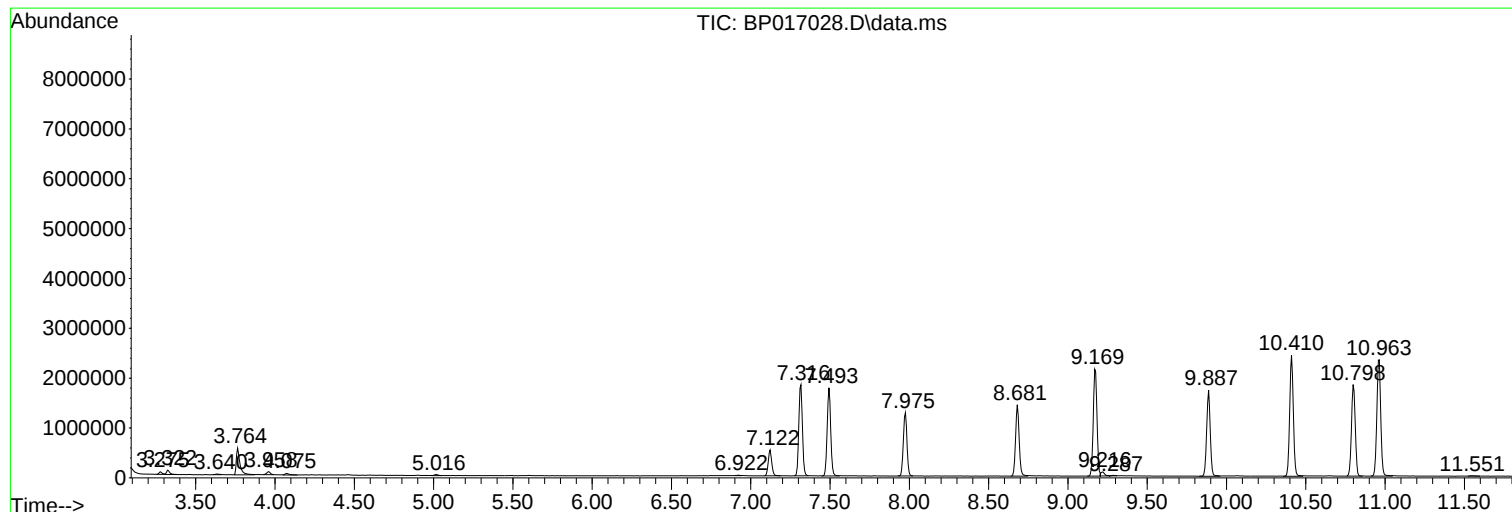

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017028.D
Acq On : 09 Sep 2023 00:52
Operator : MA/JU
Sample : 04153-07
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH465

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017028.D
Acq On : 09 Sep 2023 00:52
Operator : MA/JU
Sample : 04153-07
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH465

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------