

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
 Data File : BP017030.D
 Acq On : 09 Sep 2023 02:00
 Operator : MA/JU
 Sample : 04166-06
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBHH1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017030.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	28	32	37	rBV	131426	195719	1.27%	0.142%
2	3.322	37	40	47	rVB	102136	139031	0.90%	0.101%
3	3.764	112	115	130	rBV	465753	769227	5.01%	0.558%
4	3.958	143	148	157	rVB	63900	106914	0.70%	0.078%
5	4.075	164	168	173	rBV	25561	35886	0.23%	0.026%
6	4.464	230	234	246	rVB4	25117	57982	0.38%	0.042%
7	4.599	252	257	266	rBV	106030	170507	1.11%	0.124%
8	5.016	322	328	333	rBV	22613	34033	0.22%	0.025%
9	5.599	424	427	434	rVB2	10876	16146	0.11%	0.012%
10	6.922	647	652	667	rVB6	18111	51434	0.33%	0.037%
11	7.122	679	686	696	rBV	637445	996660	6.49%	0.723%
12	7.316	709	719	729	rBV	2262545	3599218	23.43%	2.611%
13	7.493	742	749	759	rBV	2223306	3462240	22.54%	2.511%
14	7.581	762	764	774	rVB4	10972	18409	0.12%	0.013%
15	7.975	823	831	843	rBV	1709045	2676673	17.42%	1.941%
16	8.681	943	951	970	rBV	1787838	2857896	18.60%	2.073%
17	9.169	1027	1034	1049	rBV	2716222	4453681	28.99%	3.230%
18	9.387	1067	1071	1075	rVB	12635	17320	0.11%	0.013%
19	9.887	1147	1156	1165	rBV	2243929	3582385	23.32%	2.598%
20	10.069	1181	1187	1194	rVB	7162	16907	0.11%	0.012%
21	10.410	1237	1245	1256	rBV	3227999	5177247	33.70%	3.755%
22	10.798	1300	1311	1324	rBV	2437246	4011418	26.11%	2.909%
23	10.957	1330	1338	1351	rBV	1105120	1890698	12.31%	1.371%
24	11.551	1434	1439	1445	rBV8	9520	21835	0.14%	0.016%
25	11.881	1489	1495	1502	rVB2	20418	33290	0.22%	0.024%
26	12.381	1573	1580	1588	rBV	54488	96804	0.63%	0.070%
27	13.387	1745	1751	1754	rBV3	14028	18392	0.12%	0.013%
28	13.475	1760	1766	1779	rBV	630579	989361	6.44%	0.718%
29	13.592	1779	1786	1792	rVV5	10105	20576	0.13%	0.015%
30	14.045	1856	1863	1872	rBV	6156686	8222181	53.52%	5.964%
31	14.328	1903	1911	1925	rBV	6641361	9678004	62.99%	7.019%
32	14.628	1955	1962	1971	rBV	3664572	5220616	33.98%	3.787%
33	14.839	1992	1998	2015	rBV	520164	838941	5.46%	0.608%
34	15.028	2028	2030	2033	rVB4	13523	16063	0.10%	0.012%
35	15.628	2122	2132	2140	rBV	8892005	12131998	78.97%	8.799%
36	15.751	2146	2153	2166	rBV	3172019	4065358	26.46%	2.949%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
 Data File : BP017030.D
 Acq On : 09 Sep 2023 02:00
 Operator : MA/JU
 Sample : 04166-06
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBHH1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
 Title : SVOA CALIBRATION

37	15.863	2168	2172	2178	rVB3	35643	49937	0.33%	0.036%
38	17.063	2372	2376	2382	rVB7	10480	19162	0.12%	0.014%
39	17.186	2393	2397	2402	rBV3	11281	21968	0.14%	0.016%
40	17.398	2426	2433	2443	rBV	4628976	6311718	41.08%	4.578%
41	17.498	2443	2450	2465	rBV2	9656713	13300294	86.57%	9.647%
42	18.016	2535	2538	2544	rBV3	50871	69736	0.45%	0.051%
43	18.233	2571	2575	2585	rBV	144269	209201	1.36%	0.152%
44	19.122	2723	2726	2728	rBV2	64203	73114	0.48%	0.053%
45	19.151	2728	2731	2739	rVB	390027	448049	2.92%	0.325%
46	19.304	2754	2757	2762	rVB	111635	133549	0.87%	0.097%
47	19.374	2765	2769	2773	rVB	115100	147547	0.96%	0.107%
48	19.469	2782	2785	2790	rBV2	108836	133713	0.87%	0.097%
49	19.610	2806	2809	2814	rBV3	47105	58435	0.38%	0.042%
50	19.733	2824	2830	2836	rBV	11857721	15363483	100.00%	11.143%
51	21.492	3124	3129	3135	rBV	4998868	6160587	40.10%	4.468%
52	23.862	3524	3532	3548	rVB2	6768940	13882414	90.36%	10.069%
53	24.027	3553	3560	3570	rVB	2901382	5799427	37.75%	4.206%




Sum of corrected areas: 137873384

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017030.D
Acq On : 09 Sep 2023 02:00
Operator : MA/JU
Sample : 04166-06
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBHH1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

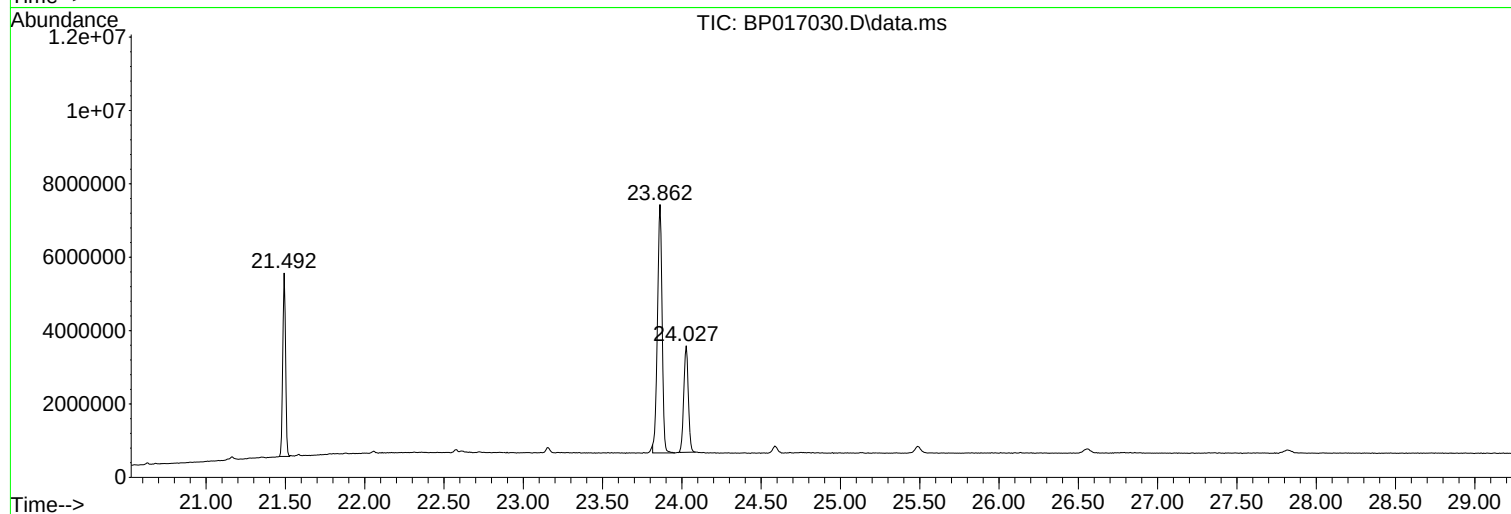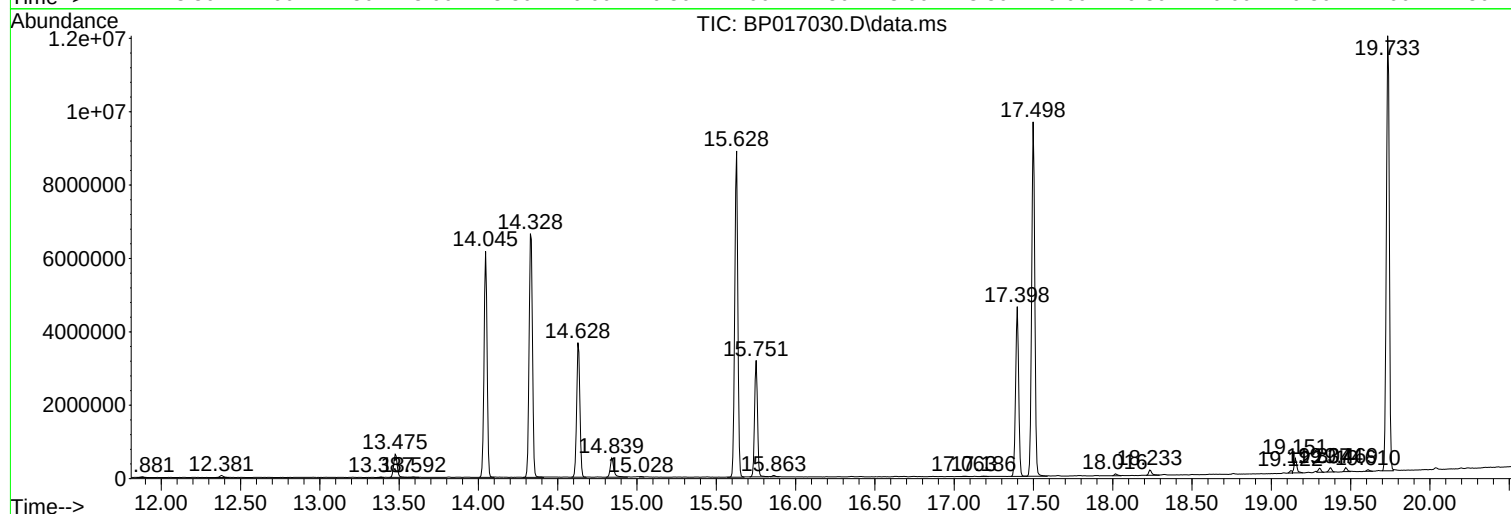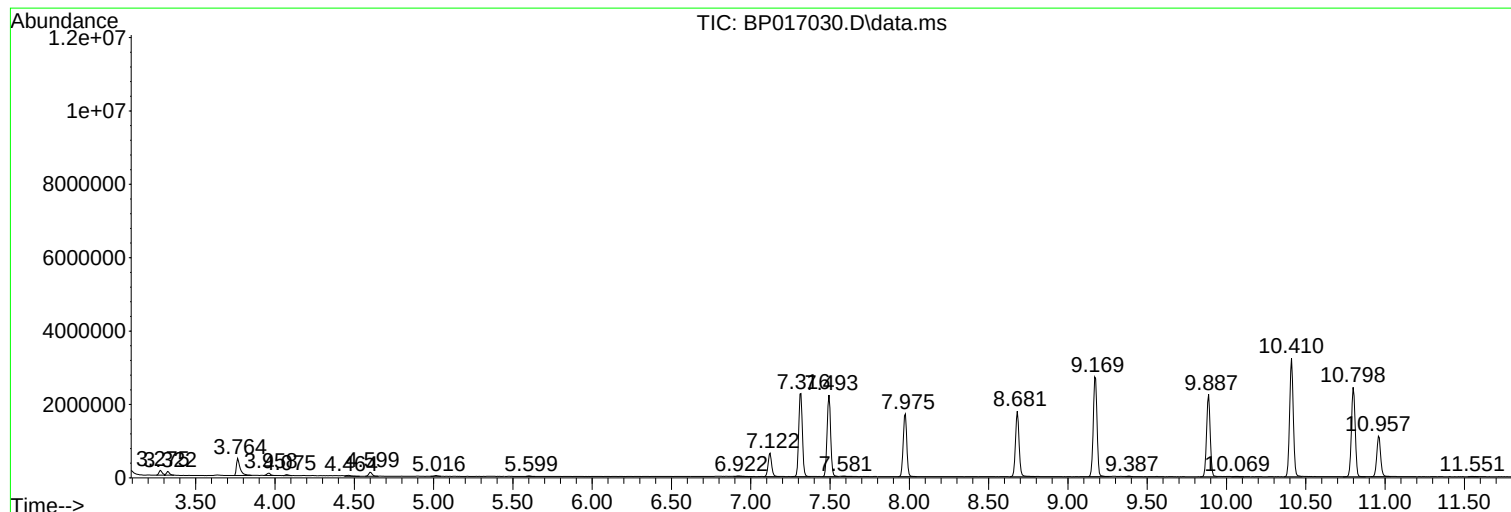

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017030.D
Acq On : 09 Sep 2023 02:00
Operator : MA/JU
Sample : 04166-06
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBHH1










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2,4,7,9-Tetramethyl-5-decyn... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.475	3.79 ng/ul	989361	Acenaphthene-d10	14.628

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2,4,7,9-Tetramethyl-5-decyn-4,7-...	226	C14H26O2	000126-86-3	87		
2	2,4,7,9-Tetramethyl-5-decyn-4,7-...	226	C14H26O2	000126-86-3	74		
3	Pyridine, 2-butyl-, 1-oxide	151	C9H13NO	031396-32-4	53		
4	Diacetamate	193	C10H11NO3	002623-33-8	47		
5	2,4,7,9-Tetramethyl-5-decyn-4,7-...	226	C14H26O2	000126-86-3	47		

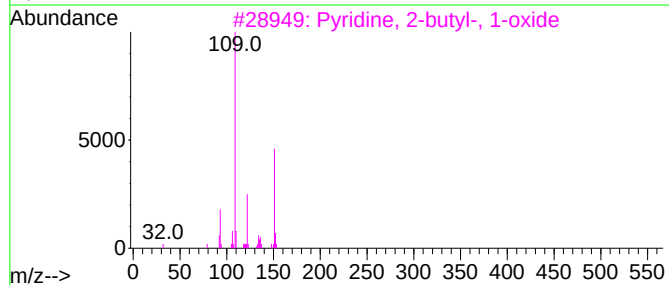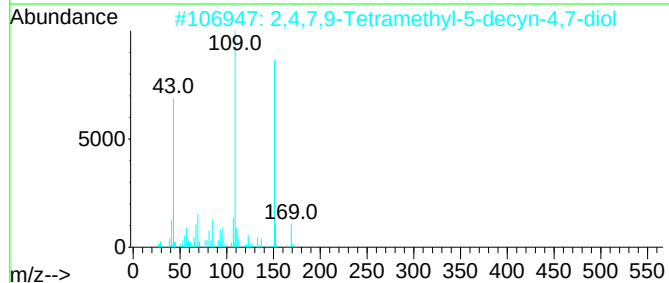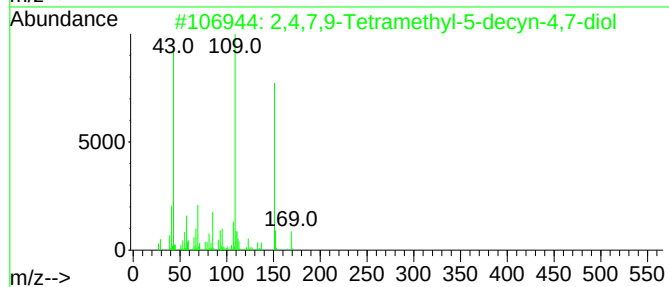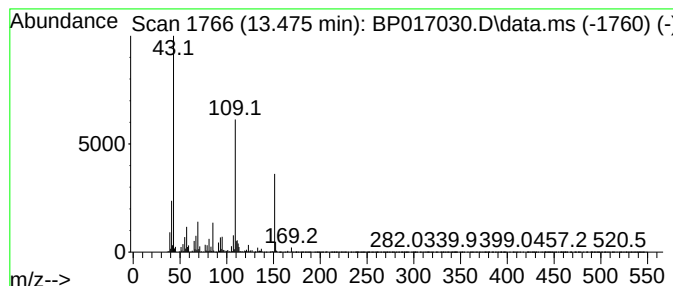

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017030.D
Acq On : 09 Sep 2023 02:00
Operator : MA/JU
Sample : 04166-06
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBHH1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2,4,7,9-Tetrame...	13.475	3.8	ng/u1	989361	3	14.628	5220620	20.0