

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
 Data File : BP017035.D
 Acq On : 09 Sep 2023 04:52
 Operator : MA/JU
 Sample : 04166-14
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBJX8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017035.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.322	36	40	48	rVB	85936	117890	0.96%	0.108%
2	3.764	111	115	133	rBV	589103	973265	7.91%	0.888%
3	3.958	144	148	155	rVB	54183	88006	0.72%	0.080%
4	4.075	164	168	175	rVB2	20793	32619	0.27%	0.030%
5	5.011	324	327	333	rVB	18680	29046	0.24%	0.027%
6	5.605	422	428	434	rVB3	8706	16029	0.13%	0.015%
7	6.922	647	652	663	rVB6	14749	36015	0.29%	0.033%
8	7.122	679	686	698	rBV	550212	884010	7.19%	0.807%
9	7.310	710	718	731	rBV	1798069	2810721	22.85%	2.565%
10	7.493	742	749	762	rBV	1750725	2768754	22.51%	2.526%
11	7.969	823	830	840	rBV	1269415	2035579	16.55%	1.857%
12	8.681	944	951	971	rBV	1500650	2414428	19.63%	2.203%
13	9.099	1018	1022	1027	rBV	13450	19765	0.16%	0.018%
14	9.169	1027	1034	1045	rBV	2156703	3472035	28.23%	3.168%
15	9.387	1067	1071	1076	rVB5	7267	12319	0.10%	0.011%
16	9.887	1147	1156	1171	rBV	1698472	2807405	22.83%	2.561%
17	10.410	1237	1245	1262	rBV	2439245	4039473	32.84%	3.686%
18	10.799	1302	1311	1320	rBV	1890059	3101423	25.22%	2.830%
19	10.957	1329	1338	1356	rBV	2312605	3818919	31.05%	3.484%
20	11.551	1434	1439	1446	rBV8	8317	17572	0.14%	0.016%
21	12.381	1573	1580	1587	rBV	42427	72017	0.59%	0.066%
22	13.475	1759	1766	1772	rBV	47495	78908	0.64%	0.072%
23	14.045	1856	1863	1875	rBV	4653185	6490817	52.77%	5.922%
24	14.328	1903	1911	1923	rBV	5373644	7664050	62.31%	6.993%
25	14.628	1955	1962	1970	rBV	2935431	4114192	33.45%	3.754%
26	14.839	1992	1998	2013	rBV	473656	781913	6.36%	0.713%
27	15.069	2033	2037	2041	rVB7	8175	13121	0.11%	0.012%
28	15.363	2083	2087	2093	rVB4	11708	19419	0.16%	0.018%
29	15.628	2124	2132	2139	rBV	6676675	9618902	78.21%	8.776%
30	15.751	2147	2153	2166	rBV	2380476	3229616	26.26%	2.947%
31	15.863	2168	2172	2178	rVB2	31564	48388	0.39%	0.044%
32	17.063	2372	2376	2381	rVB8	10229	19365	0.16%	0.018%
33	17.398	2426	2433	2443	rBV	3474425	4936250	40.13%	4.504%
34	17.498	2443	2450	2469	rBV	7813646	10860051	88.30%	9.909%
35	18.022	2537	2539	2544	rVB6	12135	12734	0.10%	0.012%
36	18.233	2571	2575	2583	rBV	109605	154973	1.26%	0.141%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017035.D
Acq On : 09 Sep 2023 04:52
Operator : MA/JU
Sample : 04166-14
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJX8

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Title : SVOA CALIBRATION

37	19.304	2753	2757	2761	rBV2	88879	117471	0.96%	0.107%
38	19.375	2765	2769	2774	rVB	84546	121182	0.99%	0.111%
39	19.469	2782	2785	2790	rBV2	69655	85188	0.69%	0.078%
40	19.610	2806	2809	2813	rBV3	40573	53551	0.44%	0.049%
41	19.733	2824	2830	2841	rBV	9663545	12299144	100.00%	11.222%
42	21.492	3124	3129	3135	rBV	3715915	4651195	37.82%	4.244%
43	23.863	3524	3532	3542	rVB2	4942279	10347267	84.13%	9.441%
44	24.021	3553	3559	3574	rVB	2054026	4315323	35.09%	3.937%




Sum of corrected areas: 109600310

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017035.D
Acq On : 09 Sep 2023 04:52
Operator : MA/JU
Sample : 04166-14
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJX8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

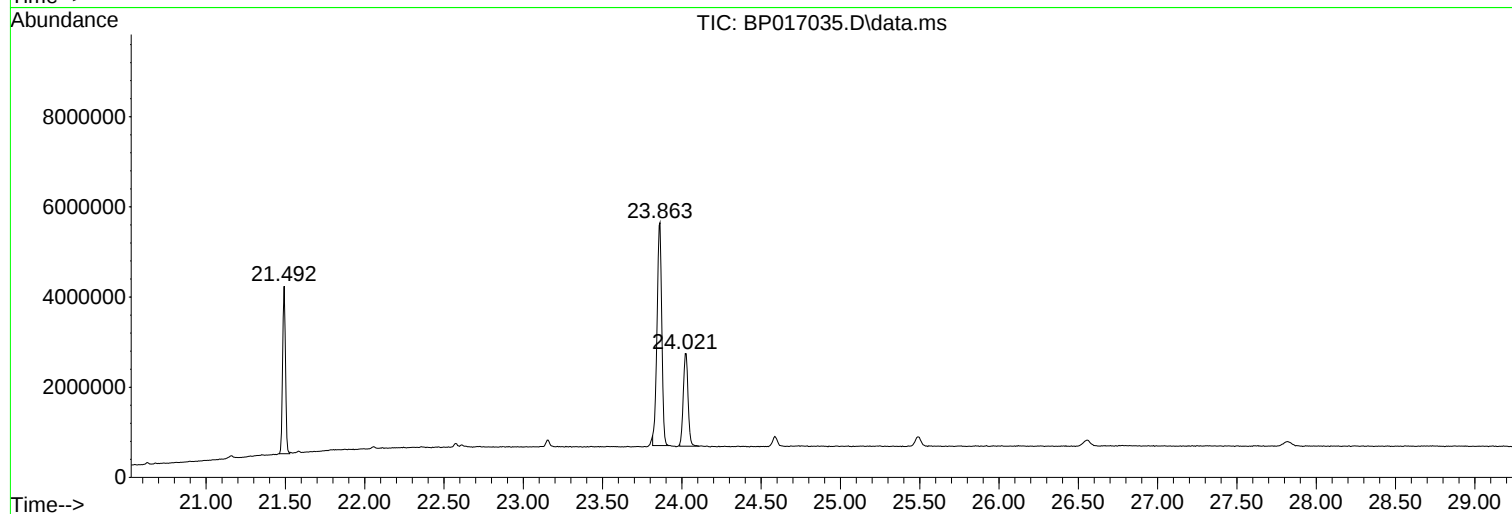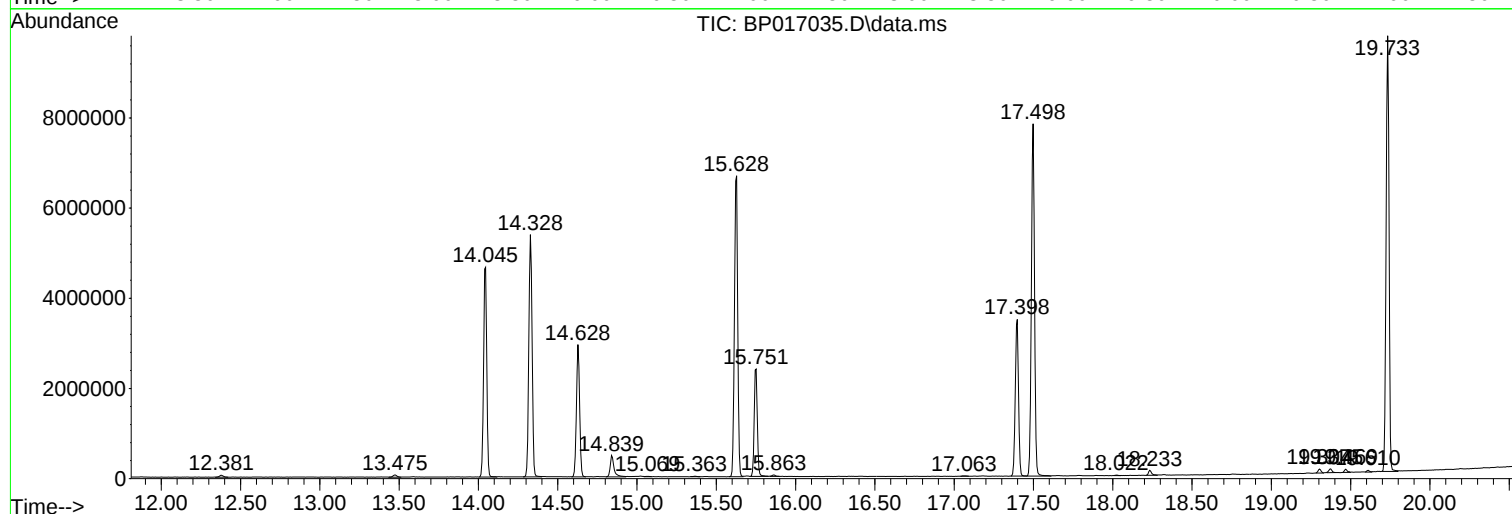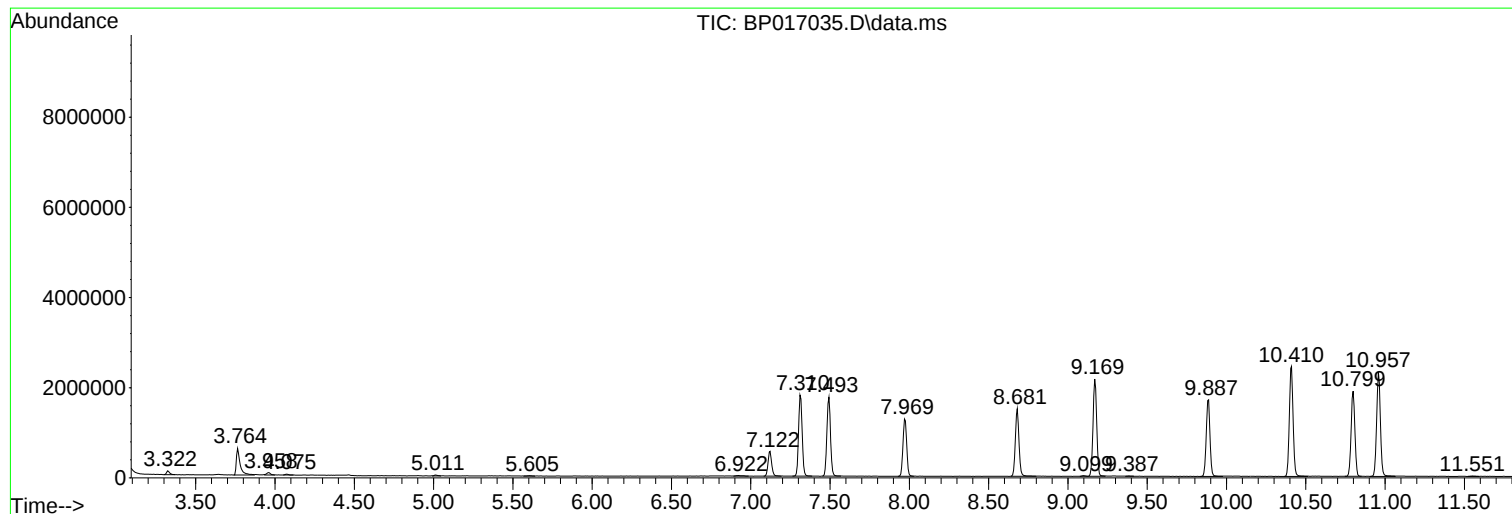

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017035.D
Acq On : 09 Sep 2023 04:52
Operator : MA/JU
Sample : 04166-14
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJX8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017035.D
Acq On : 09 Sep 2023 04:52
Operator : MA/JU
Sample : 04166-14
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJX8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc