

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
 Data File : BP017036.D
 Acq On : 09 Sep 2023 05:26
 Operator : MA/JU
 Sample : 04166-15
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBJJ2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017036.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.323	36	40	44	rBV	87877	114049	0.85%	0.093%
2	3.358	44	46	55	rVB2	25760	39731	0.30%	0.032%
3	3.634	89	93	100	rBV4	12845	22900	0.17%	0.019%
4	3.764	111	115	129	rBV	485983	795905	5.92%	0.650%
5	3.958	143	148	153	rVB	53533	84490	0.63%	0.069%
6	4.075	164	168	173	rVB2	23756	32680	0.24%	0.027%
7	4.470	231	235	239	rVB6	12709	22486	0.17%	0.018%
8	4.599	253	257	264	rVB4	18654	29980	0.22%	0.024%
9	5.017	323	328	332	rBV	19665	28664	0.21%	0.023%
10	5.599	423	427	431	rBV2	11940	16612	0.12%	0.014%
11	6.917	647	651	654	rBV2	10575	16764	0.12%	0.014%
12	7.122	679	686	696	rBV	567379	898684	6.69%	0.734%
13	7.311	710	718	730	rBV	1817857	2811026	20.92%	2.295%
14	7.493	741	749	759	rBV	1792441	2793817	20.79%	2.281%
15	7.575	759	763	772	rVB2	27329	54586	0.41%	0.045%
16	7.969	823	830	844	rBV	1578103	2465853	18.35%	2.013%
17	8.681	943	951	962	rBV	1475542	2389805	17.79%	1.951%
18	9.169	1026	1034	1044	rBV	2163984	3459602	25.75%	2.824%
19	9.381	1065	1070	1079	rVB	87338	140913	1.05%	0.115%
20	9.881	1148	1155	1172	rBV	1660962	2769757	20.62%	2.261%
21	10.058	1182	1185	1192	rVB9	8091	16368	0.12%	0.013%
22	10.410	1237	1245	1259	rBV	2428052	4044351	30.10%	3.302%
23	10.799	1299	1311	1323	rBV	2303051	3720735	27.69%	3.037%
24	10.957	1331	1338	1352	rBV	1940592	3215109	23.93%	2.625%
25	11.081	1354	1359	1369	rVB	49186	98156	0.73%	0.080%
26	11.334	1397	1402	1410	rBV6	24652	42193	0.31%	0.034%
27	11.546	1434	1438	1443	rBV8	8852	18032	0.13%	0.015%
28	11.616	1445	1450	1457	rVB5	23906	44244	0.33%	0.036%
29	11.875	1489	1494	1501	rVB	70931	109597	0.82%	0.089%
30	11.946	1501	1506	1509	rBV7	11234	18379	0.14%	0.015%
31	12.199	1543	1549	1551	rBV2	30613	51837	0.39%	0.042%
32	12.375	1575	1579	1587	rVB	45930	75192	0.56%	0.061%
33	12.516	1598	1603	1608	rVB9	14925	23110	0.17%	0.019%
34	12.587	1608	1615	1616	rVV6	13930	21211	0.16%	0.017%
35	12.616	1616	1620	1626	rVB5	22794	39140	0.29%	0.032%
36	12.863	1656	1662	1668	rBV9	10929	24314	0.18%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
 Data File : BP017036.D
 Acq On : 09 Sep 2023 05:26
 Operator : MA/JU
 Sample : 04166-15
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBJJ2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
 Title : SVOA CALIBRATION

37	13.387	1746	1751	1758	rBV6	18333	33582	0.25%	0.027%
38	13.475	1759	1766	1778	rBV	792746	1220401	9.08%	0.996%
39	13.622	1788	1791	1798	rVB7	11850	19245	0.14%	0.016%
40	13.716	1804	1807	1812	rBV2	11732	17195	0.13%	0.014%
41	13.810	1819	1823	1829	rBV6	13307	20879	0.16%	0.017%
42	13.869	1829	1833	1838	rVB3	18946	28539	0.21%	0.023%
43	13.946	1838	1846	1849	rBV5	20759	32755	0.24%	0.027%
44	14.046	1856	1863	1875	rBV	5230866	6921034	51.51%	5.650%
45	14.328	1904	1911	1924	rBV2	5412023	7727062	57.51%	6.308%
46	14.481	1935	1937	1944	rVB3	10356	17141	0.13%	0.014%
47	14.575	1946	1953	1957	rBV	155935	241448	1.80%	0.197%
48	14.628	1957	1962	1969	rVB	3392874	4876121	36.29%	3.981%
49	14.763	1979	1985	1990	rBV5	23614	48494	0.36%	0.040%
50	14.840	1993	1998	2012	rBV	559769	883489	6.58%	0.721%
51	15.057	2033	2035	2043	rVB9	14966	22677	0.17%	0.019%
52	15.445	2097	2101	2105	rVB3	13909	22754	0.17%	0.019%
53	15.622	2124	2131	2138	rBV	7051220	10086004	75.07%	8.234%
54	15.687	2138	2142	2147	rVV	111179	165028	1.23%	0.135%
55	15.751	2147	2153	2167	rVV	2671254	3563441	26.52%	2.909%
56	15.857	2168	2171	2175	rVV2	33291	54827	0.41%	0.045%
57	15.893	2175	2177	2183	rVB2	22449	34793	0.26%	0.028%
58	16.157	2216	2222	2227	rBV	69273	106183	0.79%	0.087%
59	16.257	2235	2239	2248	rVB3	24428	45922	0.34%	0.037%
60	16.351	2253	2255	2261	rVB6	9996	14972	0.11%	0.012%
61	16.698	2307	2314	2320	rBV2	139646	209607	1.56%	0.171%
62	16.898	2345	2348	2350	rBV4	15221	15704	0.12%	0.013%
63	16.928	2350	2353	2360	rVB4	19475	28423	0.21%	0.023%
64	17.128	2383	2387	2393	rBV	127557	163558	1.22%	0.134%
65	17.187	2393	2397	2403	rBV5	11746	22667	0.17%	0.019%
66	17.240	2403	2406	2409	rBV3	15421	20816	0.15%	0.017%
67	17.398	2426	2433	2443	rBV	4216754	5876863	43.74%	4.798%
68	17.498	2443	2450	2464	rVV	8453070	11668145	86.85%	9.525%
69	18.022	2534	2539	2544	rBV4	56007	86082	0.64%	0.070%
70	18.234	2571	2575	2583	rBV	225513	335488	2.50%	0.274%
71	18.634	2639	2643	2653	rBV	74918	118552	0.88%	0.097%
72	18.745	2658	2662	2671	rBV7	33386	73310	0.55%	0.060%
73	19.122	2723	2726	2728	rVB3	38103	44582	0.33%	0.036%
74	19.151	2728	2731	2736	rVB	187677	201281	1.50%	0.164%
75	19.304	2754	2757	2762	rVB2	106762	119674	0.89%	0.098%
76	19.369	2765	2768	2775	rVB	99905	139988	1.04%	0.114%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017036.D
Acq On : 09 Sep 2023 05:26
Operator : MA/JU
Sample : 04166-15
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJJ2

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Title : SVOA CALIBRATION

77	19.469	2782	2785	2794	rBV	123547	171409	1.28%	0.140%
78	19.733	2824	2830	2836	rBV	10410105	13435474	100.00%	10.968%
79	21.163	3070	3073	3079	rVB3	164269	224038	1.67%	0.183%
80	21.492	3124	3129	3138	rBV	4482740	5582765	41.55%	4.557%
81	22.569	3309	3312	3317	rVB3	220015	290387	2.16%	0.237%
82	23.857	3524	3531	3541	rVB2	5825466	11593503	86.29%	9.464%
83	24.027	3552	3560	3568	rBV	2561884	5319873	39.60%	4.343%




Sum of corrected areas: 122496447

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017036.D
Acq On : 09 Sep 2023 05:26
Operator : MA/JU
Sample : 04166-15
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJJ2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

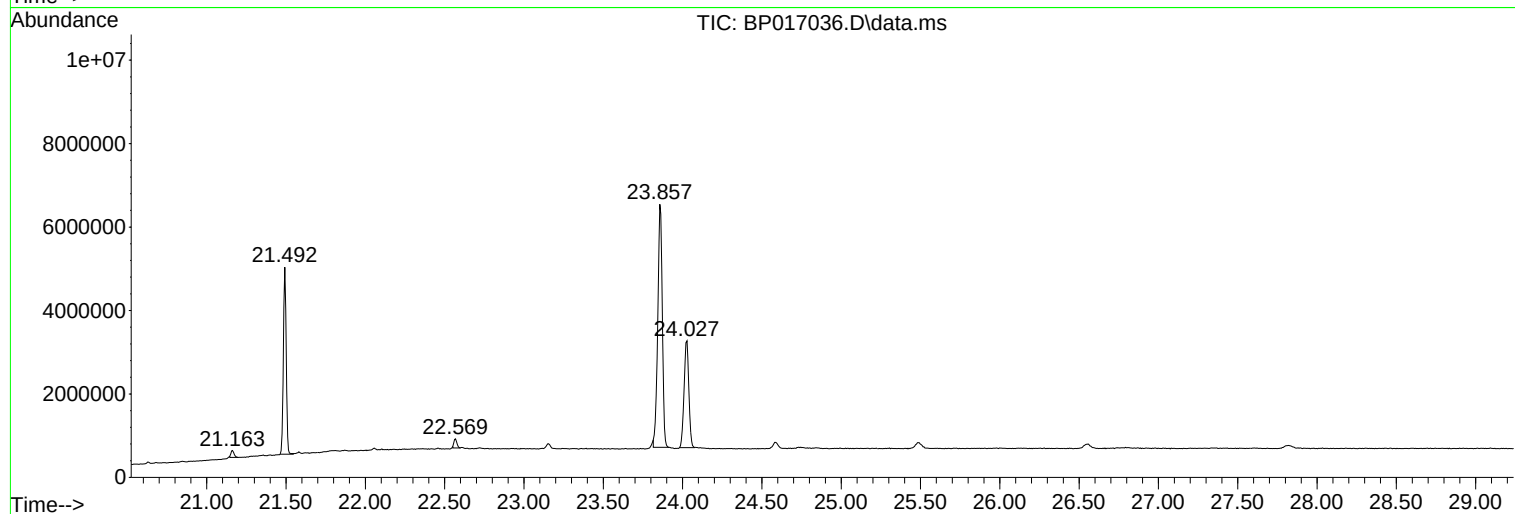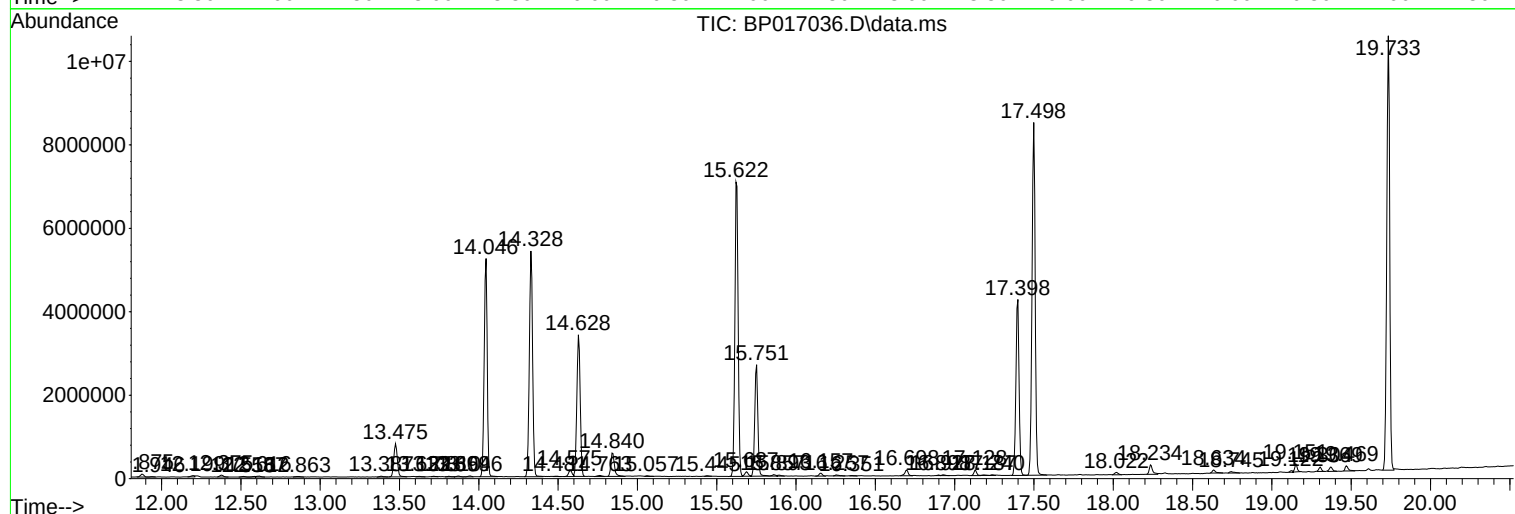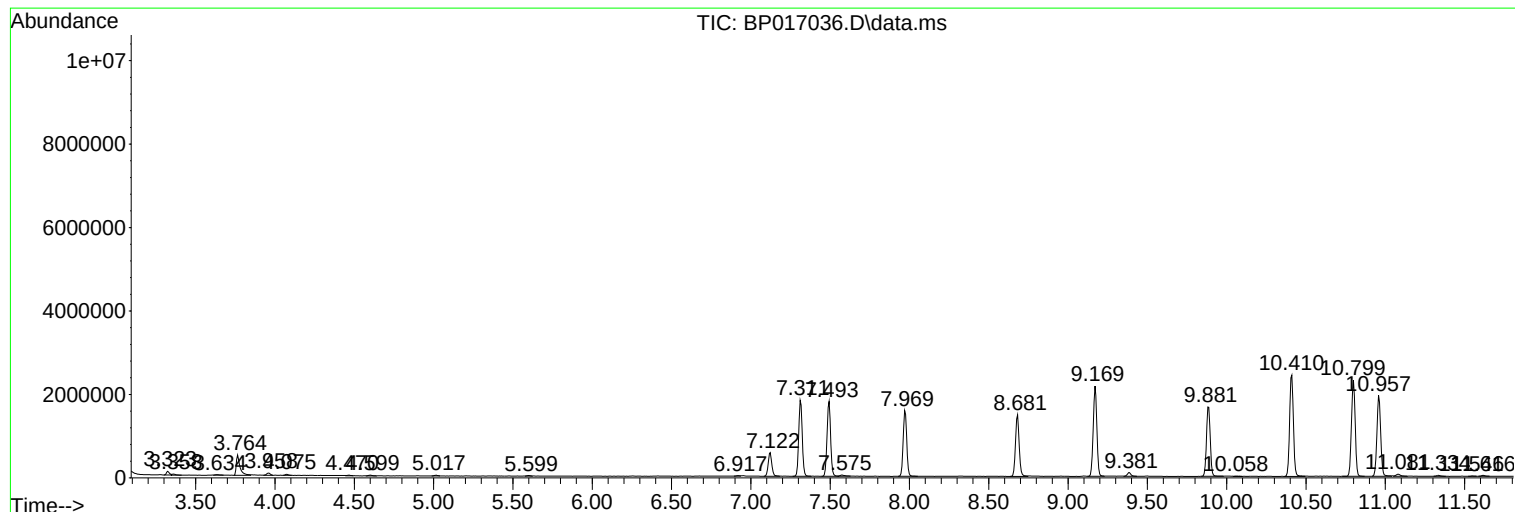

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017036.D
Acq On : 09 Sep 2023 05:26
Operator : MA/JU
Sample : 04166-15
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJJ2










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2,4,7,9-Tetramethyl-5-decyn... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.475	5.01 ng/ul	1220400	Acenaphthene-d10	14.628

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2,4,7,9-Tetramethyl-5-decyn-4,7-...	226	C14H26O2	000126-86-3	90		
2	2,4,7,9-Tetramethyl-5-decyn-4,7-...	226	C14H26O2	000126-86-3	83		
3	Pyridine, 2-butyl-, 1-oxide	151	C9H13NO	031396-32-4	59		
4	Metacetamol	151	C8H9NO2	000621-42-1	53		
5	Metacetamol	151	C8H9NO2	000621-42-1	53		

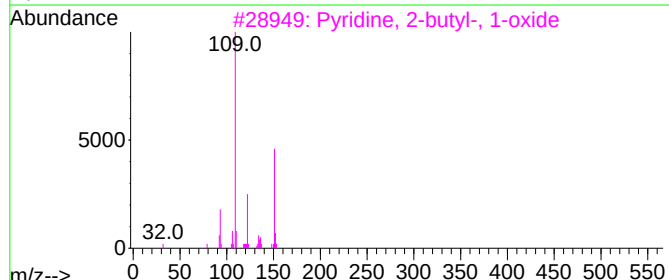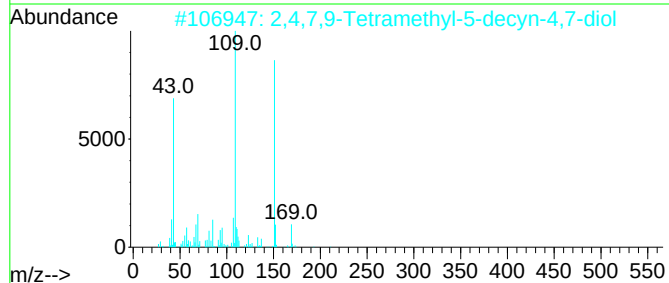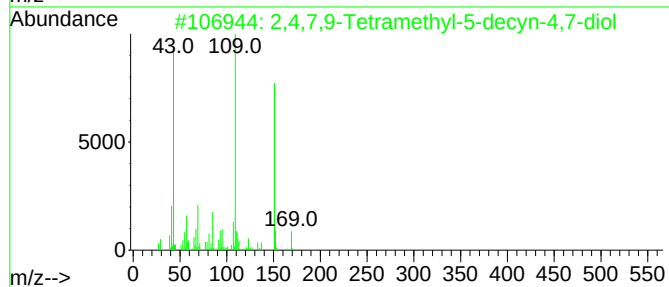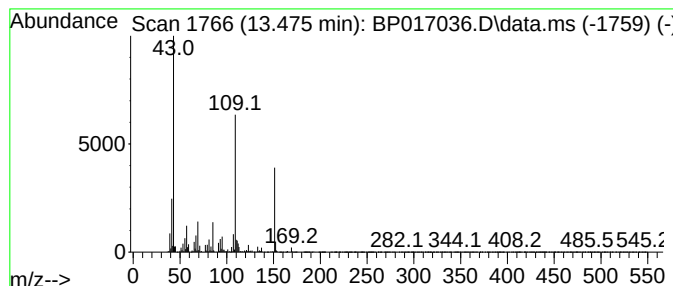

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017036.D
Acq On : 09 Sep 2023 05:26
Operator : MA/JU
Sample : 04166-15
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJJ2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2,4,7,9-Tetrame...	13.475	5.0	ng/u1	1220400	3	14.628	4876120	20.0