

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
 Data File : BP017046.D
 Acq On : 09 Sep 2023 11:42
 Operator : MA/JU
 Sample : 04166-13
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBHH3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017046.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.276	29	32	36	rBV4	35705	44278	0.39%	0.043%
2	3.323	36	40	45	rVV	97729	116078	1.01%	0.114%
3	3.764	112	115	133	rBV	299878	489412	4.27%	0.480%
4	3.958	143	148	154	rVB	52558	81276	0.71%	0.080%
5	4.076	163	168	174	rVB2	20114	29367	0.26%	0.029%
6	5.011	324	327	332	rVB2	16853	22796	0.20%	0.022%
7	6.917	647	651	654	rBV4	8167	11619	0.10%	0.011%
8	7.117	677	685	697	rBV	466470	739646	6.45%	0.725%
9	7.311	711	718	729	rBV	1768510	2682142	23.39%	2.629%
10	7.493	741	749	758	rBV	1579823	2548594	22.23%	2.498%
11	7.969	823	830	842	rBV	1272574	1986140	17.32%	1.947%
12	8.675	941	950	962	rBV	1284564	2061799	17.98%	2.021%
13	9.169	1025	1034	1046	rBV	2035371	3286467	28.66%	3.221%
14	9.287	1050	1054	1059	rVB7	10387	16089	0.14%	0.016%
15	9.381	1065	1070	1076	rVB3	11093	19198	0.17%	0.019%
16	9.881	1147	1155	1164	rBV	1574491	2547755	22.22%	2.497%
17	10.405	1237	1244	1259	rBV	2213304	3603997	31.43%	3.532%
18	10.799	1301	1311	1319	rBV	1777204	2928371	25.54%	2.870%
19	10.958	1330	1338	1358	rBV	1907827	3189298	27.81%	3.126%
20	11.875	1489	1494	1502	rVB	33136	53559	0.47%	0.052%
21	12.381	1573	1580	1585	rBV	40569	67215	0.59%	0.066%
22	13.469	1759	1765	1771	rBV	30776	51167	0.45%	0.050%
23	13.587	1781	1785	1791	rBV6	7514	14235	0.12%	0.014%
24	13.869	1828	1833	1838	rVB	19333	28403	0.25%	0.028%
25	14.040	1856	1862	1875	rBV	4614854	6242136	54.44%	6.118%
26	14.328	1903	1911	1930	rBV2	5052398	7157128	62.42%	7.015%
27	14.628	1954	1962	1970	rBV	2601552	3716559	32.41%	3.643%
28	14.840	1991	1998	2008	rBV	345334	578959	5.05%	0.567%
29	15.428	2095	2098	2103	rVB6	7630	13014	0.11%	0.013%
30	15.622	2124	2131	2140	rBV	6634036	9137805	79.69%	8.956%
31	15.746	2146	2152	2167	rBV	2144519	2851774	24.87%	2.795%
32	15.863	2168	2172	2181	rVB	31031	52856	0.46%	0.052%
33	16.610	2295	2299	2304	rBV5	15784	25537	0.22%	0.025%
34	17.063	2372	2376	2382	rVB7	9291	15450	0.13%	0.015%
35	17.187	2392	2397	2399	rBV3	8164	13709	0.12%	0.013%
36	17.392	2426	2432	2442	rBV	3191171	4446127	38.77%	4.358%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
 Data File : BP017046.D
 Acq On : 09 Sep 2023 11:42
 Operator : MA/JU
 Sample : 04166-13
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBHH3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
 Title : SVOA CALIBRATION

37	17.498	2443	2450	2471	rVV	7420945	10410626	90.79%	10.204%
38	18.234	2570	2575	2583	rBV2	111304	167528	1.46%	0.164%
39	19.304	2753	2757	2761	rBV2	78948	100659	0.88%	0.099%
40	19.369	2764	2768	2774	rVB	82143	115002	1.00%	0.113%
41	19.469	2781	2785	2792	rBV2	96479	138501	1.21%	0.136%
42	19.604	2806	2808	2813	rVB3	38686	41573	0.36%	0.041%
43	19.734	2824	2830	2836	rBV	8985580	11466961	100.00%	11.239%
44	20.192	2905	2908	2912	rBV2	68379	77109	0.67%	0.076%
45	20.681	2988	2991	2997	rVB2	93461	102236	0.89%	0.100%
46	21.133	3065	3068	3072	rBV	118907	157496	1.37%	0.154%
47	21.492	3124	3129	3136	rVB	3089423	4074916	35.54%	3.994%
48	23.857	3521	3531	3549	rVB	4928756	10420772	90.88%	10.214%
49	24.022	3552	3559	3568	rVB	1867893	3881155	33.85%	3.804%




Sum of corrected areas: 102024489

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017046.D
Acq On : 09 Sep 2023 11:42
Operator : MA/JU
Sample : 04166-13
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBHH3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

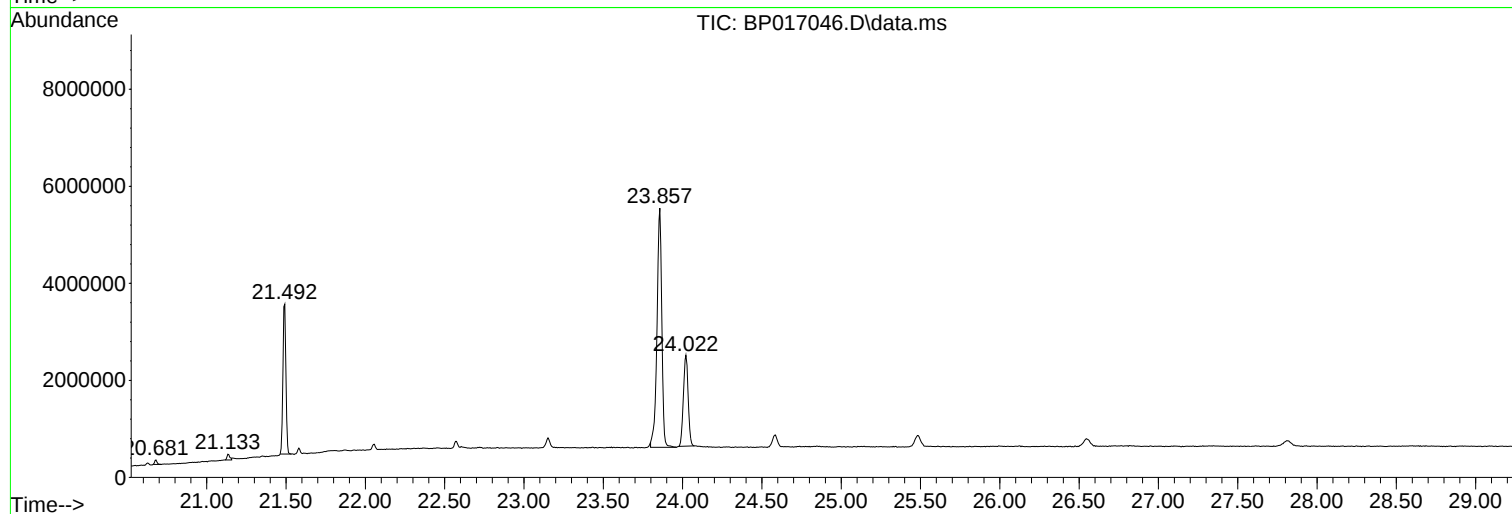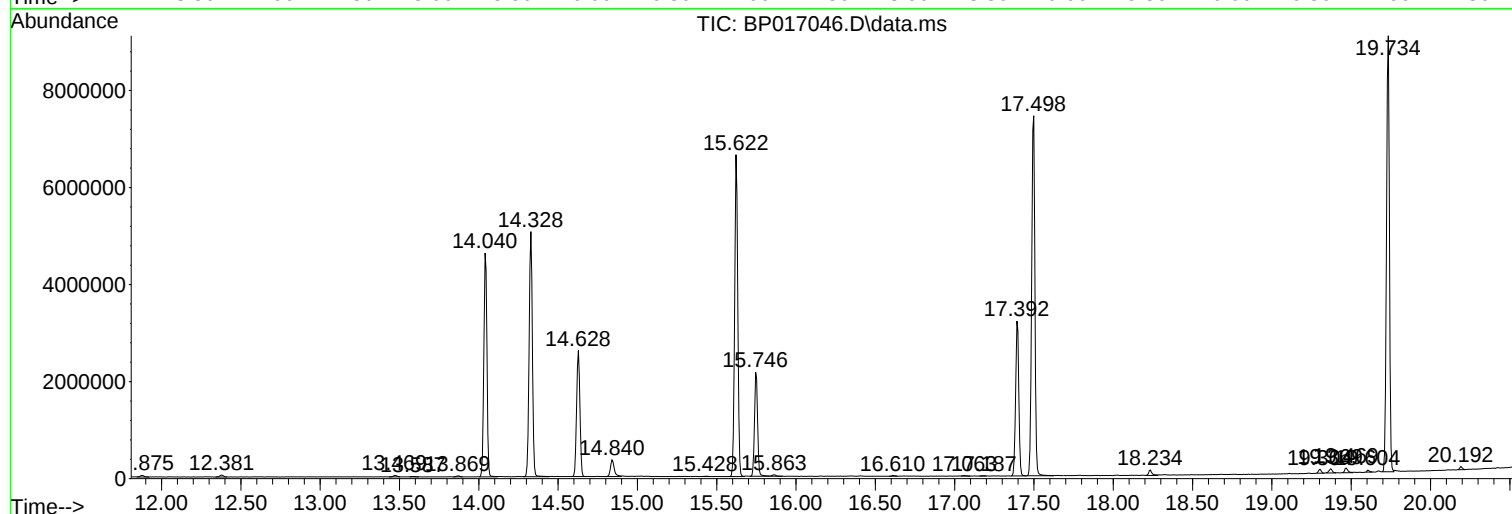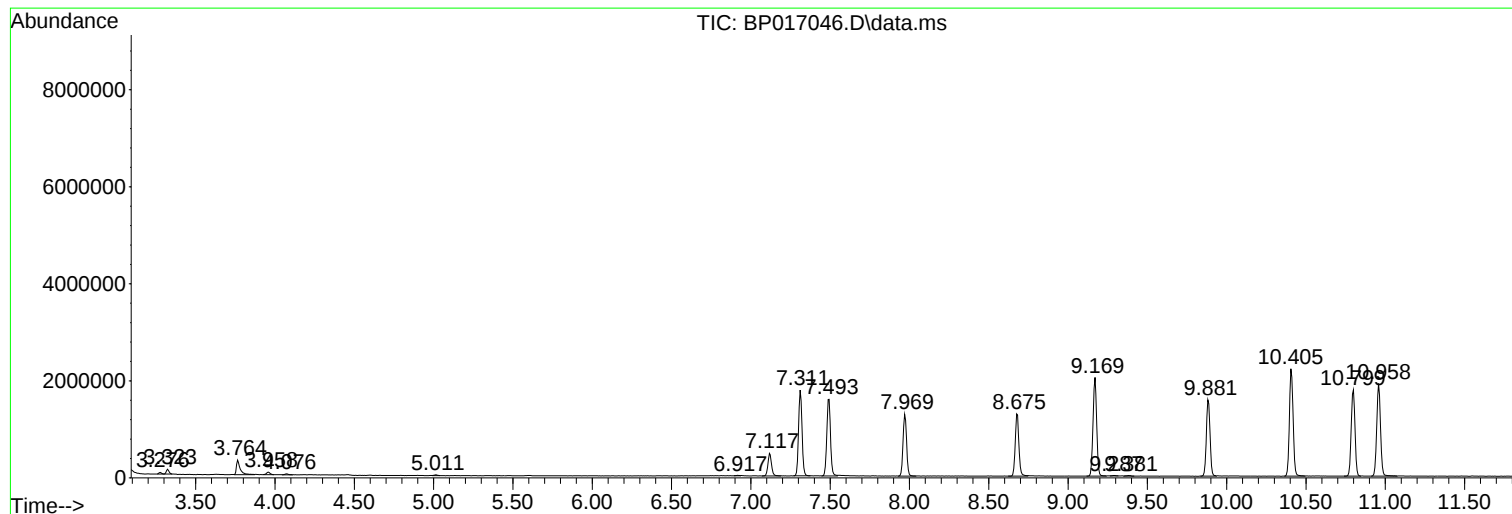

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017046.D
Acq On : 09 Sep 2023 11:42
Operator : MA/JU
Sample : 04166-13
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBHH3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017046.D
Acq On : 09 Sep 2023 11:42
Operator : MA/JU
Sample : 04166-13
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBHH3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc