

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
 Data File : BP017047.D
 Acq On : 09 Sep 2023 12:17
 Operator : MA/JU
 Sample : 04227-07
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH9X8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017047.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	27	32	38	rBV	809576	1202109	2.47%	0.737%
2	3.322	38	40	52	rVB2	146546	240705	0.50%	0.148%
3	3.764	111	115	136	rBV	625277	986735	2.03%	0.605%
4	3.958	144	148	156	rVB	51198	77321	0.16%	0.047%
5	4.599	250	257	259	rBV	33169493	48610479	100.00%	29.807%
6	7.116	678	685	699	rBV	413997	654880	1.35%	0.402%
7	7.310	711	718	730	rVB	1722724	2638806	5.43%	1.618%
8	7.493	741	749	762	rBV	1511417	2425655	4.99%	1.487%
9	7.969	822	830	841	rBV	1345034	2088395	4.30%	1.281%
10	8.675	943	950	960	rBV	1207471	1970893	4.05%	1.209%
11	9.169	1026	1034	1048	rBV	2048997	3294226	6.78%	2.020%
12	9.881	1148	1155	1168	rBV	1566139	2542699	5.23%	1.559%
13	10.404	1237	1244	1258	rBV	2265775	3735190	7.68%	2.290%
14	10.799	1302	1311	1320	rBV	1899444	3151530	6.48%	1.932%
15	10.957	1328	1338	1353	rBV	2201915	3592185	7.39%	2.203%
16	11.875	1489	1494	1500	rVB	52698	78480	0.16%	0.048%
17	12.381	1572	1580	1586	rBV2	41733	70668	0.15%	0.043%
18	13.475	1760	1766	1771	rVB	39473	63921	0.13%	0.039%
19	14.040	1856	1862	1875	rBV	4913370	6854070	14.10%	4.203%
20	14.328	1903	1911	1926	rBV	5524256	7730288	15.90%	4.740%
21	14.628	1955	1962	1970	rBV	2891190	4138443	8.51%	2.538%
22	14.839	1991	1998	2008	rBV	364336	641954	1.32%	0.394%
23	15.622	2124	2131	2138	rBV	7332428	10076497	20.73%	6.179%
24	15.686	2138	2142	2146	rVV	120832	171445	0.35%	0.105%
25	15.745	2146	2152	2167	rVB	2502248	3359561	6.91%	2.060%
26	17.392	2426	2432	2443	rBV	3573625	4957962	10.20%	3.040%
27	17.498	2443	2450	2461	rBV	8347081	11484098	23.62%	7.042%
28	18.233	2571	2575	2583	rBV	192978	282521	0.58%	0.173%
29	19.304	2753	2757	2761	rBV2	91295	117580	0.24%	0.072%
30	19.369	2765	2768	2772	rVB	93206	117764	0.24%	0.072%
31	19.469	2781	2785	2792	rBV	125712	170751	0.35%	0.105%
32	19.610	2806	2809	2812	rBV	47157	49275	0.10%	0.030%
33	19.733	2824	2830	2836	rBV	10409764	13199244	27.15%	8.093%
34	20.627	2980	2982	2986	rVB4	52459	53798	0.11%	0.033%
35	21.163	3070	3073	3081	rVB4	128078	195204	0.40%	0.120%
36	21.492	3124	3129	3135	rBV	3869456	4846551	9.97%	2.972%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017047.D
Acq On : 09 Sep 2023 12:17
Operator : MA/JU
Sample : 04227-07
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH9X8

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Title : SVOA CALIBRATION

37	23.857	3521	3531	3548	rVB2	5899303	12447005	25.61%	7.632%
38	24.021	3552	3559	3572	rVB	2314227	4766293	9.81%	2.923%




Sum of corrected areas: 163085181

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017047.D
Acq On : 09 Sep 2023 12:17
Operator : MA/JU
Sample : 04227-07
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH9X8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

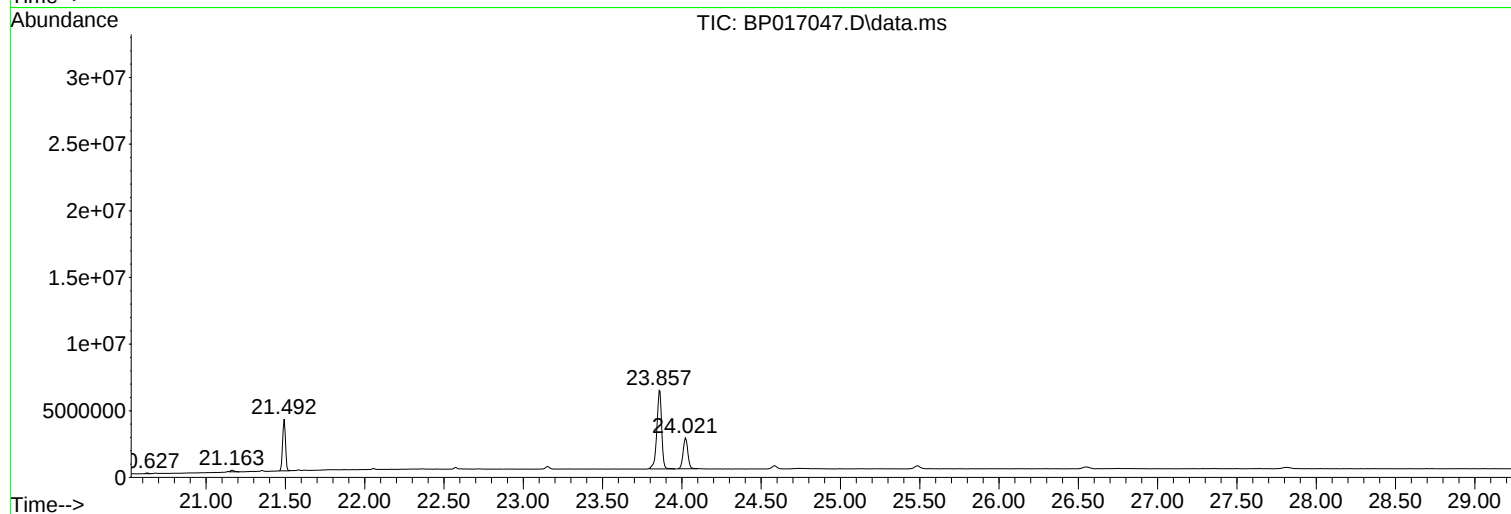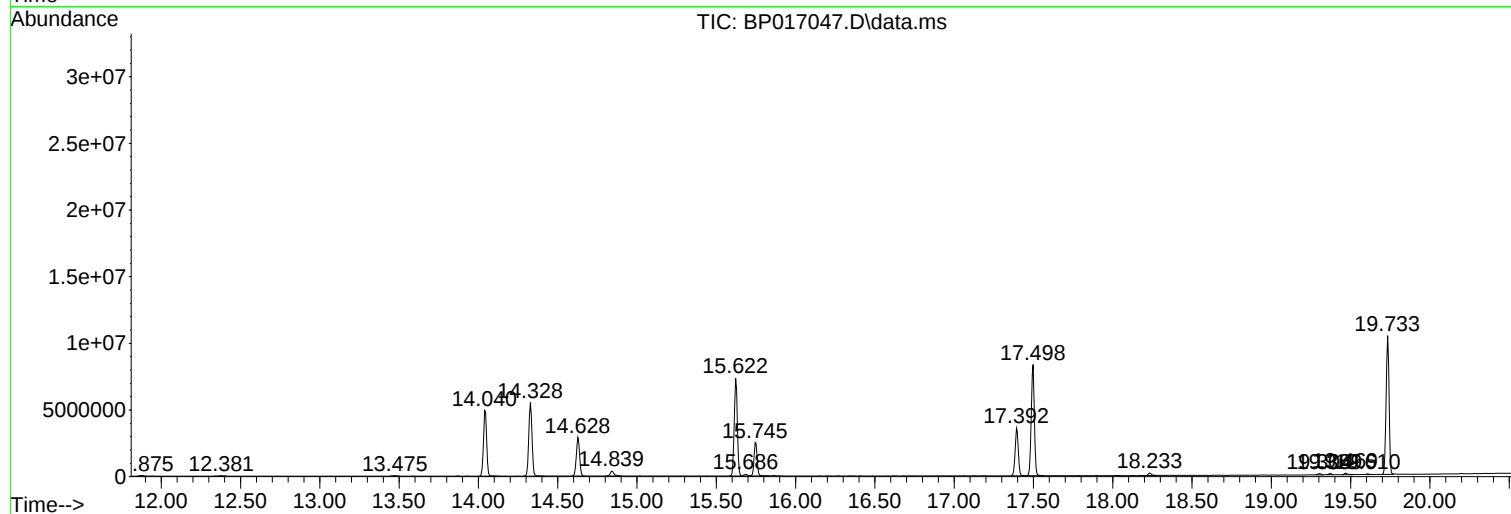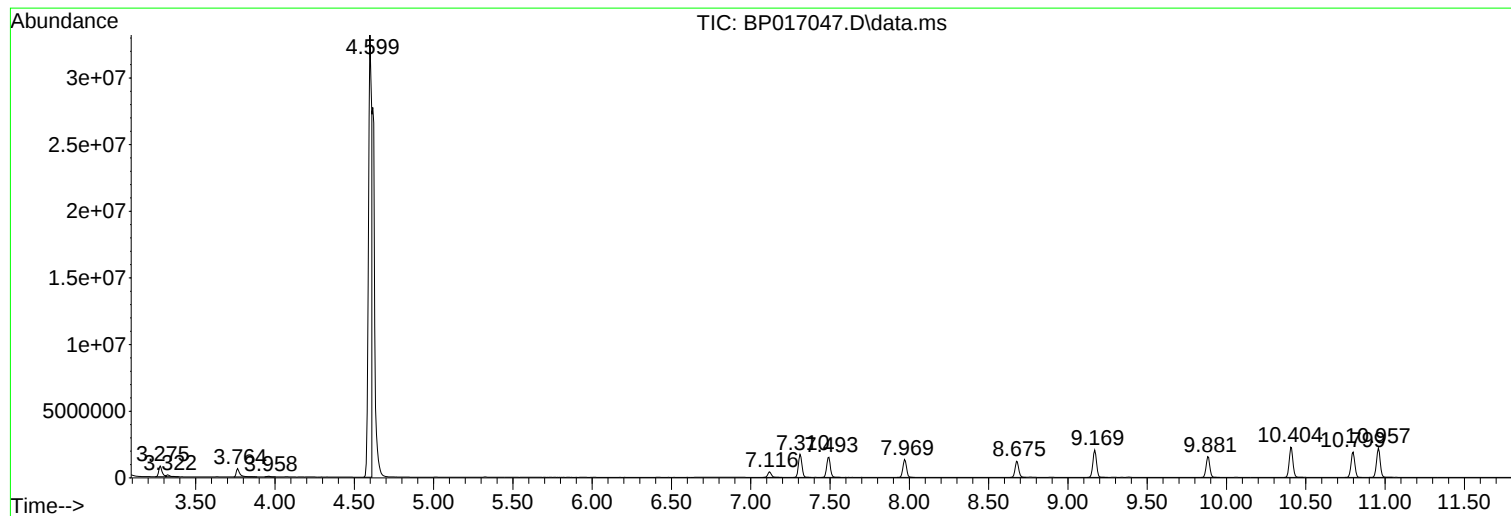

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017047.D
Acq On : 09 Sep 2023 12:17
Operator : MA/JU
Sample : 04227-07
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH9X8










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.599	465.53 ng/ul	48610500	1,4-Dichlorobenzene-d4	7.969

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	99
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	99
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
5			Pyrimidine, 5-fluoro-2,4-dichloro-	166	C4HC12FN2	002927-71-1	38

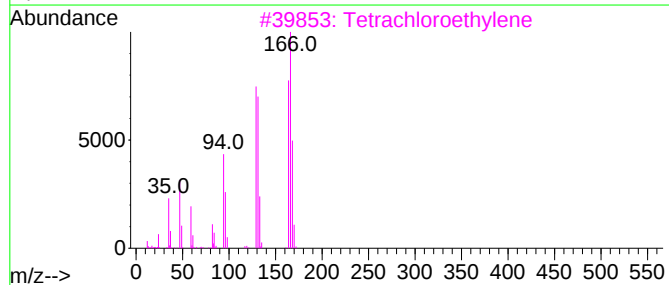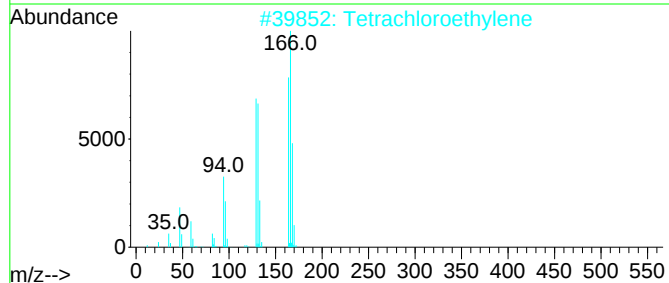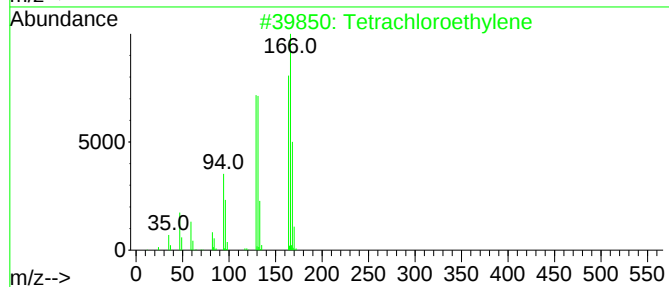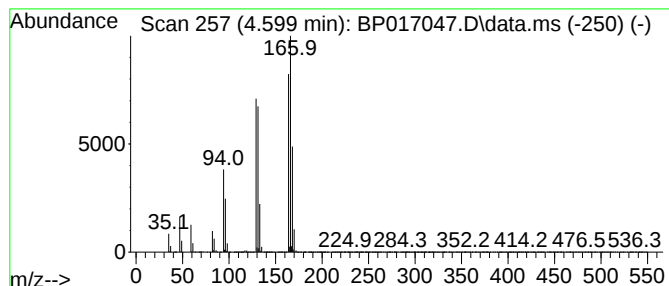

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017047.D
Acq On : 09 Sep 2023 12:17
Operator : MA/JU
Sample : 04227-07
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH9X8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.599	465.5	ng/ul	48610500	1	7.969	2088400	20.0