

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
 Data File : BP017051.D
 Acq On : 09 Sep 2023 14:34
 Operator : MA/JU
 Sample : 04227-15
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHA06

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017051.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	27	32	38	rBV	1051284	1539974	13.03%	1.256%
2	3.323	38	40	51	rVB	136779	196643	1.66%	0.160%
3	3.758	111	114	131	rBV	736664	1215454	10.28%	0.992%
4	3.958	143	148	155	rVB	69842	104976	0.89%	0.086%
5	4.070	164	167	173	rVB	22203	28845	0.24%	0.024%
6	4.464	231	234	240	rVB5	20096	31417	0.27%	0.026%
7	4.599	251	257	273	rVB	7825680	11462779	96.96%	9.352%
8	5.017	323	328	332	rBV	20126	32440	0.27%	0.026%
9	5.058	332	335	342	rVB9	9424	14598	0.12%	0.012%
10	5.240	362	366	372	rVB	22634	34272	0.29%	0.028%
11	5.599	424	427	432	rBV3	7984	12838	0.11%	0.010%
12	5.652	432	436	444	rVB	29959	45943	0.39%	0.037%
13	6.669	604	609	614	rBV2	9136	16938	0.14%	0.014%
14	6.916	648	651	663	rVB5	14971	34273	0.29%	0.028%
15	7.116	679	685	699	rBV	535177	862945	7.30%	0.704%
16	7.311	711	718	729	rVB	2021196	3037900	25.70%	2.478%
17	7.493	742	749	763	rBV	1815755	2937211	24.84%	2.396%
18	7.969	822	830	842	rBV	1345806	2069173	17.50%	1.688%
19	8.322	884	890	896	rBV6	11117	18202	0.15%	0.015%
20	8.681	941	951	964	rBV	1473577	2402761	20.32%	1.960%
21	9.046	1008	1013	1017	rBV4	12256	16930	0.14%	0.014%
22	9.169	1025	1034	1045	rBV	2383709	3757616	31.78%	3.066%
23	9.263	1046	1050	1058	rVV7	11601	29664	0.25%	0.024%
24	9.334	1058	1062	1067	rVV7	16772	28714	0.24%	0.023%
25	9.387	1067	1071	1078	rVB6	12435	22945	0.19%	0.019%
26	9.757	1130	1134	1139	rBV7	6681	11886	0.10%	0.010%
27	9.881	1148	1155	1165	rBV	1814384	2912627	24.64%	2.376%
28	10.404	1237	1244	1258	rBV	2528830	4215303	35.66%	3.439%
29	10.652	1282	1286	1292	rVB8	10391	20030	0.17%	0.016%
30	10.799	1302	1311	1320	rBV	1844757	3051493	25.81%	2.490%
31	10.875	1320	1324	1330	rVV4	8557	15107	0.13%	0.012%
32	10.957	1330	1338	1354	rBV	2322811	3851764	32.58%	3.142%
33	11.357	1400	1406	1412	rBV4	12368	21974	0.19%	0.018%
34	11.546	1432	1438	1440	rBV7	6862	13241	0.11%	0.011%
35	11.616	1446	1450	1455	rVB8	9161	16103	0.14%	0.013%
36	11.946	1497	1506	1514	rVB8	13023	32456	0.27%	0.026%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
 Data File : BP017051.D
 Acq On : 09 Sep 2023 14:34
 Operator : MA/JU
 Sample : 04227-15
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHA06

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
 Title : SVOA CALIBRATION

37	12.057	1519	1525	1531	rBV6	9288	18460	0.16%	0.015%
38	12.310	1563	1568	1574	rBV	109395	172558	1.46%	0.141%
39	12.375	1574	1579	1585	rVB2	45229	79388	0.67%	0.065%
40	12.698	1624	1634	1641	rBV9	10598	27757	0.23%	0.023%
41	13.340	1738	1743	1745	rBV6	9059	14208	0.12%	0.012%
42	13.475	1760	1766	1770	rBV2	50805	87485	0.74%	0.071%
43	13.610	1781	1789	1792	rBV9	17774	34753	0.29%	0.028%
44	14.040	1856	1862	1870	rBV	4853295	6636434	56.13%	5.414%
45	14.328	1904	1911	1925	rBV	5769752	8003960	67.70%	6.530%
46	14.628	1953	1962	1969	rBV	2725654	3847582	32.55%	3.139%
47	14.840	1993	1998	2013	rBV	377944	636776	5.39%	0.520%
48	15.251	2065	2068	2072	rVB6	9043	12223	0.10%	0.010%
49	15.345	2079	2084	2085	rBV5	8032	12732	0.11%	0.010%
50	15.622	2124	2131	2138	rBV	7163651	9808159	82.96%	8.002%
51	15.687	2138	2142	2146	rVV4	54505	89513	0.76%	0.073%
52	15.745	2146	2152	2160	rVV	2323935	3080950	26.06%	2.514%
53	15.816	2162	2164	2167	rVV	33603	44038	0.37%	0.036%
54	15.857	2168	2171	2181	rVV4	37356	91155	0.77%	0.074%
55	15.957	2185	2188	2196	rVB7	18354	33866	0.29%	0.028%
56	16.410	2261	2265	2269	rVB6	10651	13908	0.12%	0.011%
57	17.128	2384	2387	2391	rVB5	12094	16137	0.14%	0.013%
58	17.392	2426	2432	2442	rBV	3313509	4505228	38.11%	3.676%
59	17.492	2443	2449	2463	rBV	7381987	10596163	89.63%	8.645%
60	18.233	2571	2575	2582	rBV	145895	216687	1.83%	0.177%
61	19.304	2753	2757	2761	rBV2	77262	110404	0.93%	0.090%
62	19.369	2765	2768	2778	rVB	82747	121191	1.03%	0.099%
63	19.469	2782	2785	2792	rVV2	98983	131229	1.11%	0.107%
64	19.610	2806	2809	2812	rBV	39979	46231	0.39%	0.038%
65	19.733	2824	2830	2836	rBV	9540351	11822325	100.00%	9.645%
66	21.492	3124	3129	3135	rBV	3393411	4189771	35.44%	3.418%
67	23.863	3524	3532	3546	rVB2	4954848	10004988	84.63%	8.162%
68	24.027	3553	3560	3573	rVB	1902875	3949303	33.41%	3.222%




Sum of corrected areas: 122572997

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017051.D
Acq On : 09 Sep 2023 14:34
Operator : MA/JU
Sample : 04227-15
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHA06

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

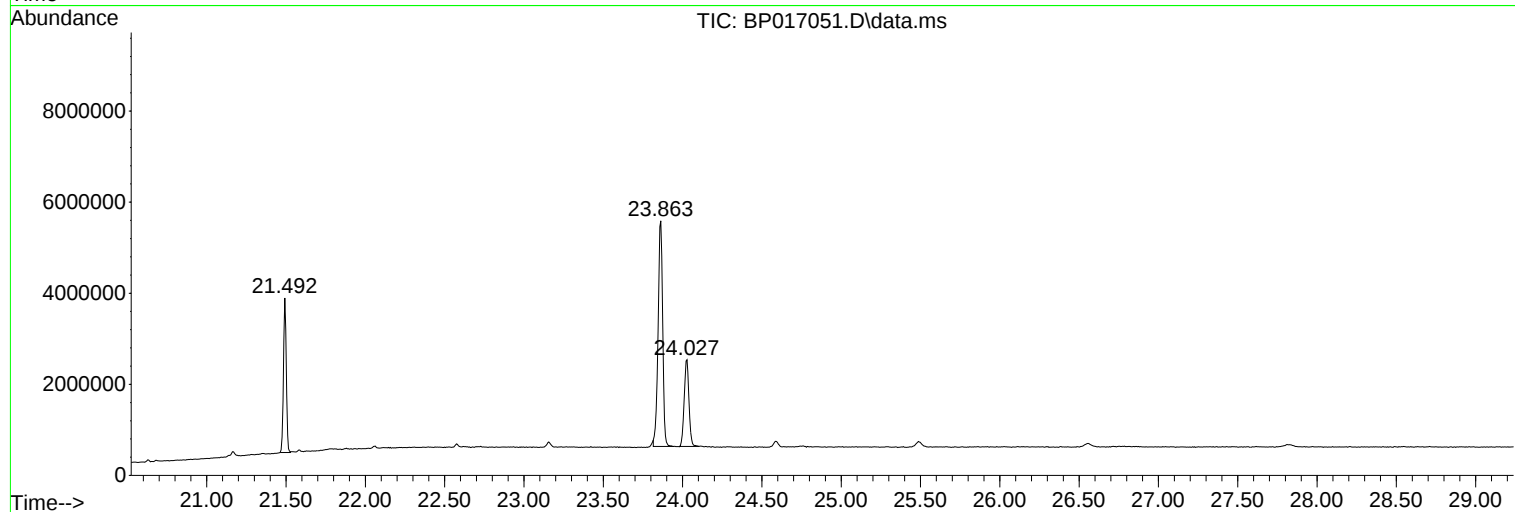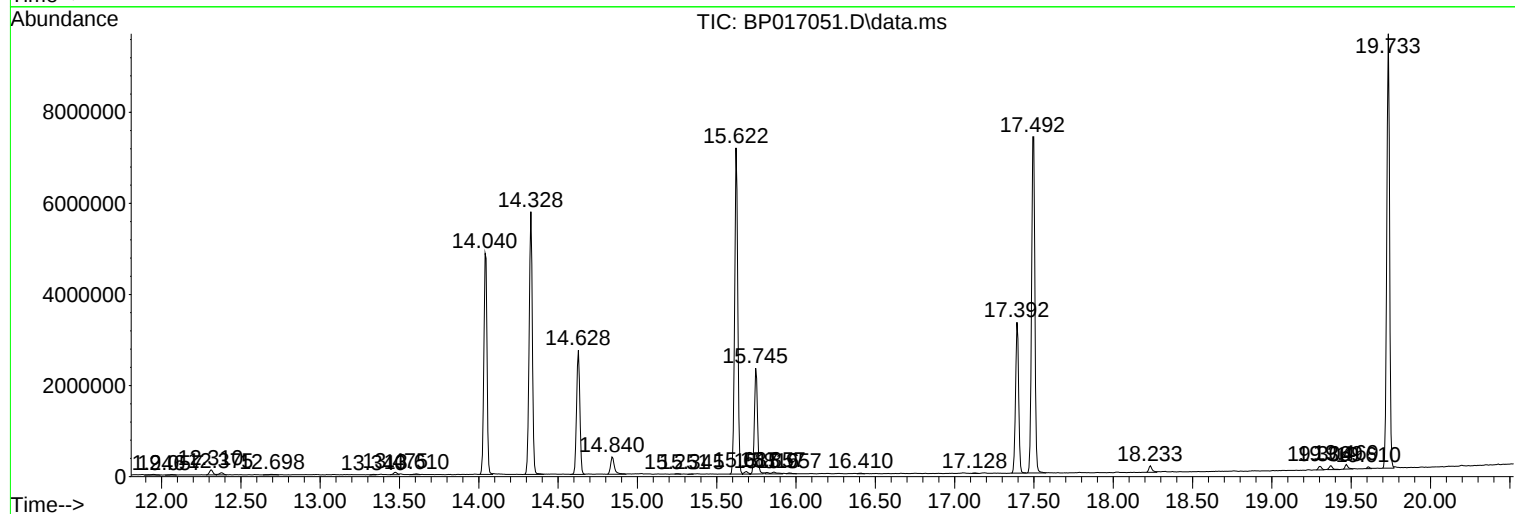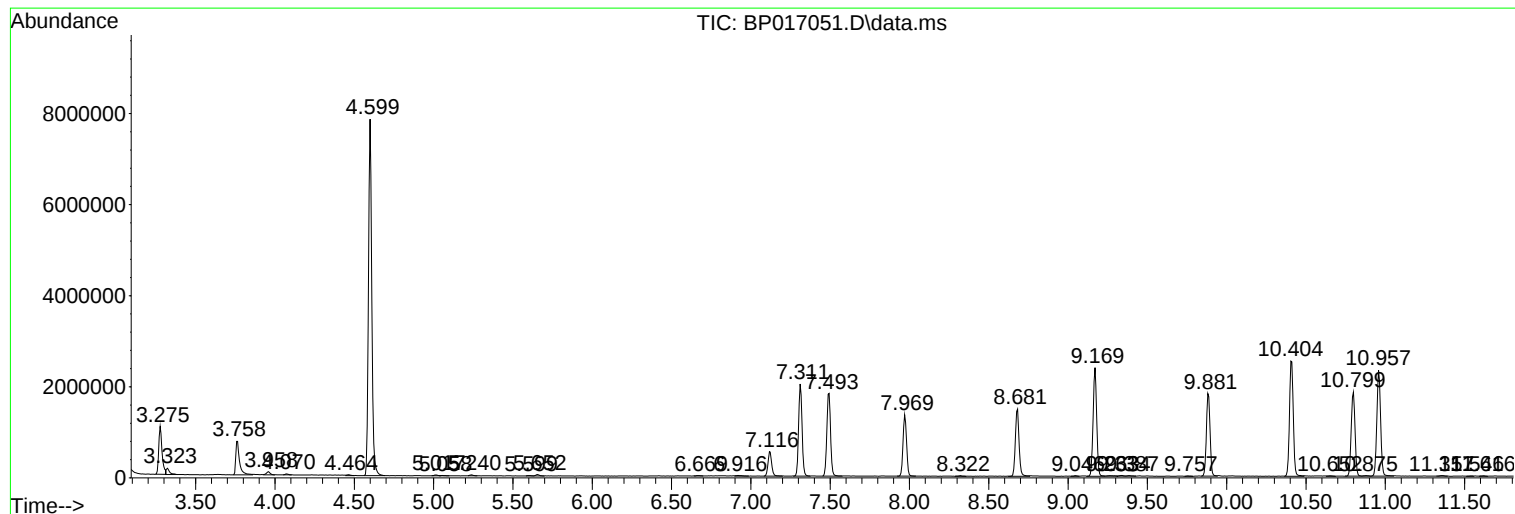

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017051.D
Acq On : 09 Sep 2023 14:34
Operator : MA/JU
Sample : 04227-15
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHA06










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.599	110.80 ng/ul	11462800	1,4-Dichlorobenzene-d4	7.969

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	94
5			Pyrimidine, 5-fluoro-2,4-dichloro-	166	C4HC12FN2	002927-71-1	35

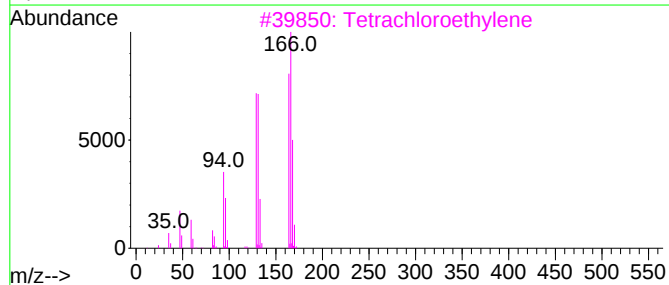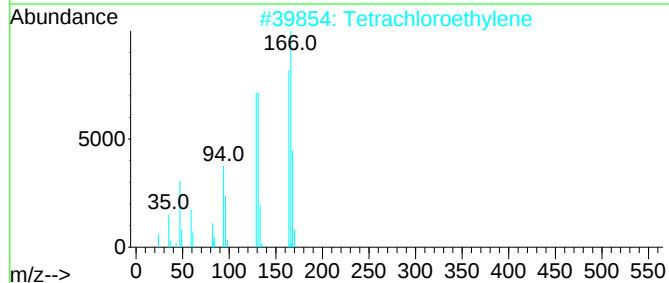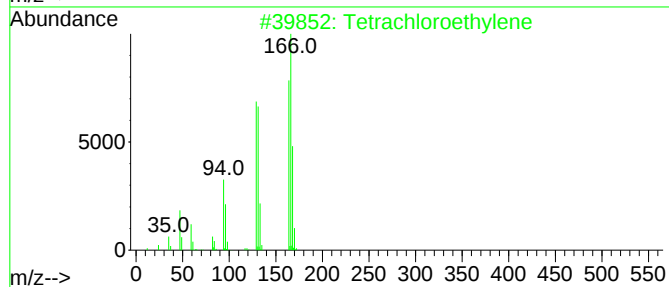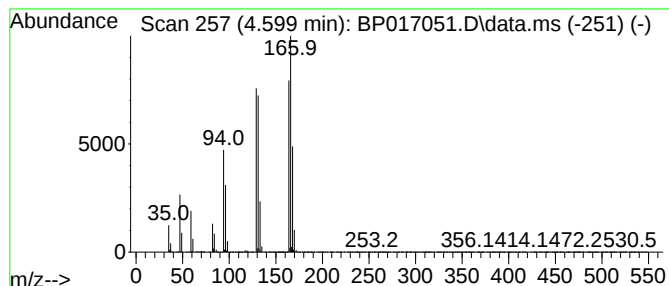

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017051.D
Acq On : 09 Sep 2023 14:34
Operator : MA/JU
Sample : 04227-15
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHA06

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.599	110.8	ng/ul	11462800	1	7.969	2069170	20.0