

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
 Data File : BP017053.D
 Acq On : 09 Sep 2023 15:43
 Operator : MA/JU
 Sample : 04227-17
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBKF2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017053.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.322	36	40	49	rVB	84708	111563	0.94%	0.111%
2	3.764	111	115	134	rBV	549713	952503	8.05%	0.947%
3	3.958	143	148	156	rVB	52058	84894	0.72%	0.084%
4	4.075	164	168	174	rVB	18067	31571	0.27%	0.031%
5	4.599	252	257	264	rBV	37907	60764	0.51%	0.060%
6	5.011	324	327	331	rBV	14071	18192	0.15%	0.018%
7	6.916	648	651	660	rBV	6468	14298	0.12%	0.014%
8	7.116	678	685	696	rBV	413021	684189	5.79%	0.680%
9	7.310	711	718	729	rBV	1692730	2586711	21.87%	2.572%
10	7.493	742	749	758	rBV	1519443	2450629	20.72%	2.437%
11	7.657	772	777	783	rVB9	5783	14369	0.12%	0.014%
12	7.905	814	819	821	rBV2	8311	11910	0.10%	0.012%
13	7.969	823	830	842	rVB	1104511	1719622	14.54%	1.710%
14	8.675	942	950	964	rBV	1188532	1950583	16.49%	1.940%
15	9.169	1026	1034	1045	rBV	2040751	3251514	27.50%	3.234%
16	9.281	1050	1053	1059	rVB8	8504	14554	0.12%	0.014%
17	9.381	1066	1070	1076	rVB6	7802	13484	0.11%	0.013%
18	9.881	1148	1155	1167	rBV	1572717	2557407	21.63%	2.543%
19	10.404	1236	1244	1258	rBV	2183467	3597931	30.43%	3.578%
20	10.798	1302	1311	1321	rBV	1514589	2556853	21.62%	2.543%
21	10.957	1330	1338	1358	rBV	2208365	3666040	31.00%	3.646%
22	11.487	1423	1428	1433	rVB8	5995	13443	0.11%	0.013%
23	12.375	1574	1579	1586	rVB	39134	65806	0.56%	0.065%
24	13.475	1759	1766	1772	rBV3	24739	44261	0.37%	0.044%
25	13.587	1779	1785	1789	rBV8	7217	13191	0.11%	0.013%
26	14.039	1856	1862	1872	rBV	4485006	6123372	51.78%	6.090%
27	14.328	1904	1911	1922	rBV	4940389	7108493	60.11%	7.069%
28	14.628	1955	1962	1974	rBV	2279067	3275904	27.70%	3.258%
29	14.839	1993	1998	2013	rBV	321340	551243	4.66%	0.548%
30	14.998	2022	2025	2028	rBV5	8415	11955	0.10%	0.012%
31	15.057	2033	2035	2042	rVB8	10214	15894	0.13%	0.016%
32	15.622	2124	2131	2140	rBV	6901993	9105891	77.00%	9.056%
33	15.745	2146	2152	2167	rBV	2136284	2815035	23.80%	2.799%
34	15.857	2167	2171	2177	rVB	26899	38679	0.33%	0.038%
35	16.410	2259	2265	2268	rBV8	7459	13699	0.12%	0.014%
36	16.904	2345	2349	2352	rVB6	8544	12535	0.11%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017053.D
Acq On : 09 Sep 2023 15:43
Operator : MA/JU
Sample : 04227-17
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBKF2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Title : SVOA CALIBRATION

37	17.051	2368	2374	2379	rBV10	10881	24405	0.21%	0.024%
38	17.186	2392	2397	2399	rBV2	7841	12767	0.11%	0.013%
39	17.392	2426	2432	2441	rBV	2872186	3940678	33.32%	3.919%
40	17.498	2443	2450	2461	rBV	7269196	10297628	87.08%	10.241%
41	18.028	2536	2540	2544	rBV7	8977	11997	0.10%	0.012%
42	18.233	2570	2575	2584	rBV	242161	367855	3.11%	0.366%
43	19.304	2753	2757	2760	rBV2	77505	99427	0.84%	0.099%
44	19.369	2765	2768	2773	rVB	76998	107501	0.91%	0.107%
45	19.469	2781	2785	2795	rBV	172738	254795	2.15%	0.253%
46	19.610	2806	2809	2812	rBV2	36894	40916	0.35%	0.041%
47	19.733	2824	2830	2836	rBV	9378979	11825567	100.00%	11.760%
48	21.492	3124	3129	3137	rBV	2919750	3767322	31.86%	3.747%
49	23.857	3521	3531	3548	rVB2	5109444	10664338	90.18%	10.605%
50	24.021	3553	3559	3569	rVB	1756669	3580833	30.28%	3.561%




Sum of corrected areas: 100555011

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017053.D
Acq On : 09 Sep 2023 15:43
Operator : MA/JU
Sample : 04227-17
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBKF2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

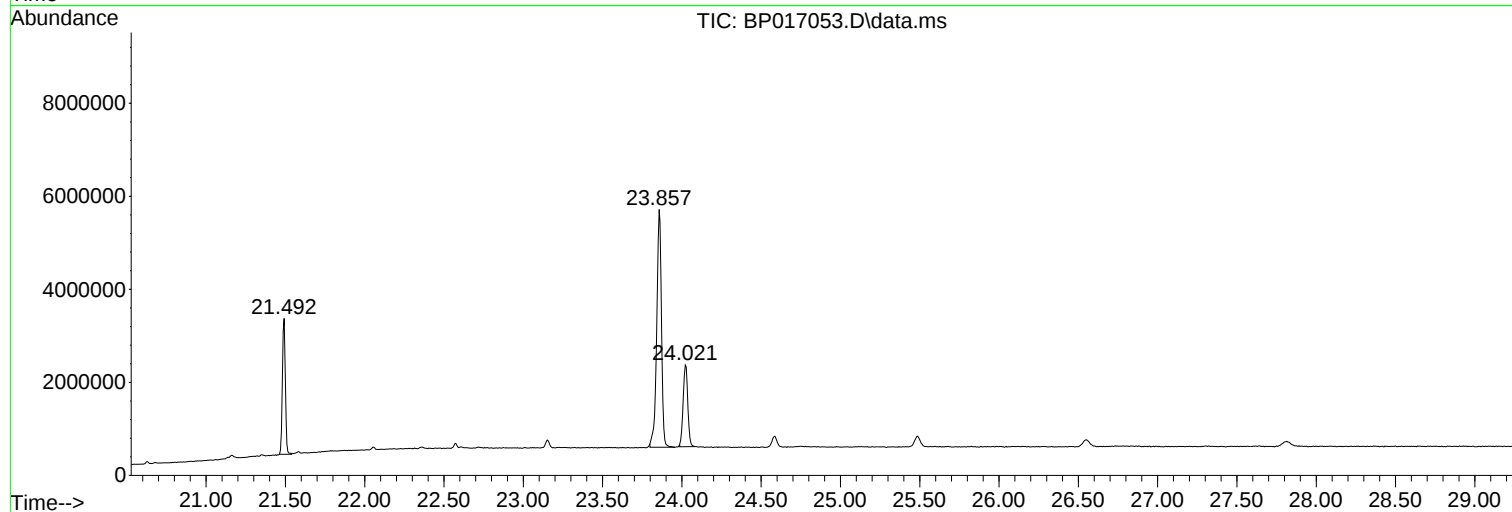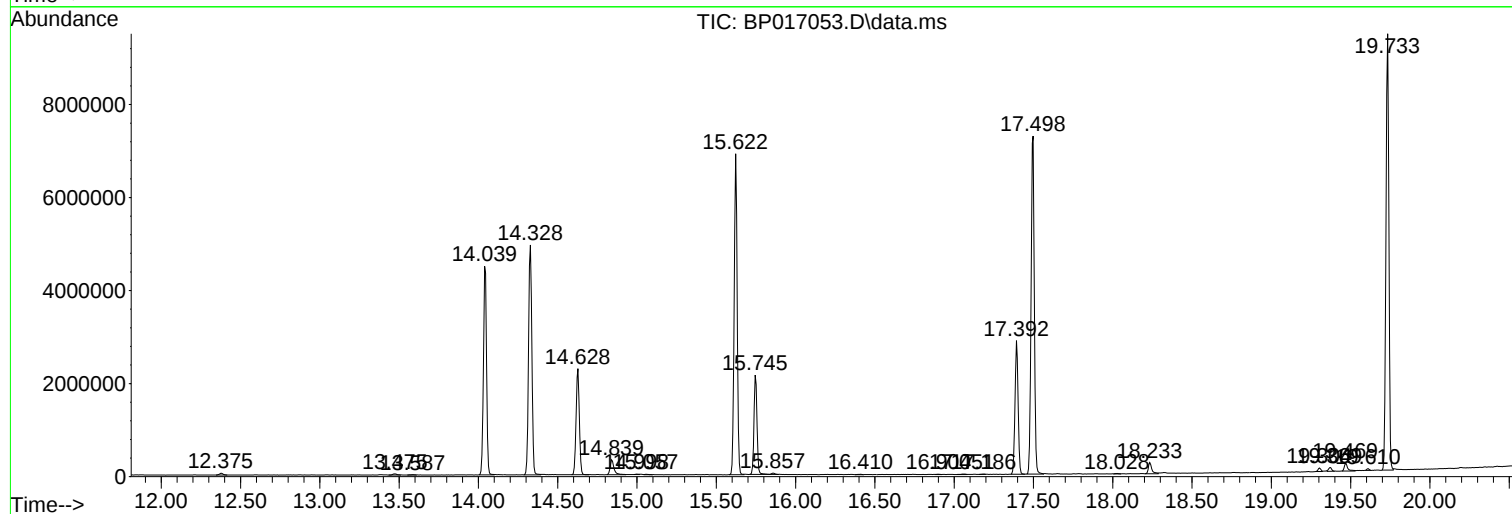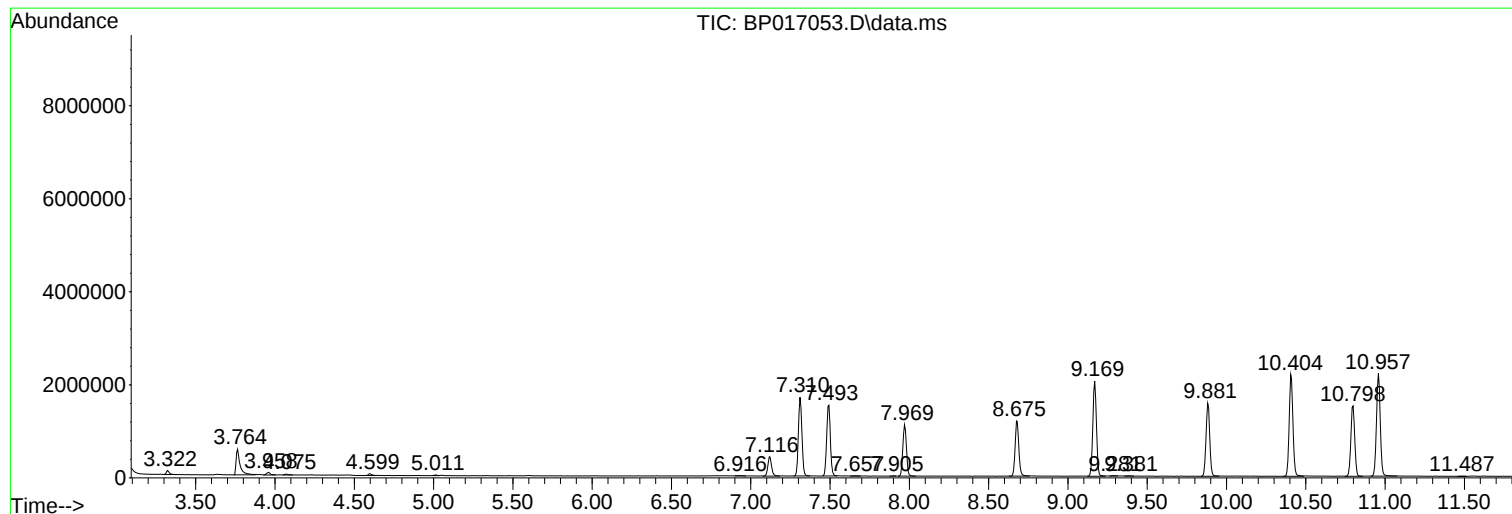

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017053.D
Acq On : 09 Sep 2023 15:43
Operator : MA/JU
Sample : 04227-17
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBKF2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017053.D
Acq On : 09 Sep 2023 15:43
Operator : MA/JU
Sample : 04227-17
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBKF2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc