

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
 Data File : BP017056.D
 Acq On : 09 Sep 2023 17:26
 Operator : MA/JU
 Sample : 04227-20
 Misc :
 ALS Vial : 67 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBJ92

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017056.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.322	36	40	46	rVB	89797	113464	1.14%	0.123%
2	3.763	111	115	130	rBV	579610	925329	9.26%	1.001%
3	3.958	143	148	156	rVB	53057	86878	0.87%	0.094%
4	4.069	164	167	171	rVB	19435	24791	0.25%	0.027%
5	4.599	252	257	264	rBV2	43196	66035	0.66%	0.071%
6	5.016	324	328	331	rBV	14199	19517	0.20%	0.021%
7	5.052	332	334	338	rVB3	8999	10704	0.11%	0.012%
8	6.022	494	499	503	rVB5	10914	17227	0.17%	0.019%
9	6.916	649	651	659	rVB8	10235	17871	0.18%	0.019%
10	7.116	679	685	696	rBV	387501	611311	6.12%	0.661%
11	7.310	711	718	728	rVB	1634760	2454424	24.58%	2.655%
12	7.487	741	748	757	rBV	1440064	2260434	22.63%	2.445%
13	7.969	822	830	842	rVB	1293853	1993310	19.96%	2.156%
14	8.675	942	950	962	rBV	1077135	1761016	17.63%	1.905%
15	9.169	1026	1034	1045	rBV	1903848	3020839	30.25%	3.268%
16	9.281	1050	1053	1058	rVB6	6499	10341	0.10%	0.011%
17	9.487	1082	1088	1092	rBV4	12734	21453	0.21%	0.023%
18	9.881	1147	1155	1171	rBV	1448553	2376988	23.80%	2.571%
19	10.404	1237	1244	1258	rBV	2063834	3345129	33.49%	3.618%
20	10.793	1303	1310	1321	rBV	1720182	2925991	29.30%	3.165%
21	10.957	1329	1338	1355	rBV	1851319	3103561	31.07%	3.357%
22	11.540	1433	1437	1443	rBV9	6665	14947	0.15%	0.016%
23	11.616	1444	1450	1456	rVV	35698	59094	0.59%	0.064%
24	12.375	1572	1579	1585	rBV	37646	64854	0.65%	0.070%
25	13.475	1759	1766	1772	rBV	43479	73927	0.74%	0.080%
26	13.587	1782	1785	1791	rVB7	6903	11260	0.11%	0.012%
27	14.039	1856	1862	1876	rBV	4336154	5632201	56.39%	6.092%
28	14.328	1903	1911	1923	rBV	4612454	6550649	65.59%	7.086%
29	14.628	1955	1962	1969	rBV	2581634	3669689	36.74%	3.969%
30	14.839	1992	1998	2015	rBV	254287	473216	4.74%	0.512%
31	15.622	2123	2131	2137	rBV	6044323	8191348	82.02%	8.861%
32	15.686	2137	2142	2147	rVV	215270	316664	3.17%	0.343%
33	15.745	2147	2152	2167	rVV	1882460	2490668	24.94%	2.694%
34	15.857	2167	2171	2176	rVB2	23177	36747	0.37%	0.040%
35	16.357	2252	2256	2260	rVB6	8873	11583	0.12%	0.013%
36	16.404	2260	2264	2267	rBV6	8027	11591	0.12%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
 Data File : BP017056.D
 Acq On : 09 Sep 2023 17:26
 Operator : MA/JU
 Sample : 04227-20
 Misc :
 ALS Vial : 67 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBJ92

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
 Title : SVOA CALIBRATION

37	17.063	2372	2376	2380	rBV7	7548	12259	0.12%	0.013%
38	17.175	2393	2395	2402	rVB4	5551	10080	0.10%	0.011%
39	17.392	2426	2432	2442	rBV	3070131	4239941	42.45%	4.586%
40	17.492	2442	2449	2462	rVV	6596724	8891324	89.03%	9.618%
41	17.639	2472	2474	2480	rVB5	8669	13650	0.14%	0.015%
42	18.233	2571	2575	2584	rBV	107702	158471	1.59%	0.171%
43	19.298	2753	2756	2760	rBV2	64674	78595	0.79%	0.085%
44	19.369	2764	2768	2778	rVB	73389	102879	1.03%	0.111%
45	19.469	2782	2785	2792	rVB3	55258	71258	0.71%	0.077%
46	19.604	2805	2808	2812	rBV4	41885	53894	0.54%	0.058%
47	19.733	2824	2830	2836	rBV	7668695	9987401	100.00%	10.803%
48	21.486	3123	3128	3138	rBV	3041008	3937376	39.42%	4.259%
49	23.851	3523	3530	3541	rVB2	4263960	8444153	84.55%	9.134%
50	24.015	3552	3558	3568	rVB	1766079	3670973	36.76%	3.971%




Sum of corrected areas: 92447305

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017056.D
Acq On : 09 Sep 2023 17:26
Operator : MA/JU
Sample : 04227-20
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJ92

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

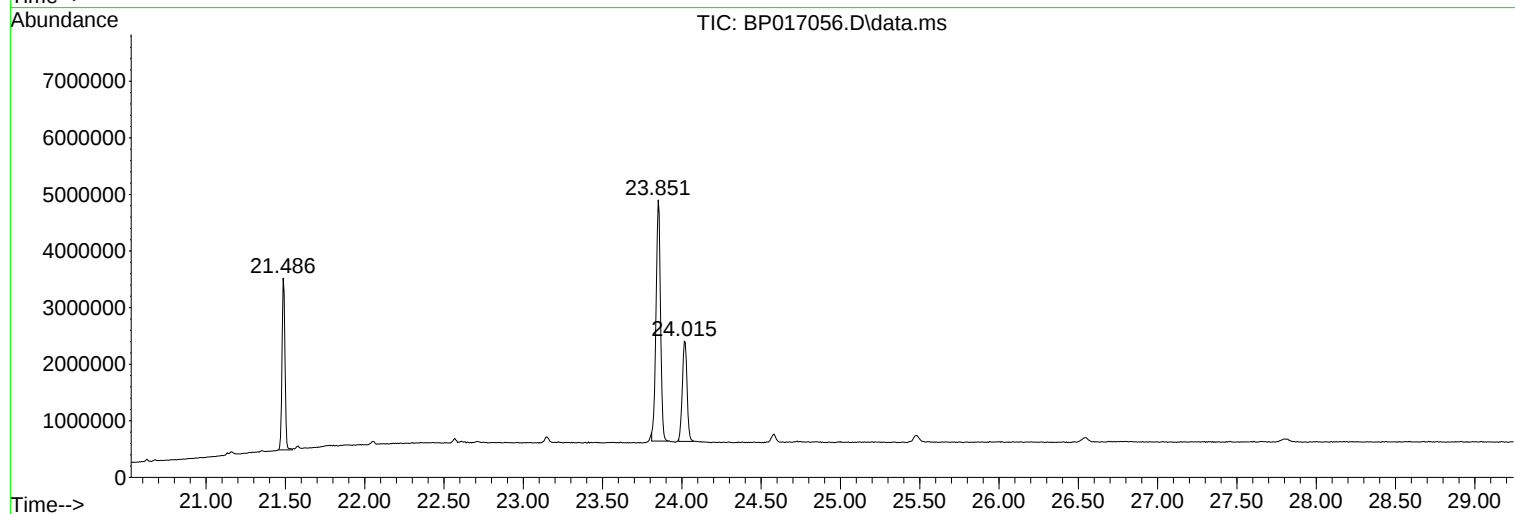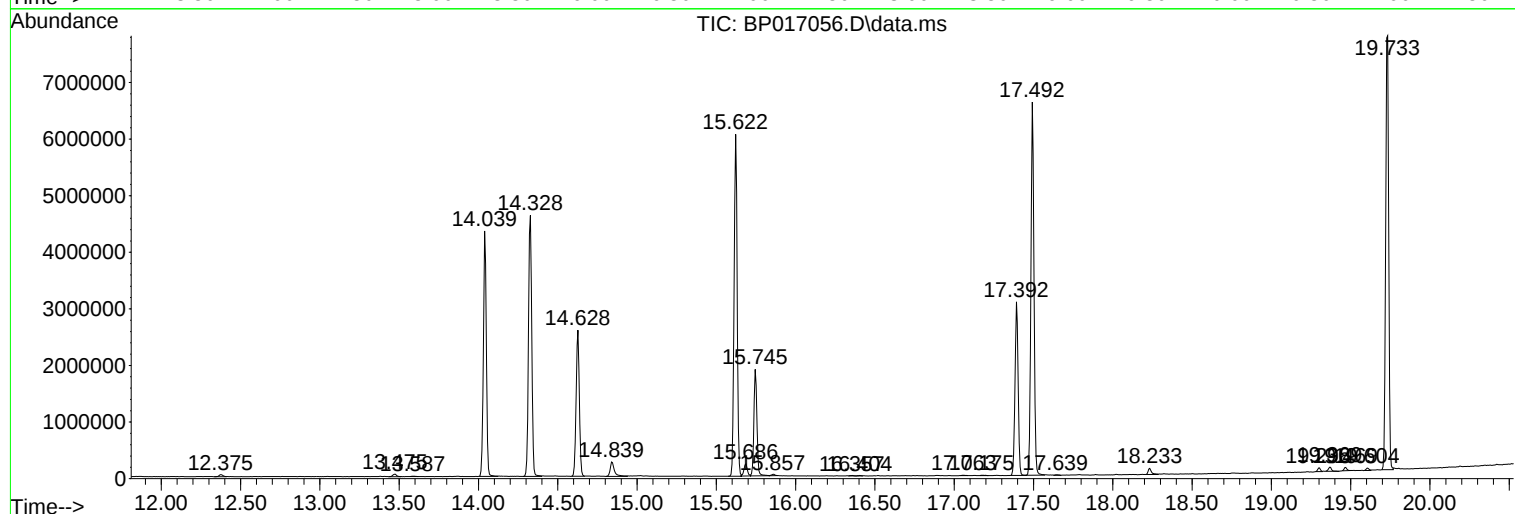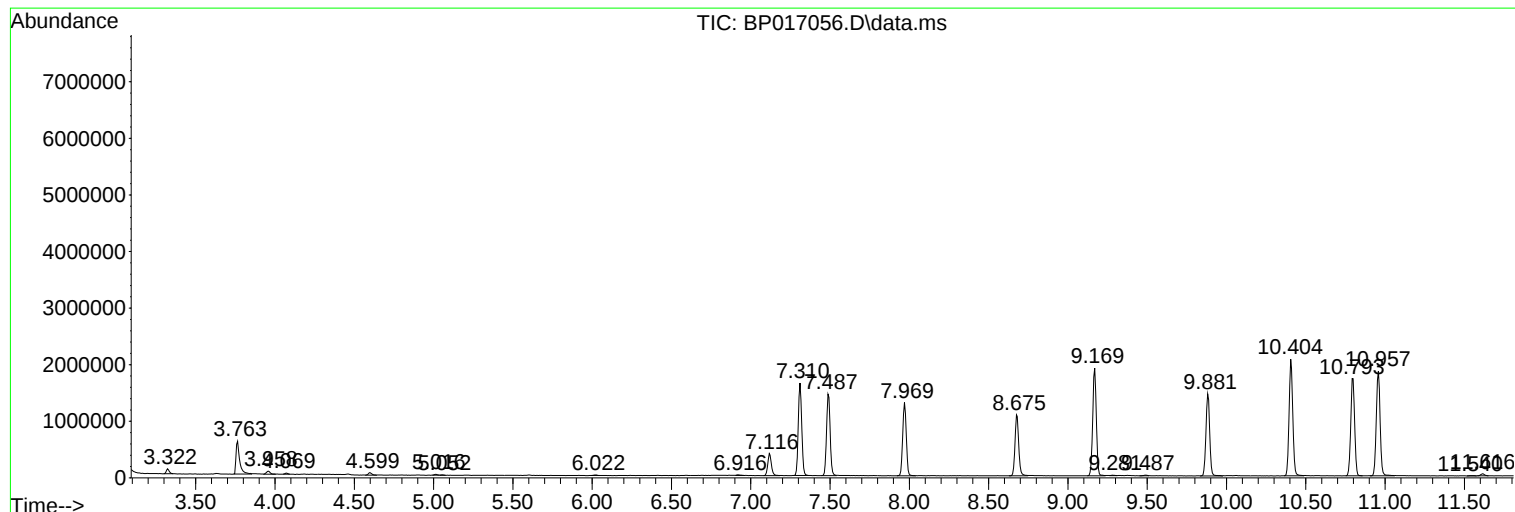

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017056.D
Acq On : 09 Sep 2023 17:26
Operator : MA/JU
Sample : 04227-20
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJ92

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017056.D
Acq On : 09 Sep 2023 17:26
Operator : MA/JU
Sample : 04227-20
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJ92

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc