

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
 Data File : BP017060.D
 Acq On : 09 Sep 2023 20:22
 Operator : MA/JU
 Sample : PB155261BL
 Misc :
 ALS Vial : 72 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK261

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017060.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.323	36	40	46	rBV	166545	218385	1.66%	0.154%
2	3.758	110	114	142	rBV	2280223	3489208	26.60%	2.457%
3	4.070	163	167	176	rVB	66626	95630	0.73%	0.067%
4	7.116	678	685	705	rVB	2642476	4124229	31.44%	2.905%
5	7.311	711	718	730	rVB	2242289	3355612	25.58%	2.363%
6	7.487	741	748	758	rBV	2660950	4171525	31.80%	2.938%
7	7.969	823	830	838	rBV	2058449	3124355	23.82%	2.200%
8	8.675	943	950	968	rBV	3130454	5143819	39.22%	3.623%
9	9.169	1026	1034	1047	rBV	2598197	4124899	31.45%	2.905%
10	9.881	1146	1155	1166	rBV	2149124	3382964	25.79%	2.383%
11	10.404	1236	1244	1259	rBV	3005429	4928495	37.57%	3.471%
12	10.793	1303	1310	1320	rBV	2812109	4636319	35.35%	3.265%
13	10.957	1329	1338	1355	rBV	3273061	5418830	41.31%	3.816%
14	12.375	1574	1579	1587	rVB	50154	83478	0.64%	0.059%
15	13.469	1760	1765	1772	rVB	45082	71935	0.55%	0.051%
16	14.040	1854	1862	1874	rBV	5650238	7610673	58.02%	5.360%
17	14.328	1903	1911	1928	rBV	6260231	8890063	67.78%	6.261%
18	14.628	1950	1962	1970	rBV	4234023	5987024	45.64%	4.217%
19	14.751	1977	1983	1989	rBV9	11042	17281	0.13%	0.012%
20	14.840	1991	1998	2019	rBV	2714008	4009419	30.57%	2.824%
21	15.063	2034	2036	2041	rVB6	9912	13535	0.10%	0.010%
22	15.428	2093	2098	2104	rBV5	8040	15220	0.12%	0.011%
23	15.622	2124	2131	2141	rBV	7857542	10774450	82.14%	7.588%
24	15.745	2146	2152	2164	rVV	2615068	3327723	25.37%	2.344%
25	15.857	2167	2171	2177	rVB	32679	49903	0.38%	0.035%
26	16.198	2224	2229	2234	rBV8	6691	13213	0.10%	0.009%
27	17.057	2371	2375	2382	rVB8	8548	16048	0.12%	0.011%
28	17.181	2391	2396	2403	rBV3	10173	19443	0.15%	0.014%
29	17.392	2425	2432	2441	rBV	5137753	6934175	52.87%	4.884%
30	17.492	2443	2449	2468	rVV2	8666779	11781991	89.82%	8.298%
31	18.228	2571	2574	2579	rBV7	15008	16617	0.13%	0.012%
32	19.298	2752	2756	2762	rBV2	84431	122338	0.93%	0.086%
33	19.369	2764	2768	2773	rVB	79584	108268	0.83%	0.076%
34	19.604	2805	2808	2813	rBV5	19585	29317	0.22%	0.021%
35	19.728	2823	2829	2843	rBV	10341773	13116626	100.00%	9.238%
36	21.486	3123	3128	3138	rBV2	4954102	6195864	47.24%	4.364%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017060.D
Acq On : 09 Sep 2023 20:22
Operator : MA/JU
Sample : PB155261BL
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK261

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Title : SVOA CALIBRATION

37	23.851	3520	3530	3545	rVB2	5338376	10984428	83.74%	7.736%
38	24.016	3551	3558	3571	rVB	2749856	5581534	42.55%	3.931%




Sum of corrected areas: 141984836

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017060.D
Acq On : 09 Sep 2023 20:22
Operator : MA/JU
Sample : PB155261BL
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK261

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

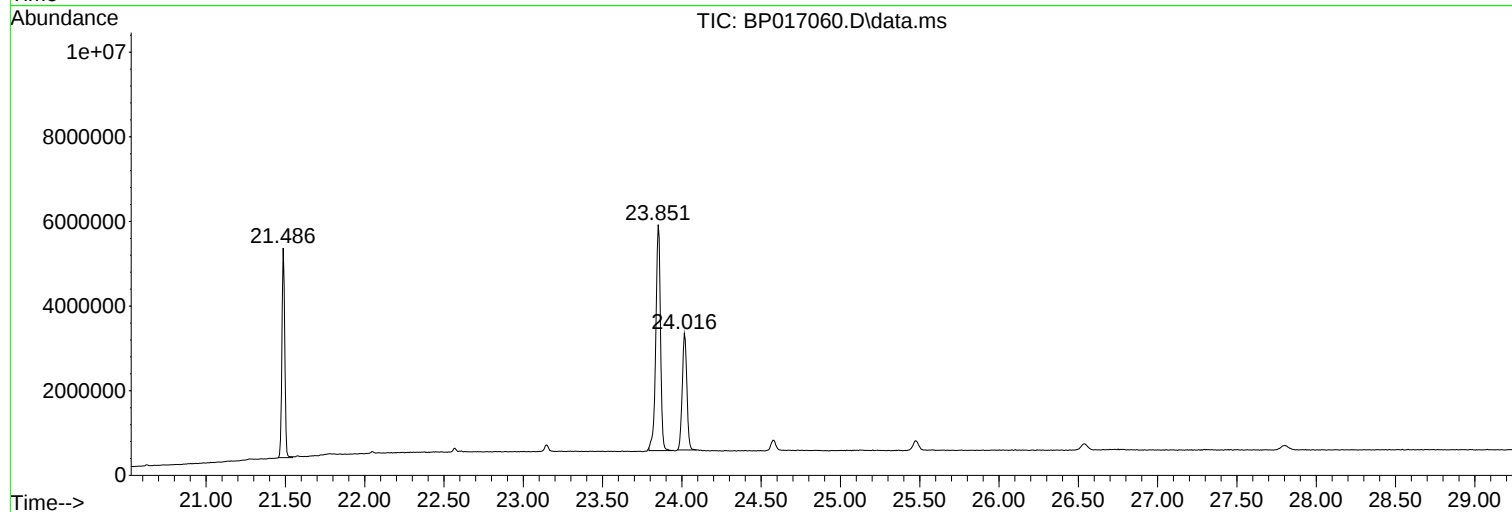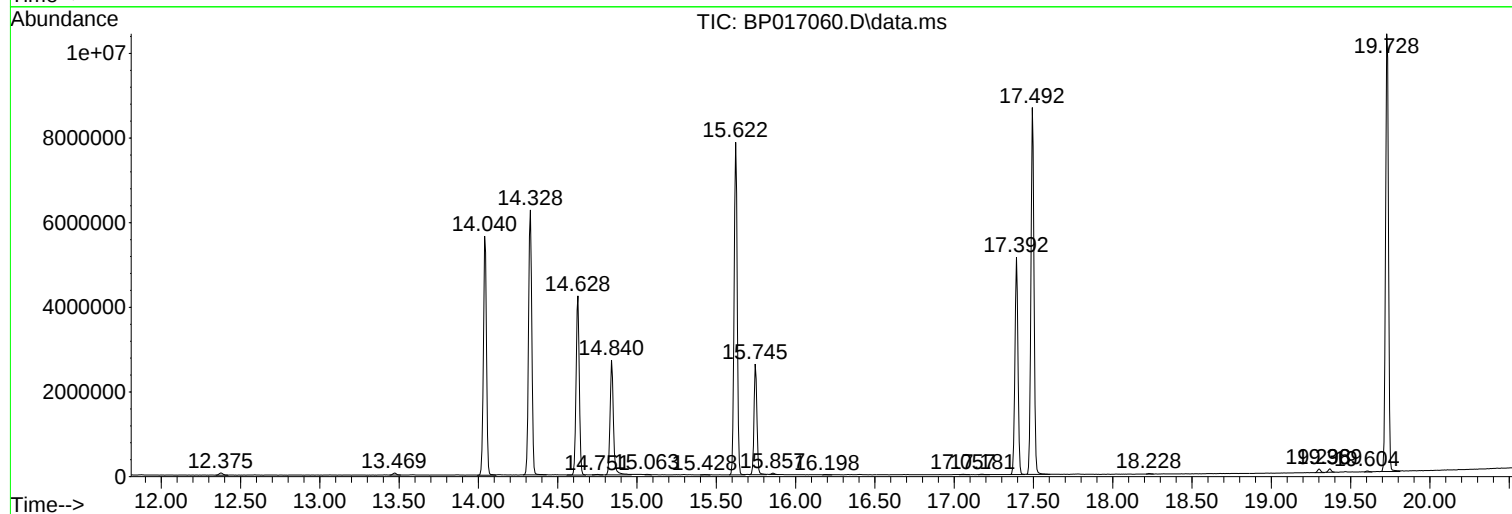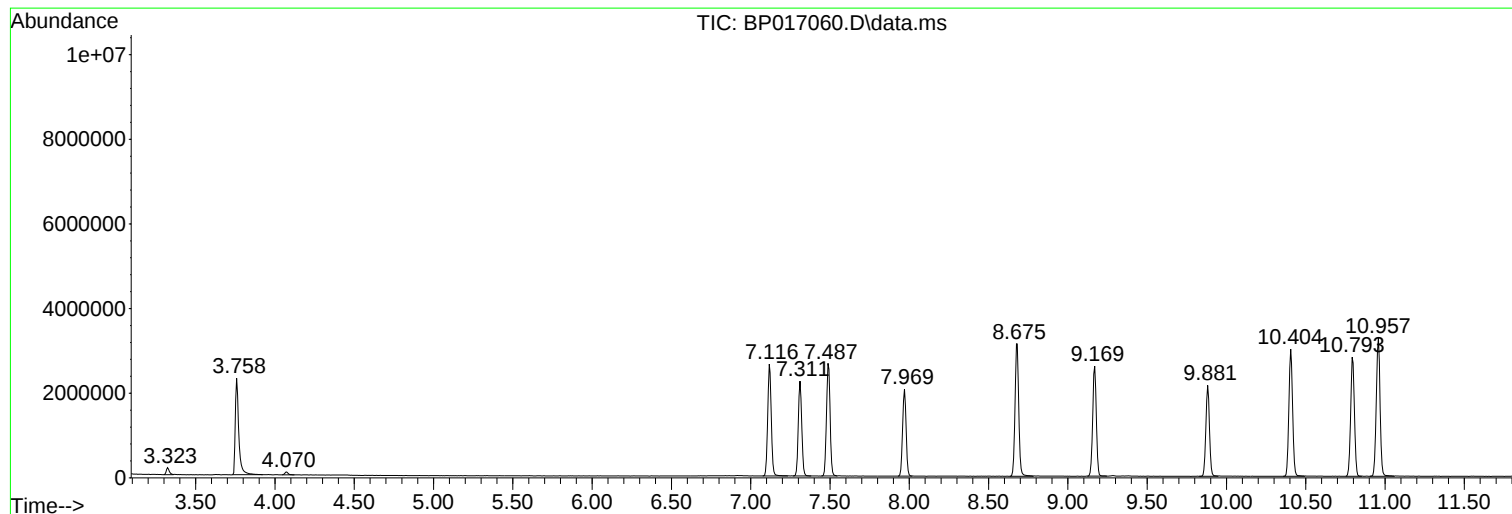

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017060.D
Acq On : 09 Sep 2023 20:22
Operator : MA/JU
Sample : PB155261BL
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK261

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017060.D
Acq On : 09 Sep 2023 20:22
Operator : MA/JU
Sample : PB155261BL
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK261

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc