

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
 Data File : BP017061.D
 Acq On : 09 Sep 2023 20:57
 Operator : MA/JU
 Sample : PB155264BL
 Misc :
 ALS Vial : 73 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK264

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017061.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.322	36	40	48	rBV	131902	173718	1.88%	0.176%
2	3.757	110	114	132	rBV	1808990	2815739	30.50%	2.854%
3	4.069	164	167	173	rVB3	18016	29398	0.32%	0.030%
4	7.116	676	685	702	rBV	2121927	3343352	36.21%	3.389%
5	7.310	710	718	726	rBV	1718049	2580297	27.95%	2.616%
6	7.487	740	748	761	rBV	2080346	3211854	34.79%	3.256%
7	7.969	822	830	839	rBV	1194170	1851541	20.05%	1.877%
8	8.675	942	950	968	rBV	2433640	3884913	42.08%	3.938%
9	9.169	1026	1034	1044	rBV	1945259	3116847	33.76%	3.160%
10	9.287	1050	1054	1058	rBV7	5240	9734	0.11%	0.010%
11	9.881	1146	1155	1164	rBV	1604081	2520989	27.30%	2.556%
12	10.404	1233	1244	1260	rBV	2320728	3764933	40.78%	3.817%
13	10.792	1303	1310	1319	rBV	1629918	2687255	29.11%	2.724%
14	10.957	1328	1338	1351	rBV	2351071	3900782	42.25%	3.954%
15	12.310	1565	1568	1574	rBV4	10985	17358	0.19%	0.018%
16	12.375	1574	1579	1587	rVB2	35966	62096	0.67%	0.063%
17	13.469	1760	1765	1774	rVB2	28323	48882	0.53%	0.050%
18	14.039	1855	1862	1874	rBV	3973665	5277600	57.16%	5.350%
19	14.327	1902	1911	1925	rBV	4403287	6386968	69.18%	6.475%
20	14.622	1955	1961	1972	rBV	2321226	3401995	36.85%	3.449%
21	14.839	1990	1998	2015	rBV	1825998	2730732	29.58%	2.768%
22	15.622	2122	2131	2142	rBV	5922453	7841936	84.93%	7.950%
23	15.745	2146	2152	2166	rVV	1671981	2171536	23.52%	2.201%
24	15.857	2166	2171	2181	rVB3	25306	49863	0.54%	0.051%
25	16.398	2260	2263	2270	rBV9	7256	14613	0.16%	0.015%
26	17.051	2371	2374	2381	rVB8	8249	14374	0.16%	0.015%
27	17.174	2391	2395	2400	rBV6	7903	12790	0.14%	0.013%
28	17.392	2425	2432	2442	rBV	2900814	3923971	42.50%	3.978%
29	17.492	2442	2449	2467	rVV	6287868	8415602	91.15%	8.531%
30	18.227	2571	2574	2578	rBV5	8562	13888	0.15%	0.014%
31	19.298	2752	2756	2761	rBV	63556	82501	0.89%	0.084%
32	19.368	2764	2768	2777	rVV	62529	90387	0.98%	0.092%
33	19.727	2823	2829	2839	rBV	7453745	9232962	100.00%	9.360%
34	21.486	3123	3128	3134	rBV	2894885	3525765	38.19%	3.574%
35	23.851	3523	3530	3542	rVB2	4091708	8043840	87.12%	8.154%
36	24.015	3551	3558	3570	rVB	1646319	3393404	36.75%	3.440%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017061.D
Acq On : 09 Sep 2023 20:57
Operator : MA/JU
Sample : PB155264BL
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK264

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 98644415

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017061.D
Acq On : 09 Sep 2023 20:57
Operator : MA/JU
Sample : PB155264BL
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK264

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

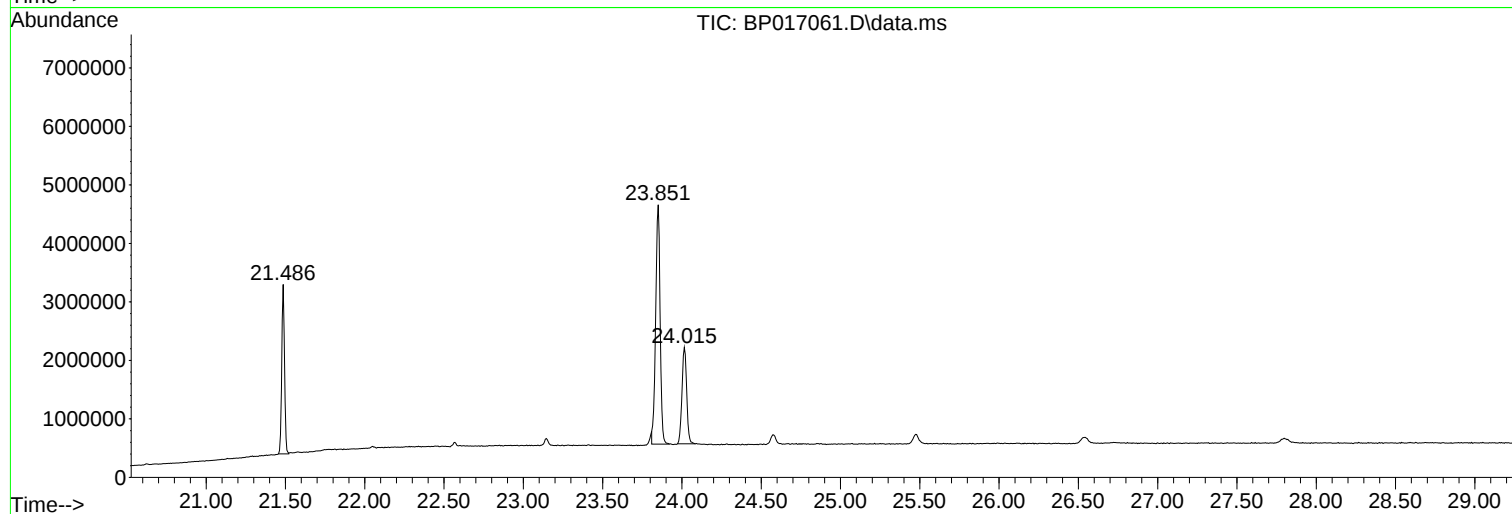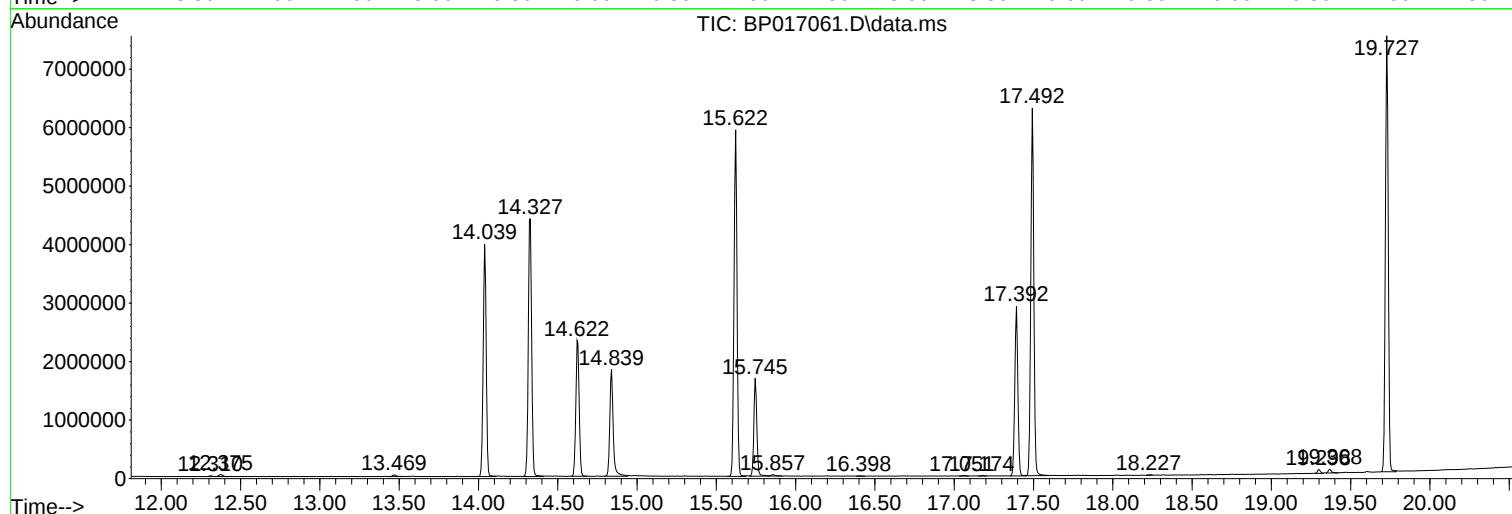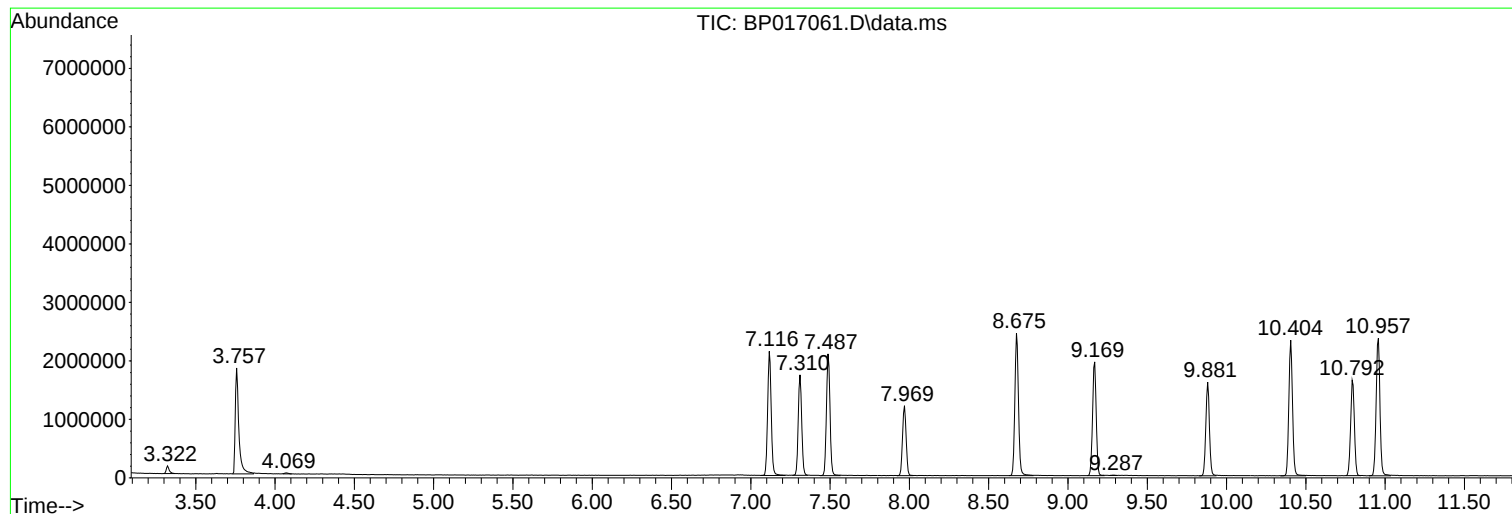

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017061.D
Acq On : 09 Sep 2023 20:57
Operator : MA/JU
Sample : PB155264BL
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK264

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017061.D
Acq On : 09 Sep 2023 20:57
Operator : MA/JU
Sample : PB155264BL
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK264

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc