

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
 Data File : BP017063.D
 Acq On : 09 Sep 2023 22:05
 Operator : MA/JU
 Sample : PB155238BL
 Misc :
 ALS Vial : 75 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK238

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017063.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.322	36	40	49	rBV	173318	228370	2.61%	0.202%
2	3.764	111	115	129	rBV	1250530	1815356	20.74%	1.610%
3	4.069	164	167	173	rBV	36025	54792	0.63%	0.049%
4	7.116	678	685	705	rBV	2585985	4078516	46.59%	3.616%
5	7.310	711	718	728	rVB	2176458	3256520	37.20%	2.887%
6	7.487	741	748	760	rBV	2570908	4052735	46.29%	3.593%
7	7.969	823	830	838	rBV	2279454	3524732	40.26%	3.125%
8	8.675	943	950	967	rBV	2962403	4839295	55.28%	4.291%
9	9.169	1026	1034	1043	rBV	2451860	3887610	44.41%	3.447%
10	9.287	1050	1054	1058	rVB7	10970	15284	0.17%	0.014%
11	9.881	1147	1155	1165	rBV	1956614	3157421	36.07%	2.799%
12	10.404	1234	1244	1258	rBV	2834631	4605107	52.60%	4.083%
13	10.793	1301	1310	1320	rBV	3002648	4987141	56.97%	4.422%
14	10.957	1330	1338	1352	rBV	963560	1648053	18.83%	1.461%
15	12.375	1571	1579	1587	rBV	45528	81358	0.93%	0.072%
16	13.469	1759	1765	1771	rVV2	42595	68351	0.78%	0.061%
17	13.587	1778	1785	1790	rBV6	7327	15395	0.18%	0.014%
18	14.040	1855	1862	1871	rBV	4738355	6101491	69.70%	5.410%
19	14.328	1903	1911	1924	rBV	5208386	7514507	85.84%	6.663%
20	14.628	1954	1962	1972	rBV	4212604	5945228	67.91%	5.271%
21	14.745	1979	1982	1988	rBV8	5676	10737	0.12%	0.010%
22	14.839	1991	1998	2016	rBV	1891300	2919721	33.35%	2.589%
23	15.622	2123	2131	2140	rBV	6510310	8754410	100.00%	7.762%
24	15.745	2146	2152	2167	rBV	1939496	2458962	28.09%	2.180%
25	15.857	2167	2171	2176	rVB2	25968	38082	0.44%	0.034%
26	16.404	2262	2264	2270	rVB7	7481	9931	0.11%	0.009%
27	17.057	2371	2375	2378	rBV6	8974	11351	0.13%	0.010%
28	17.175	2393	2395	2403	rVB7	10372	16471	0.19%	0.015%
29	17.392	2425	2432	2442	rBV	4465667	5987066	68.39%	5.308%
30	17.492	2442	2449	2467	rVV	6409602	8585047	98.07%	7.612%
31	18.022	2534	2539	2543	rBV8	15873	24477	0.28%	0.022%
32	18.228	2571	2574	2578	rBV5	22709	33944	0.39%	0.030%
33	19.298	2752	2756	2761	rBV3	56631	74563	0.85%	0.066%
34	19.369	2764	2768	2773	rVB	53230	72156	0.82%	0.064%
35	19.604	2806	2808	2813	rBV5	17449	19411	0.22%	0.017%
36	19.727	2823	2829	2836	rBV	6663755	8234497	94.06%	7.301%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017063.D
Acq On : 09 Sep 2023 22:05
Operator : MA/JU
Sample : PB155238BL
Misc :
ALS Vial : 75 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK238

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Title : SVOA CALIBRATION

37	21.486	3123	3128	3138	rBV	3571098	4471418	51.08%	3.964%
38	23.845	3523	3529	3542	rVB2	3400139	6797136	77.64%	6.026%
39	24.015	3551	3558	3571	rVB	2131240	4391043	50.16%	3.893%




Sum of corrected areas: 112787685

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017063.D
Acq On : 09 Sep 2023 22:05
Operator : MA/JU
Sample : PB155238BL
Misc :
ALS Vial : 75 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK238

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

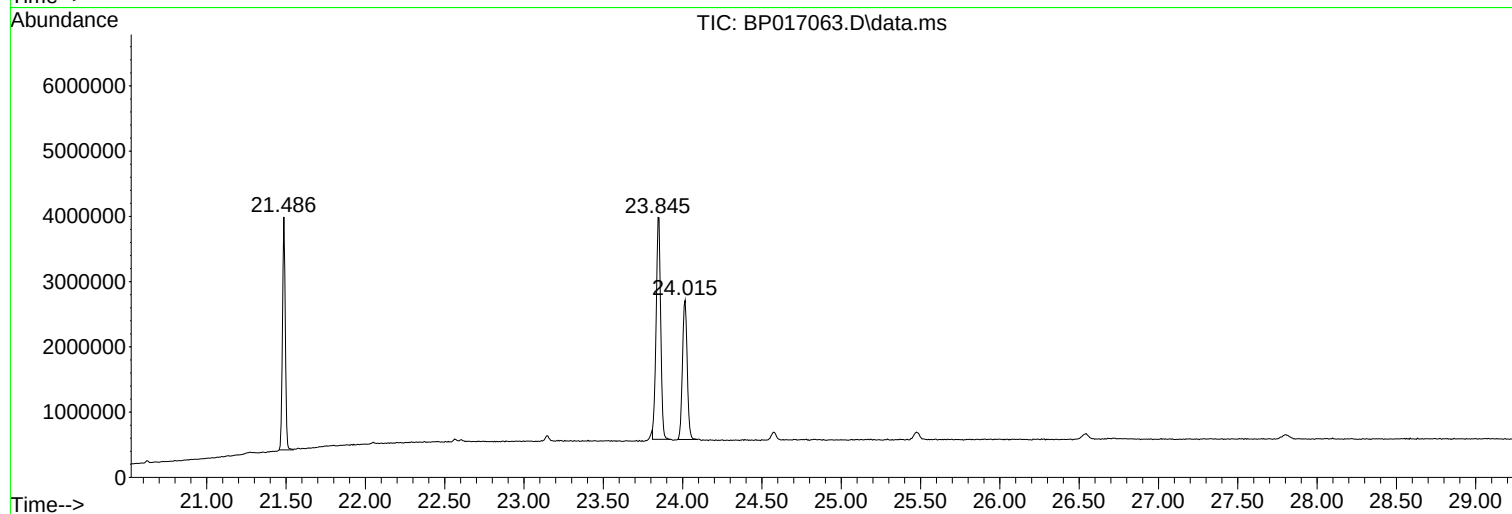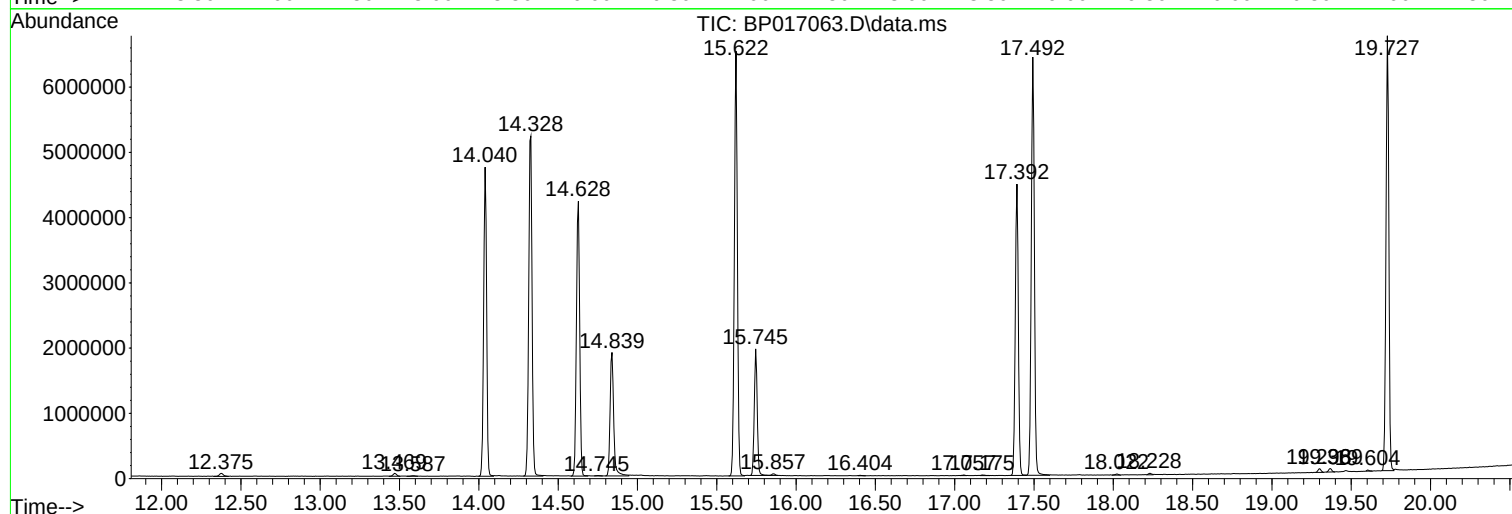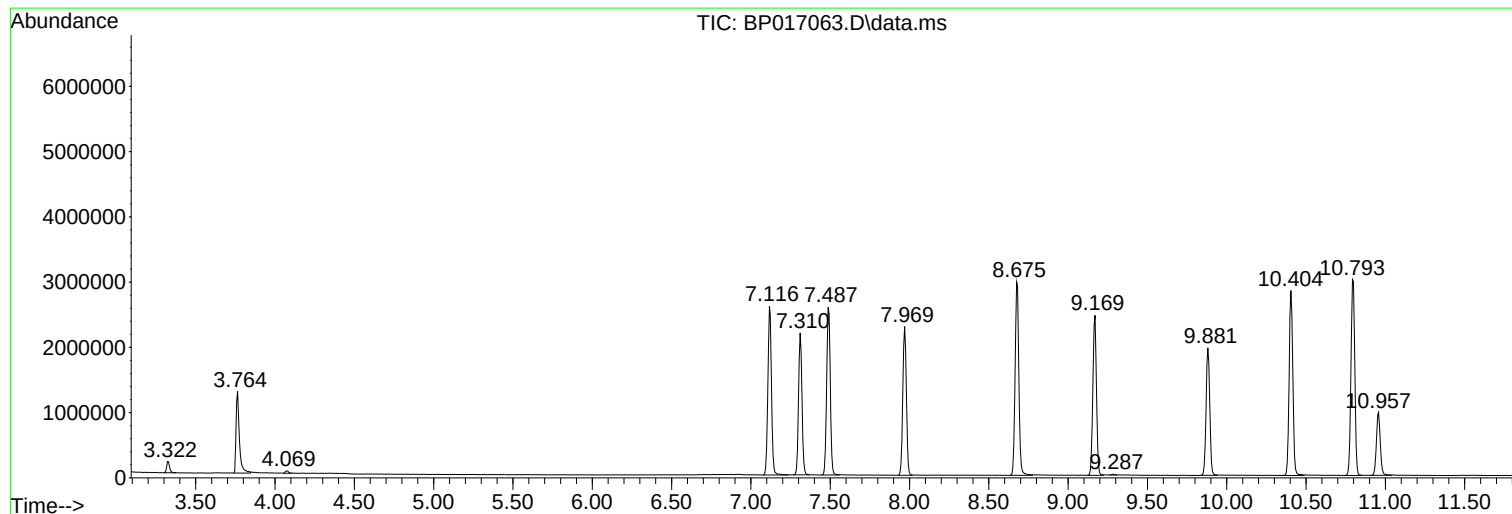

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017063.D
Acq On : 09 Sep 2023 22:05
Operator : MA/JU
Sample : PB155238BL
Misc :
ALS Vial : 75 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK238

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017063.D
Acq On : 09 Sep 2023 22:05
Operator : MA/JU
Sample : PB155238BL
Misc :
ALS Vial : 75 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK238

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc