

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
 Data File : BP017065.D
 Acq On : 09 Sep 2023 23:14
 Operator : MA/JU
 Sample : PB155240BL
 Misc :
 ALS Vial : 77 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK240

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017065.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.322	36	40	50	rBV	313607	419938	1.70%	0.161%
2	3.758	109	114	140	rBV	4576698	7072721	28.65%	2.705%
3	4.069	163	167	177	rVB	45767	70421	0.29%	0.027%
4	7.122	678	686	707	rBV	5409220	8439325	34.18%	3.228%
5	7.316	711	719	728	rVB	4112703	6420535	26.00%	2.456%
6	7.493	741	749	762	rBV	5114388	8023854	32.50%	3.069%
7	7.969	823	830	841	rBV	3166408	4849893	19.64%	1.855%
8	8.681	943	951	968	rBV	6260346	9961186	40.34%	3.810%
9	9.169	1025	1034	1049	rBV	4941487	7979617	32.32%	3.052%
10	9.881	1148	1155	1165	rBV	4094089	6716452	27.20%	2.569%
11	10.404	1236	1244	1259	rBV	5855337	9728324	39.40%	3.721%
12	10.798	1300	1311	1320	rBV	4392543	7228673	29.28%	2.765%
13	10.957	1329	1338	1351	rBV	6019808	10072393	40.79%	3.852%
14	12.310	1562	1568	1573	rBV	33814	53333	0.22%	0.020%
15	12.375	1574	1579	1587	rVB2	100881	160554	0.65%	0.061%
16	13.469	1759	1765	1771	rBV	66794	110206	0.45%	0.042%
17	13.587	1781	1785	1790	rVB2	17965	25271	0.10%	0.010%
18	14.045	1855	1863	1873	rBV	10287685	13891510	56.26%	5.313%
19	14.328	1903	1911	1924	rBV2	11655766	16894097	68.42%	6.461%
20	14.628	1955	1962	1970	rBV	6560368	9309681	37.71%	3.561%
21	14.745	1977	1982	1987	rBV8	13916	26491	0.11%	0.010%
22	14.845	1990	1999	2016	rBV	5296132	7749993	31.39%	2.964%
23	15.622	2124	2131	2139	rBV	14307319	20474483	82.92%	7.831%
24	15.751	2146	2153	2167	rBV	4921182	6517850	26.40%	2.493%
25	15.857	2167	2171	2182	rVB	62410	98266	0.40%	0.038%
26	16.404	2259	2264	2273	rBV5	14857	27507	0.11%	0.011%
27	17.057	2371	2375	2383	rVB2	19782	30618	0.12%	0.012%
28	17.392	2425	2432	2442	rBV	8074302	10919440	44.22%	4.176%
29	17.498	2443	2450	2466	rVV	16354491	22328459	90.43%	8.540%
30	18.233	2571	2575	2581	rBV6	19653	35215	0.14%	0.013%
31	19.298	2752	2756	2761	rBV	162583	222860	0.90%	0.085%
32	19.369	2763	2768	2773	rVV	165819	215842	0.87%	0.083%
33	19.604	2805	2808	2813	rBV5	29460	38367	0.16%	0.015%
34	19.733	2823	2830	2844	rBV	19229708	24690733	100.00%	9.443%
35	21.492	3123	3129	3140	rBV	8049227	10042233	40.67%	3.841%
36	23.862	3520	3532	3546	rVB2	10285813	21135009	85.60%	8.083%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017065.D
Acq On : 09 Sep 2023 23:14
Operator : MA/JU
Sample : PB155240BL
Misc :
ALS Vial : 77 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK240

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Title : SVOA CALIBRATION

37	24.021	3551	3559	3571	rVV	4358607	8897079	36.03%	3.403%
38	24.580	3650	3654	3662	rVB2	305517	592175	2.40%	0.226%




Sum of corrected areas: 261470604

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017065.D
Acq On : 09 Sep 2023 23:14
Operator : MA/JU
Sample : PB155240BL
Misc :
ALS Vial : 77 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK240

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

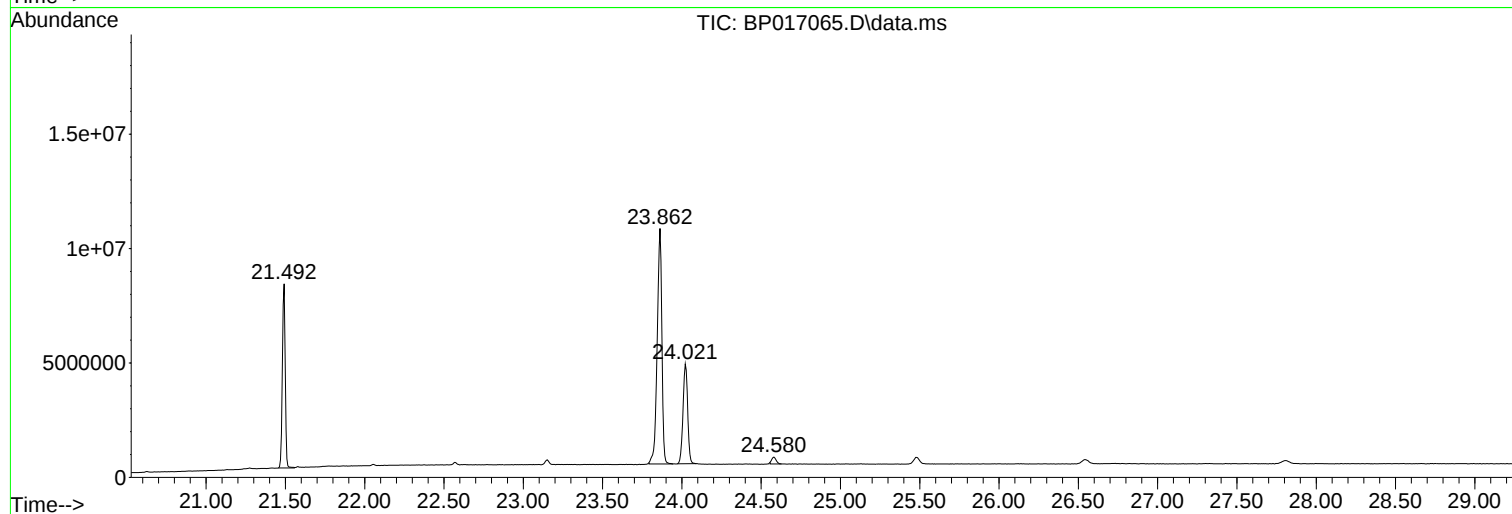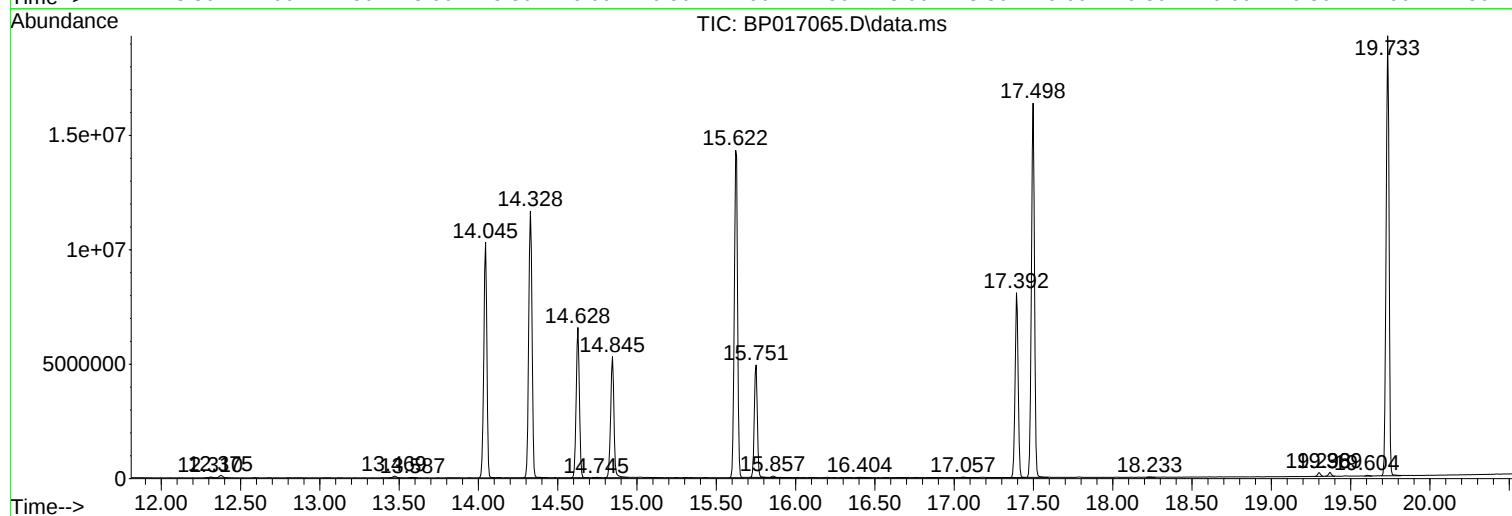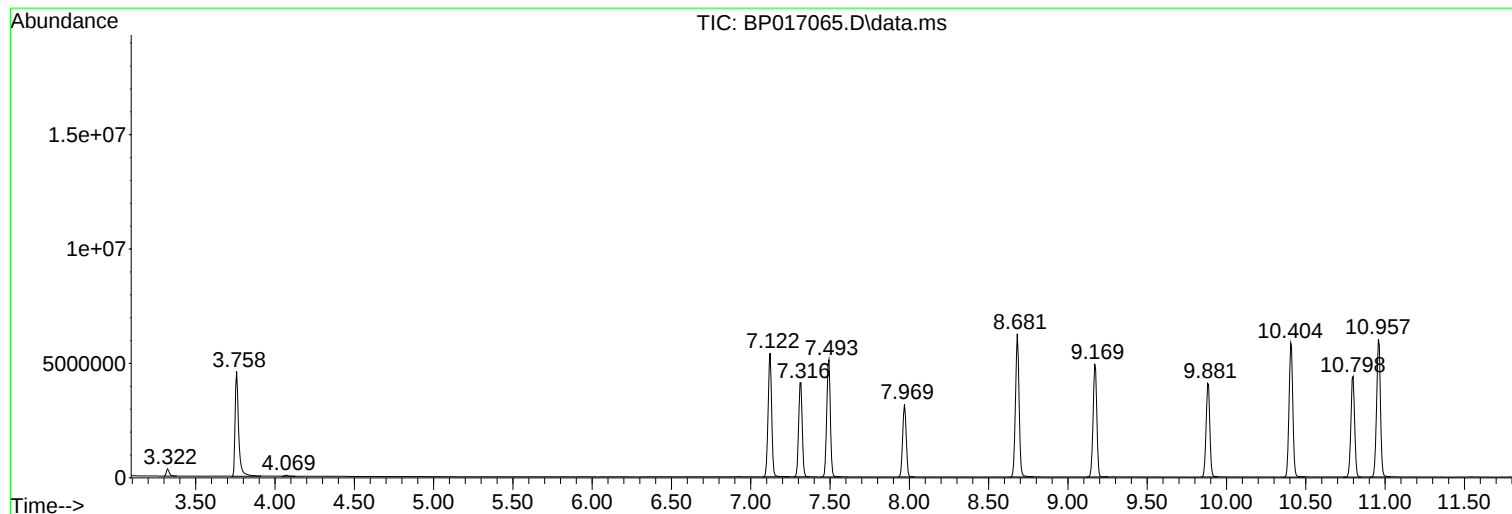

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017065.D
Acq On : 09 Sep 2023 23:14
Operator : MA/JU
Sample : PB155240BL
Misc :
ALS Vial : 77 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK240

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017065.D
Acq On : 09 Sep 2023 23:14
Operator : MA/JU
Sample : PB155240BL
Misc :
ALS Vial : 77 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK240

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------