

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
 Data File : BP017066.D
 Acq On : 09 Sep 2023 23:49
 Operator : MA/JU
 Sample : 04123-12
 Misc :
 ALS Vial : 78 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH8W9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017066.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	28	32	37	rBV	103257	153952	0.73%	0.110%
2	3.323	37	40	50	rVB	132105	187499	0.89%	0.134%
3	3.764	111	115	132	rBV	763075	1264207	6.03%	0.901%
4	3.958	143	148	156	rVB	62215	102481	0.49%	0.073%
5	4.070	162	167	182	rVB	141524	231795	1.11%	0.165%
6	4.458	232	233	240	rVB2	20945	24285	0.12%	0.017%
7	4.599	250	257	273	rBV	13614642	20950051	100.00%	14.937%
8	5.011	322	327	334	rBV	21977	35365	0.17%	0.025%
9	6.487	572	578	589	rVB	499724	753020	3.59%	0.537%
10	6.916	647	651	662	rVB	17869	45781	0.22%	0.033%
11	7.116	678	685	698	rBV	664202	1034509	4.94%	0.738%
12	7.311	710	718	730	rBV	2057383	3097049	14.78%	2.208%
13	7.487	741	748	760	rBV	2003340	3125478	14.92%	2.228%
14	7.969	821	830	844	rBV	1756403	2741225	13.08%	1.954%
15	8.675	943	950	961	rBV	1716079	2718188	12.97%	1.938%
16	9.169	1023	1034	1046	rBV	2408561	3844304	18.35%	2.741%
17	9.881	1147	1155	1169	rBV	1930196	3061629	14.61%	2.183%
18	10.405	1235	1244	1262	rBV	2775281	4483283	21.40%	3.196%
19	10.793	1301	1310	1322	rBV	2487066	4111376	19.62%	2.931%
20	10.957	1330	1338	1357	rBV	2185030	3639216	17.37%	2.595%
21	12.375	1575	1579	1584	rBV2	43148	64799	0.31%	0.046%
22	13.469	1760	1765	1772	rBV	25425	40261	0.19%	0.029%
23	14.040	1854	1862	1874	rBV	5125513	6728594	32.12%	4.797%
24	14.328	1903	1911	1926	rBV	5601287	8134587	38.83%	5.800%
25	14.622	1955	1961	1972	rBV	3537615	5275567	25.18%	3.761%
26	14.840	1992	1998	2015	rBV	444907	754307	3.60%	0.538%
27	15.016	2022	2028	2033	rVV9	11461	25069	0.12%	0.018%
28	15.622	2124	2131	2137	rBV	7430387	10084654	48.14%	7.190%
29	15.687	2137	2142	2146	rVV	163216	248970	1.19%	0.178%
30	15.745	2146	2152	2164	rVV	2350309	3068413	14.65%	2.188%
31	15.857	2167	2171	2176	rVB3	30414	46210	0.22%	0.033%
32	17.392	2426	2432	2442	rBV	4508993	6127550	29.25%	4.369%
33	17.492	2443	2449	2466	rVV2	7820569	10787679	51.49%	7.691%
34	18.016	2534	2538	2545	rBV7	18464	40079	0.19%	0.029%
35	18.234	2571	2575	2581	rBV	166164	249328	1.19%	0.178%
36	19.304	2753	2757	2761	rBV2	82650	103122	0.49%	0.074%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017066.D
Acq On : 09 Sep 2023 23:49
Operator : MA/JU
Sample : 04123-12
Misc :
ALS Vial : 78 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH8W9

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Title : SVOA CALIBRATION

37	19.369	2764	2768	2772	rVB	83730	108369	0.52%	0.077%
38	19.469	2781	2785	2794	rBV2	116996	178866	0.85%	0.128%
39	19.733	2823	2830	2835	rBV	9013385	11804011	56.34%	8.416%
40	20.033	2877	2881	2885	rBV2	157755	195338	0.93%	0.139%
41	21.486	3123	3128	3138	rBV	4117867	5554306	26.51%	3.960%
42	23.857	3520	3531	3550	rVB2	4767002	9957619	47.53%	7.099%
43	24.021	3552	3559	3574	rVB	2512377	5076197	24.23%	3.619%




Sum of corrected areas: 140258588

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017066.D
Acq On : 09 Sep 2023 23:49
Operator : MA/JU
Sample : 04123-12
Misc :
ALS Vial : 78 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH8W9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

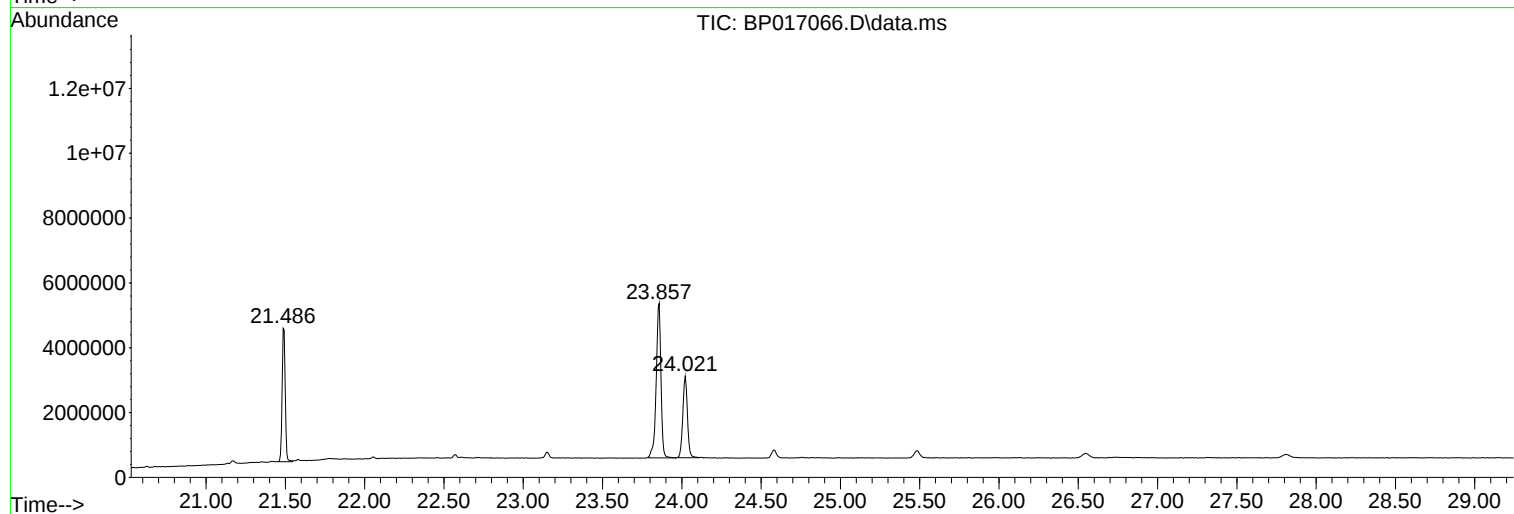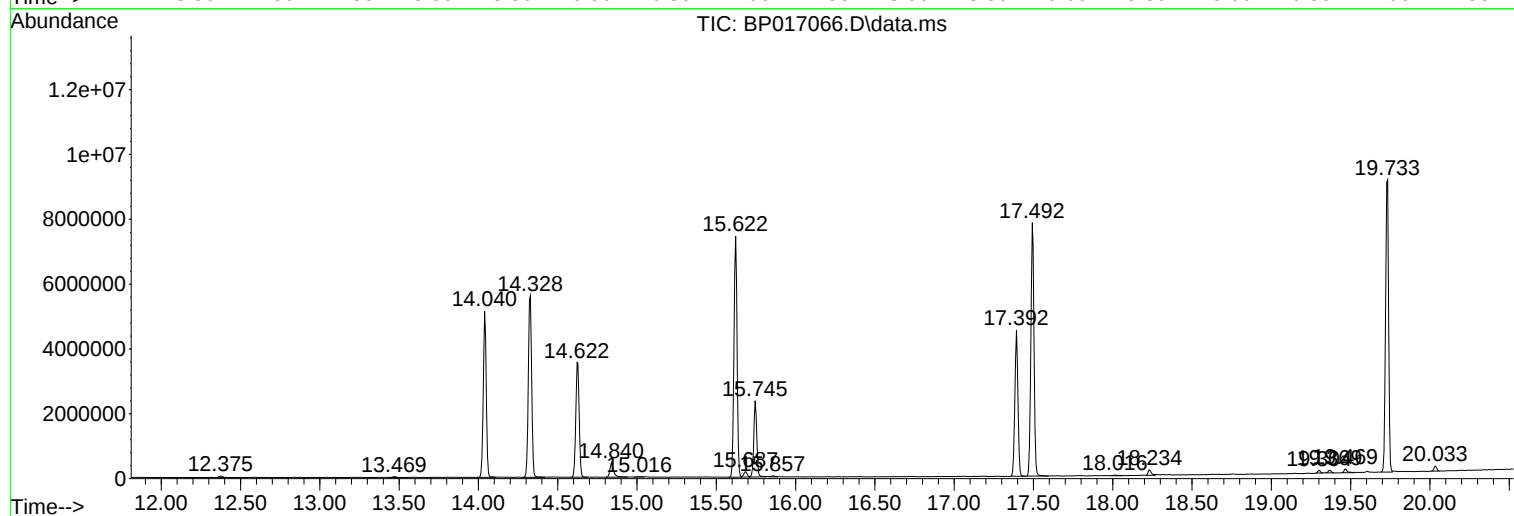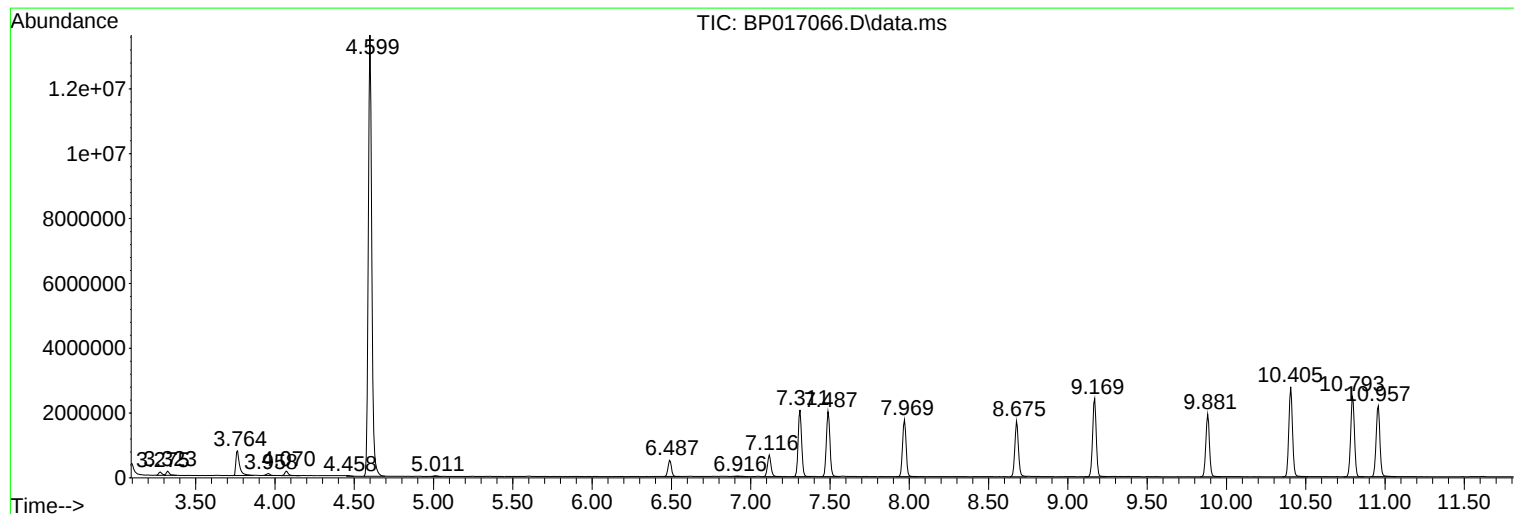

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017066.D
Acq On : 09 Sep 2023 23:49
Operator : MA/JU
Sample : 04123-12
Misc :
ALS Vial : 78 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH8W9










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.599	152.85 ng/ul	20950100	1,4-Dichlorobenzene-d4	7.969

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	99
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	99
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	93
5			Pyrimidine, 5-fluoro-2,4-dichloro-	166	C4HC12FN2	002927-71-1	35

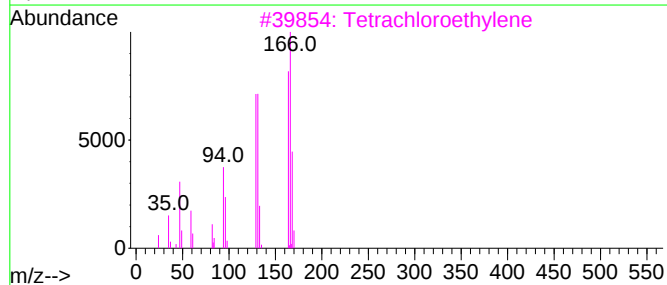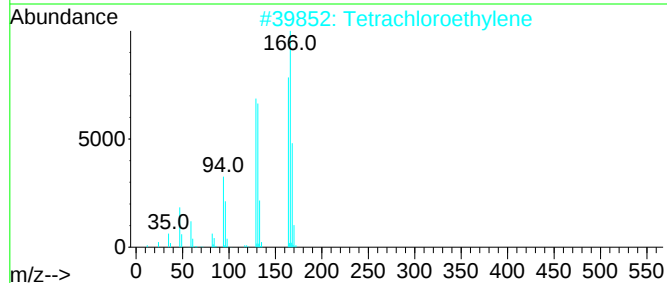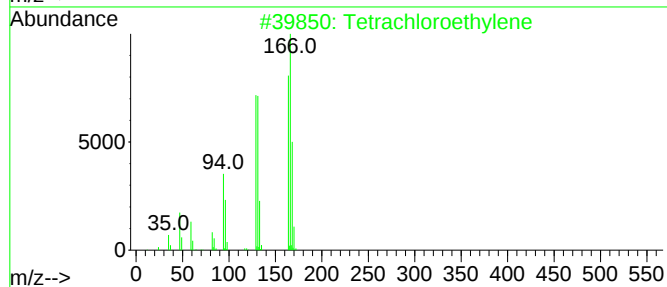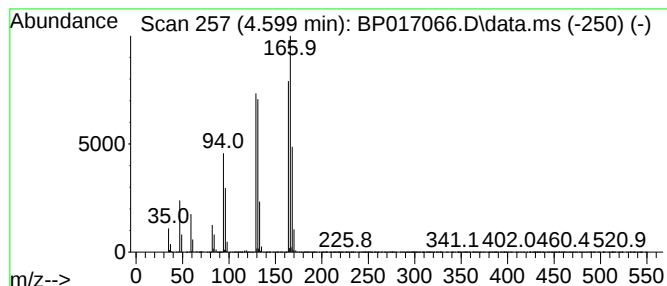

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017066.D
Acq On : 09 Sep 2023 23:49
Operator : MA/JU
Sample : 04123-12
Misc :
ALS Vial : 78 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH8W9










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Propane, 1,2,3-trichloro- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.487	5.49 ng/ul	753020	1,4-Dichlorobenzene-d4	7.969

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Propane, 1,2,3-trichloro-	146	C3H5Cl3	000096-18-4	91
2			Propane, 1,2,3-trichloro-	146	C3H5Cl3	000096-18-4	91
3			Propane, 1,2,3-trichloro-	146	C3H5Cl3	000096-18-4	91
4			1-Propene, 1,3-dichloro-, (E)-	110	C3H4Cl2	010061-02-6	86
5			1-Propene, 1,3-dichloro-, (Z)-	110	C3H4Cl2	010061-01-5	86

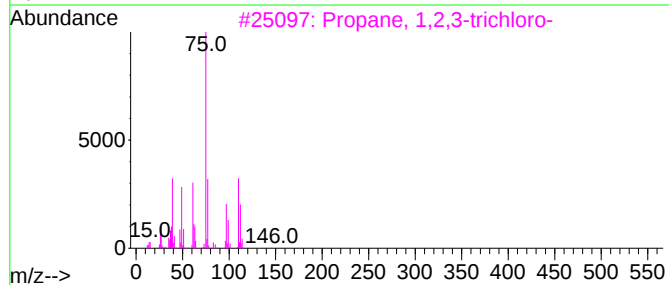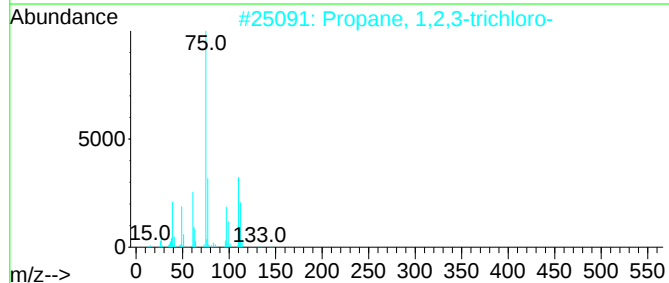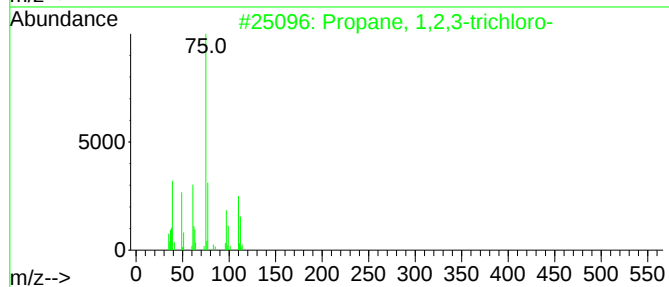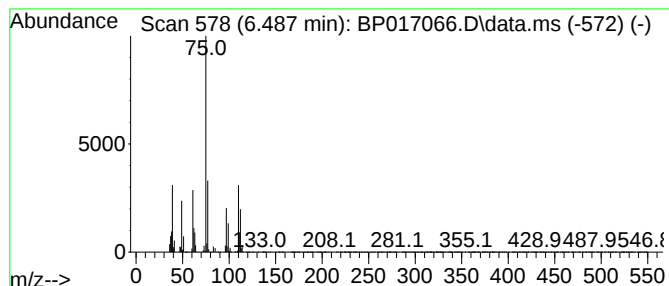

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017066.D
Acq On : 09 Sep 2023 23:49
Operator : MA/JU
Sample : 04123-12
Misc :
ALS Vial : 78 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH8W9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.599	152.8	ng/ul	20950100	1	7.969	2741230	20.0
Propane, 1,2,3-...	6.487	5.5	ng/ul	753020	1	7.969	2741230	20.0