

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
 Data File : BP017078.D
 Acq On : 10 Sep 2023 07:51
 Operator : MA/JU
 Sample : PB155347BL
 Misc :
 ALS Vial : 91 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK347

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017078.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.323	36	40	49	rBV	129191	165395	2.19%	0.170%
2	3.758	111	114	133	rBV	1649607	2512532	33.26%	2.586%
3	4.070	164	167	174	rVB	25218	37563	0.50%	0.039%
4	7.117	678	685	704	rVB	1916547	3012609	39.88%	3.101%
5	7.311	710	718	727	rBV	1542724	2361135	31.25%	2.430%
6	7.487	741	748	761	rBV	1909244	2915006	38.59%	3.001%
7	7.969	822	830	837	rBV	1745441	2754675	36.46%	2.836%
8	8.675	943	950	963	rBV	2232719	3590926	47.53%	3.696%
9	9.163	1025	1033	1049	rBV	1783949	2871774	38.01%	2.956%
10	9.881	1145	1155	1168	rBV	1461308	2369356	31.36%	2.439%
11	10.405	1236	1244	1261	rBV	2171988	3531848	46.75%	3.636%
12	10.793	1302	1310	1321	rBV	2591522	4139811	54.80%	4.261%
13	10.952	1327	1337	1354	rBV	2149840	3693326	48.89%	3.802%
14	11.481	1423	1427	1431	rBV6	6520	11373	0.15%	0.012%
15	12.375	1572	1579	1585	rBV2	35364	56070	0.74%	0.058%
16	12.581	1610	1614	1620	rBV9	4680	9818	0.13%	0.010%
17	13.469	1759	1765	1772	rBV	50592	78303	1.04%	0.081%
18	13.587	1781	1785	1790	rVB8	6553	10254	0.14%	0.011%
19	14.040	1855	1862	1870	rBV	3711229	4960090	65.66%	5.106%
20	14.322	1903	1910	1925	rBV2	4192155	5876004	77.78%	6.049%
21	14.622	1955	1961	1972	rBV	3662273	5313461	70.34%	5.470%
22	14.840	1992	1998	2020	rBV	1360637	2199671	29.12%	2.264%
23	15.293	2071	2075	2079	rBV7	5729	8795	0.12%	0.009%
24	15.622	2124	2131	2143	rBV	5126172	7182835	95.08%	7.394%
25	15.745	2146	2152	2166	rVV	1221231	1582252	20.94%	1.629%
26	15.857	2166	2171	2175	rVV	20085	29923	0.40%	0.031%
27	17.063	2367	2376	2381	rBV	9855	22638	0.30%	0.023%
28	17.181	2392	2396	2400	rBV4	7690	10825	0.14%	0.011%
29	17.392	2425	2432	2442	rBV	4368248	5921747	78.39%	6.096%
30	17.492	2442	2449	2463	rVV	5368814	7297455	96.60%	7.512%
31	19.298	2753	2756	2761	rVB2	53107	64037	0.85%	0.066%
32	19.369	2764	2768	2773	rVV2	57503	76652	1.01%	0.079%
33	19.604	2805	2808	2812	rBV	44325	46323	0.61%	0.048%
34	19.728	2823	2829	2836	rBV	6050391	7554453	100.00%	7.776%
35	21.486	3123	3128	3135	rBV	3751209	4686022	62.03%	4.824%
36	23.851	3523	3530	3540	rVB	2860177	5858448	77.55%	6.031%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017078.D
Acq On : 10 Sep 2023 07:51
Operator : MA/JU
Sample : PB155347BL
Misc :
ALS Vial : 91 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK347

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Title : SVOA CALIBRATION

37	24.016	3552	3558	3573	rVB	2092366	4333228	57.36%	4.461%
----	--------	------	------	------	-----	---------	---------	--------	--------




Sum of corrected areas: 97146633

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017078.D
Acq On : 10 Sep 2023 07:51
Operator : MA/JU
Sample : PB155347BL
Misc :
ALS Vial : 91 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK347

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

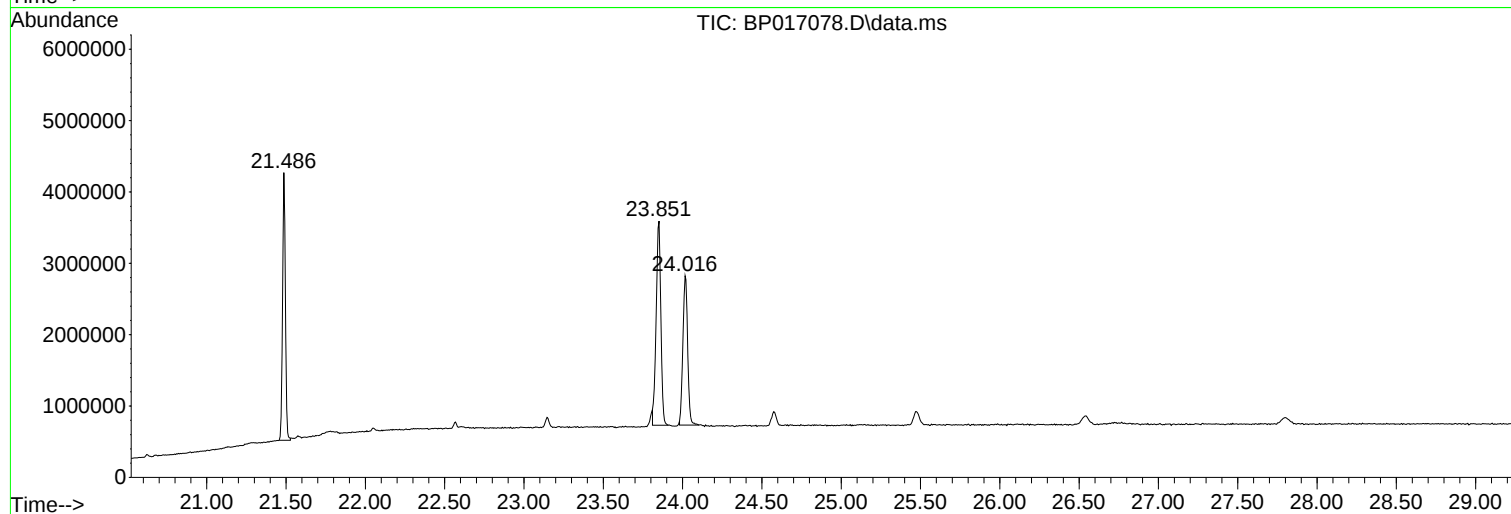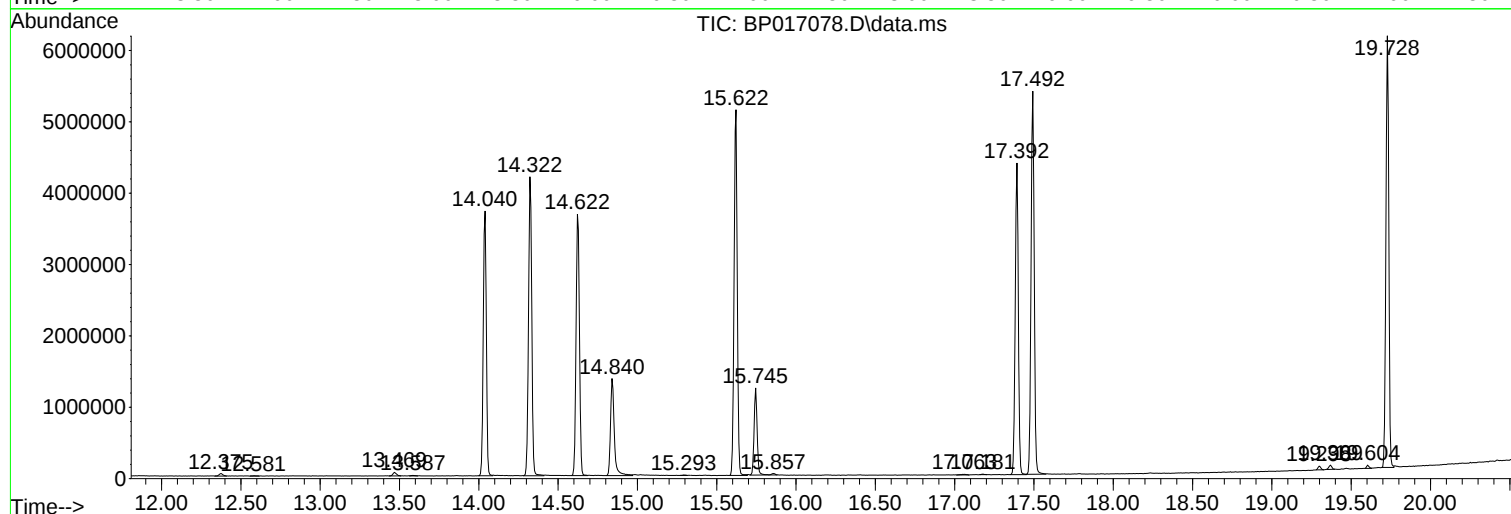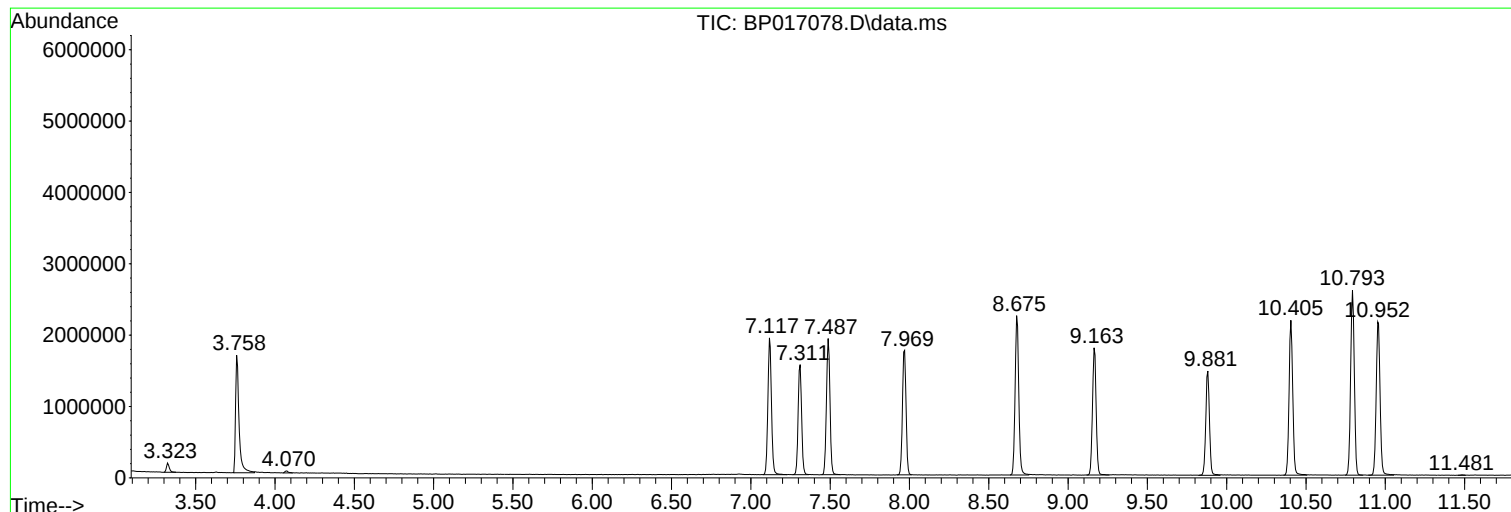

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017078.D
Acq On : 10 Sep 2023 07:51
Operator : MA/JU
Sample : PB155347BL
Misc :
ALS Vial : 91 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK347

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017078.D
Acq On : 10 Sep 2023 07:51
Operator : MA/JU
Sample : PB155347BL
Misc :
ALS Vial : 91 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK347

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc